


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102620\
Data File : VX019122.D
Acq On : 26 Oct 2020 16:34
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102620W.M
Title : SW846 8260
Last Update : Tue Oct 27 05:47:59 2020

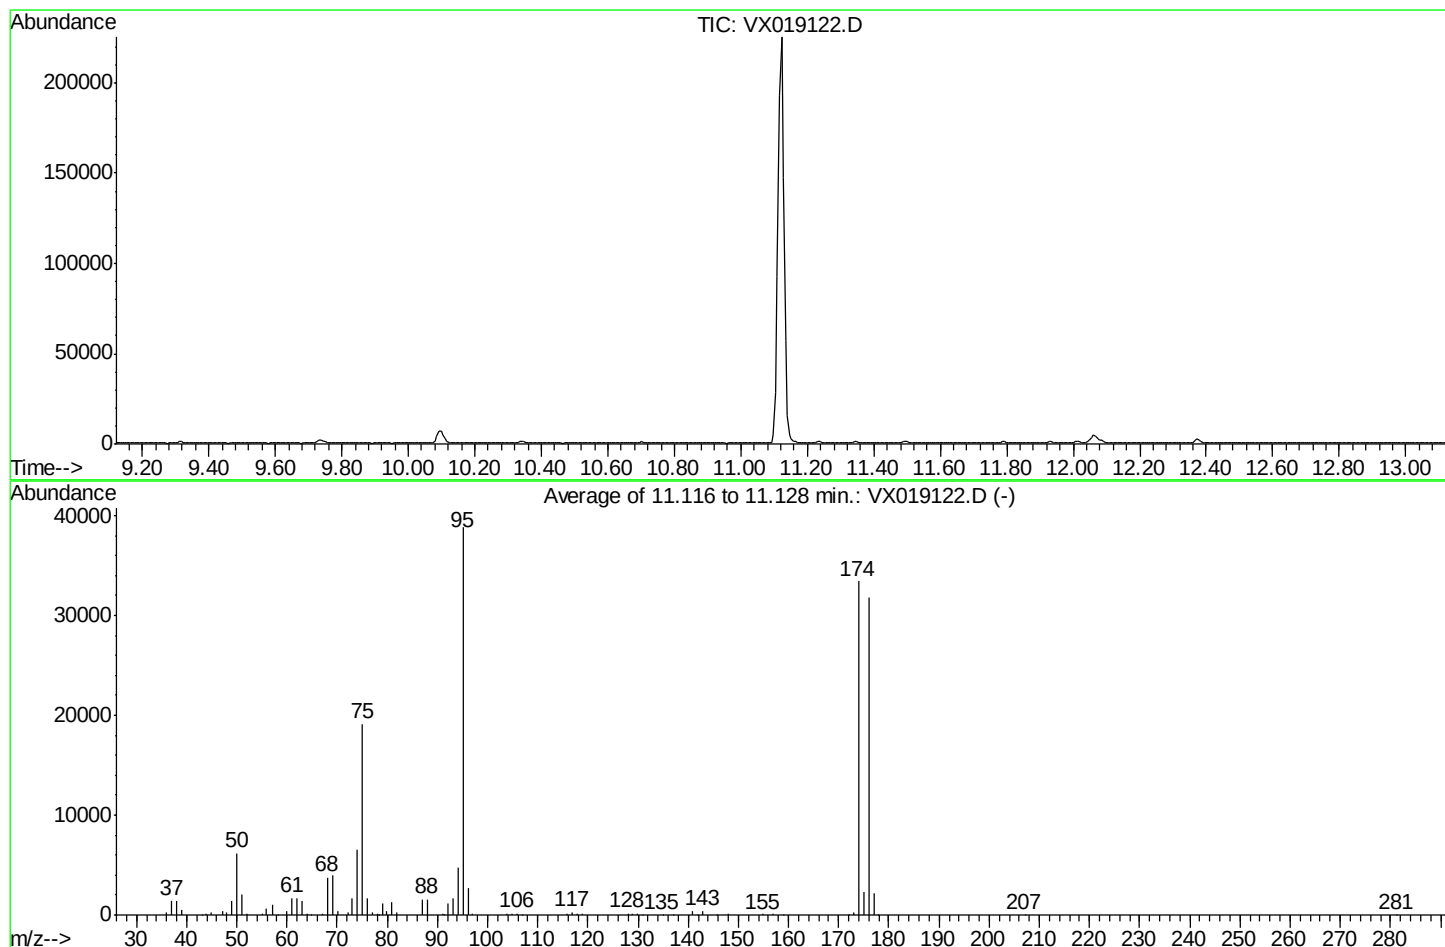

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	6214	PASS
75	95	30	60	49.3	19126	PASS
95	95	100	100	100.0	38818	PASS
96	95	5	9	6.8	2639	PASS
173	174	0.00	2	0.6	202	PASS
174	95	50	100	86.0	33397	PASS
175	174	5	9	7.0	2339	PASS
176	174	95	101	95.3	31824	PASS
177	176	5	9	6.7	2143	PASS