

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024947.D
 Acq On : 26 Oct 2021 15:36
 Operator : JC/MD
 Sample : M4304-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 P069-TW001-01

Quant Time: Oct 27 03:03:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/27/2021 1:36:14 PM

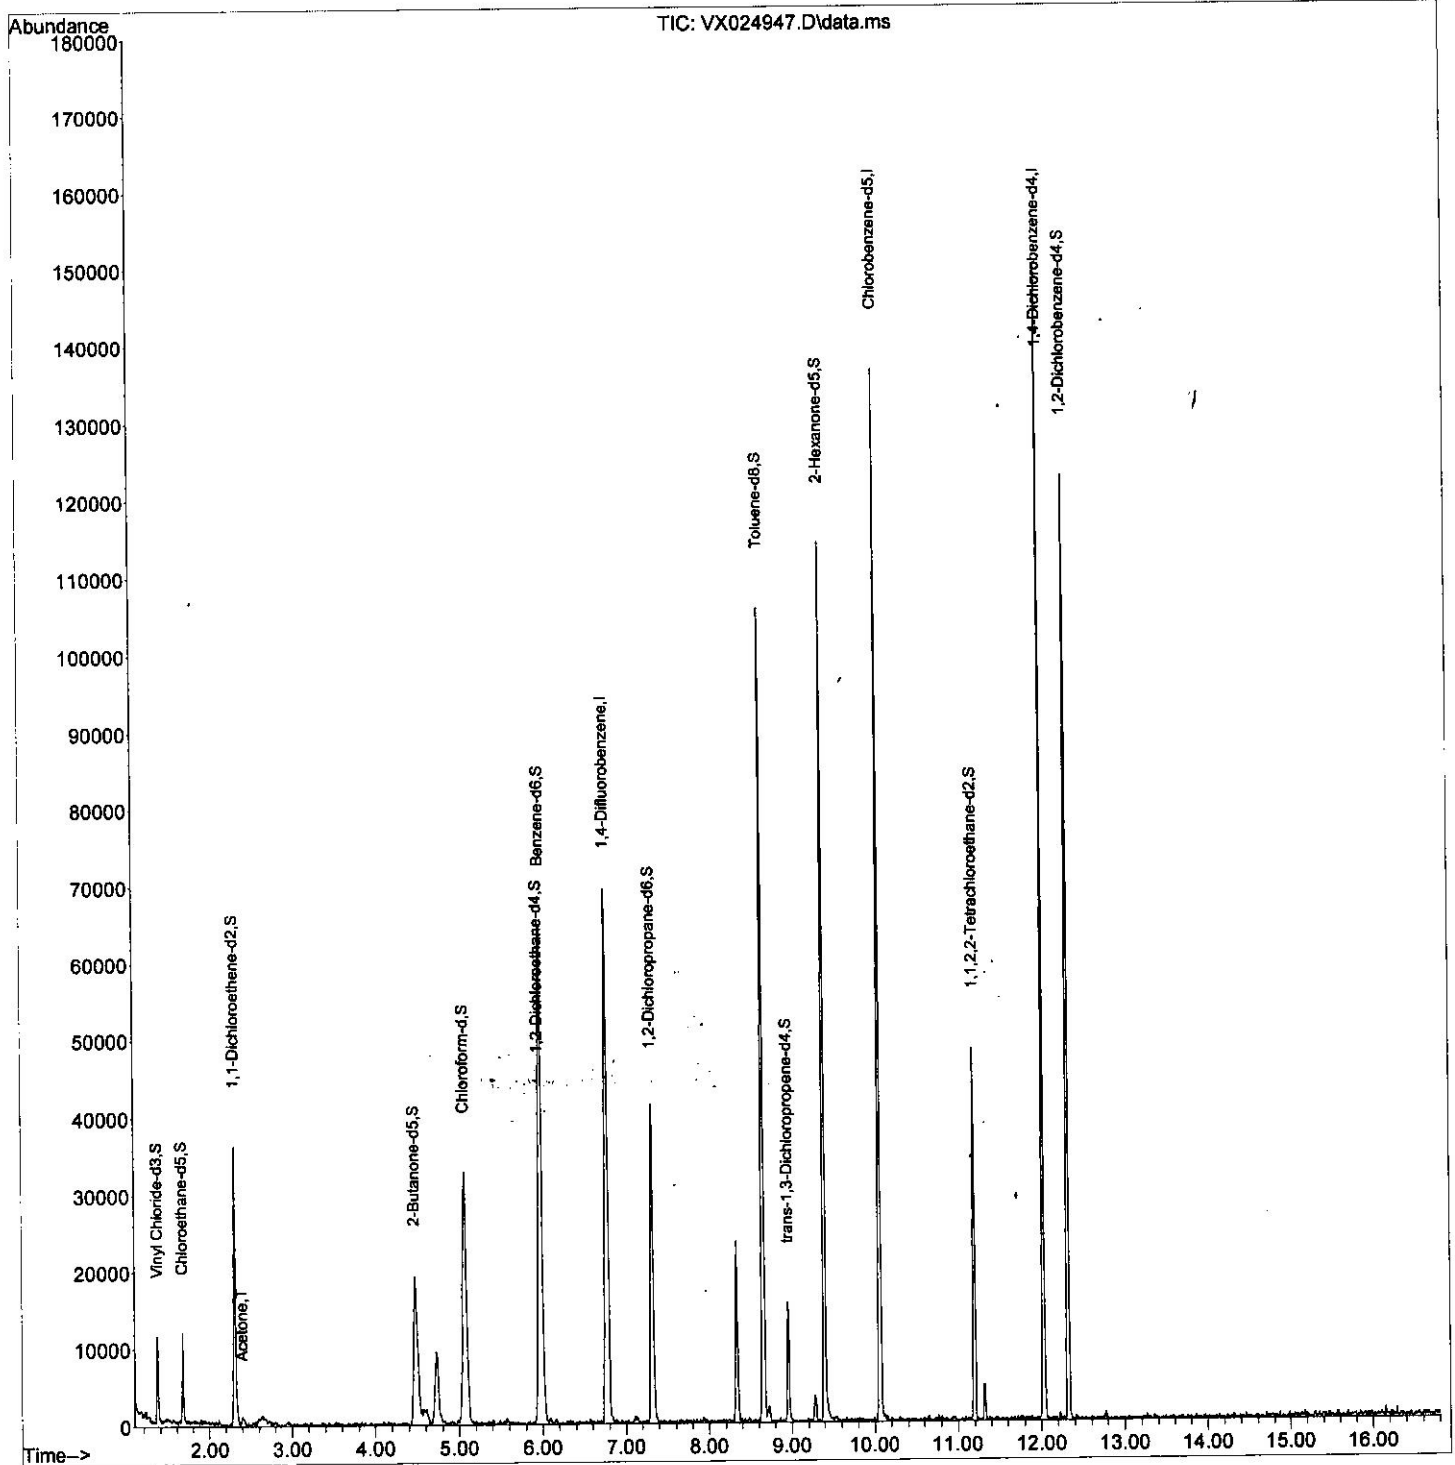

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024947.D
 Acq On : 26 Oct 2021 15:36
 Operator : JC/MD
 Sample : M4304-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P069-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/27/2021 1:36:14 PM

Quant Time: Oct 27 03:03:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

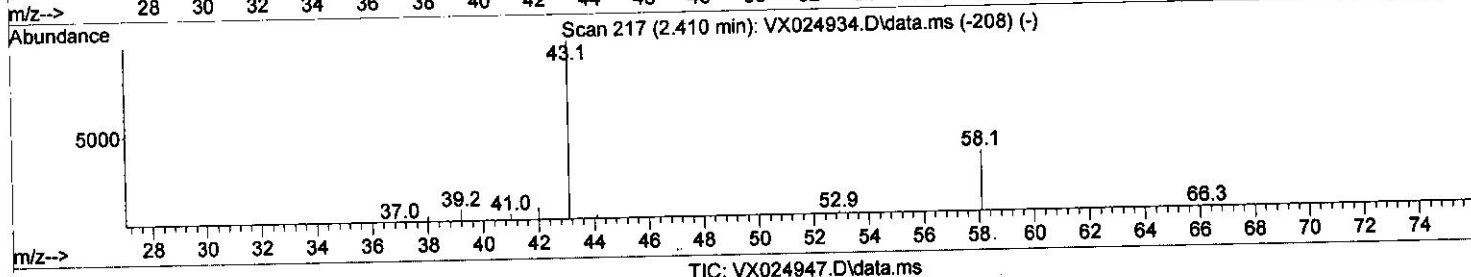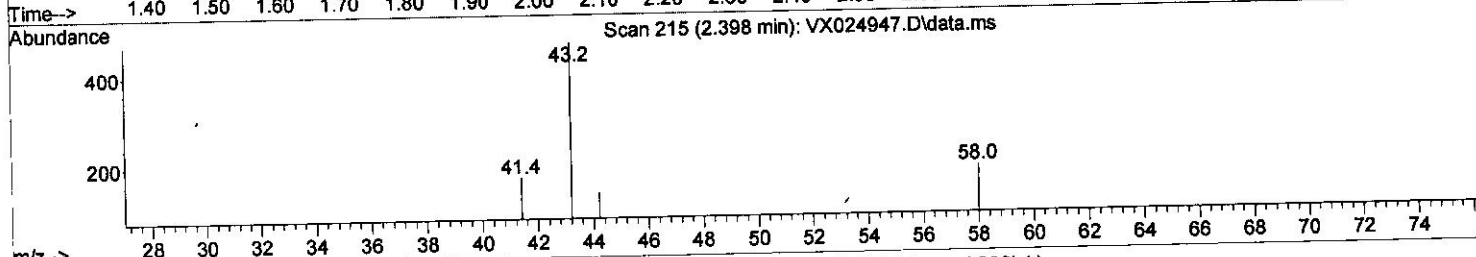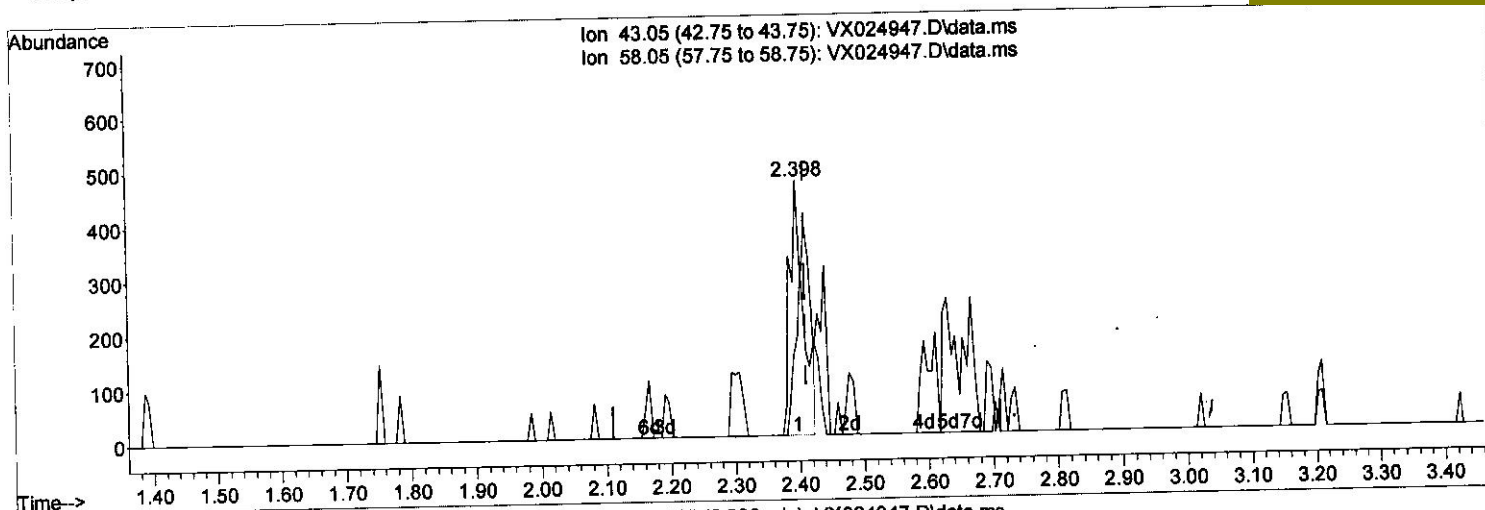

TIC: VX024947.D\data.ms

(13) Acetone (T)

2.398min (-0.012) 1.51 ug/L

response 838

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	58.71
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024947.D
 Acq On : 26 Oct 2021 15:36
 Operator : JC/MD
 Sample : M4304-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 P069-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/27/2021 1:36:14 PM

Quant Time: Oct 27 03:03:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

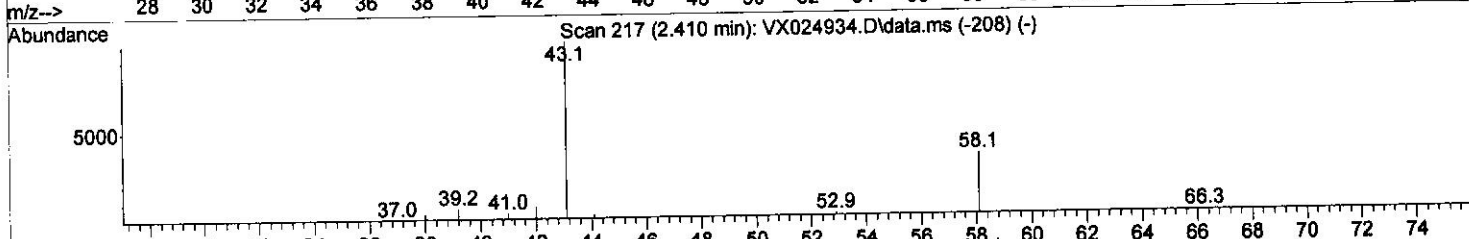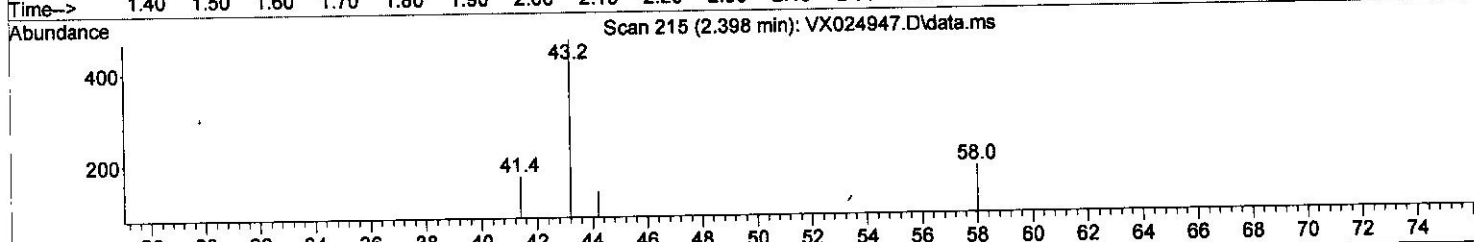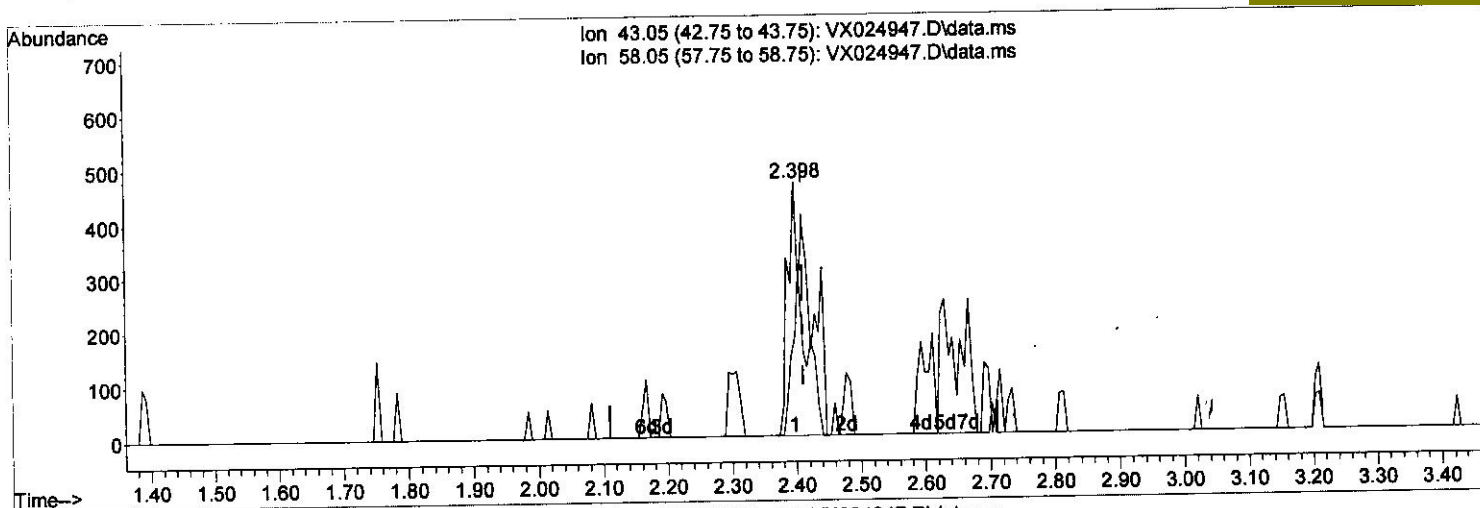

TIC: VX024947.D\data.ms

(13) Acetone (T)

2.398min (-0.012) 1.98 ug/L m

response 1102

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	44.65
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024947.D
 Acq On : 26 Oct 2021 15:36
 Operator : JC/MD
 Sample : M4304-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 P069-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/27/2021 1:36:14 PM

Quant Time: Oct 27 03:03:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	69053	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	62145	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.030	152	28558	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	6556	3.234	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	64.600%		
7) Chloroethane-d5	1.672	69	7245	3.966	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	79.400%		
11) 1,1-Dichloroethene-d2	2.313	63	20667	2.735	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	54.600%#		
20) 2-Butanone-d5	4.471	46	33768	45.560	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	91.120%		
24) Chloroform-d	5.068	84	44656	4.576	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	91.600%		
26) 1,2-Dichloroethane-d4	5.958	65	23101	4.331	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	86.600%		
32) Benzene-d6	5.983	84	65562	4.528	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.600%		
36) 1,2-Dichloropropane-d6	7.312	67	20399	4.416	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.400%		
41) Toluene-d8	8.653	98	62818	4.327	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	86.600%		
43) trans-1,3-Dichloroprop...	8.952	79	8945	4.219	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	84.400%		
46) 2-Hexanone-d5	9.390	63	36128	47.342	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	94.680%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	17265	4.890	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	97.800%		
66) 1,2-Dichlorobenzene-d4	12.323	152	23900	4.966	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	99.400%		
Target Compounds						
13) Acetone	2.398	43	1102m	1.982	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed