

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024935.D
 Acq On : 26 Oct 2021 10:39
 Operator : JC/MD
 Sample : VX1026WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK608

Quant Time: Oct 27 03:01:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	69980	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	66926	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	30975	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	8114	3.949	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.000%	
7) Chloroethane-d5	1.672	69	8519	4.602	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.000%	
11) 1,1-Dichloroethene-d2	2.312	63	24528	3.203	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.000%	
20) 2-Butanone-d5	4.495	46	39612	52.736	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.480%	
24) Chloroform-d	5.068	84	52184	5.276	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.600%	
26) 1,2-Dichloroethane-d4	5.970	65	27014	4.997	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.000%	
32) Benzene-d6	5.976	84	78245	5.018	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.400%	
36) 1,2-Dichloropropane-d6	7.318	67	24725	4.970	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.400%	
41) Toluene-d8	8.653	98	76110	4.868	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.400%	
43) trans-1,3-Dichloroprop...	8.952	79	11109	4.865	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.200%	
46) 2-Hexanone-d5	9.390	63	42245	51.403	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	102.800%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20937	5.506	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	110.200%	
66) 1,2-Dichlorobenzene-d4	12.323	152	27271	5.224	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.788	84	710	0.142	ug/L	# 42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024935.D
Acq On : 26 Oct 2021 10:39
Operator : JC/MD
Sample : VX1026WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK608

Quant Time: Oct 27 03:01:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 27 02:59:04 2021
Response via : Initial Calibration

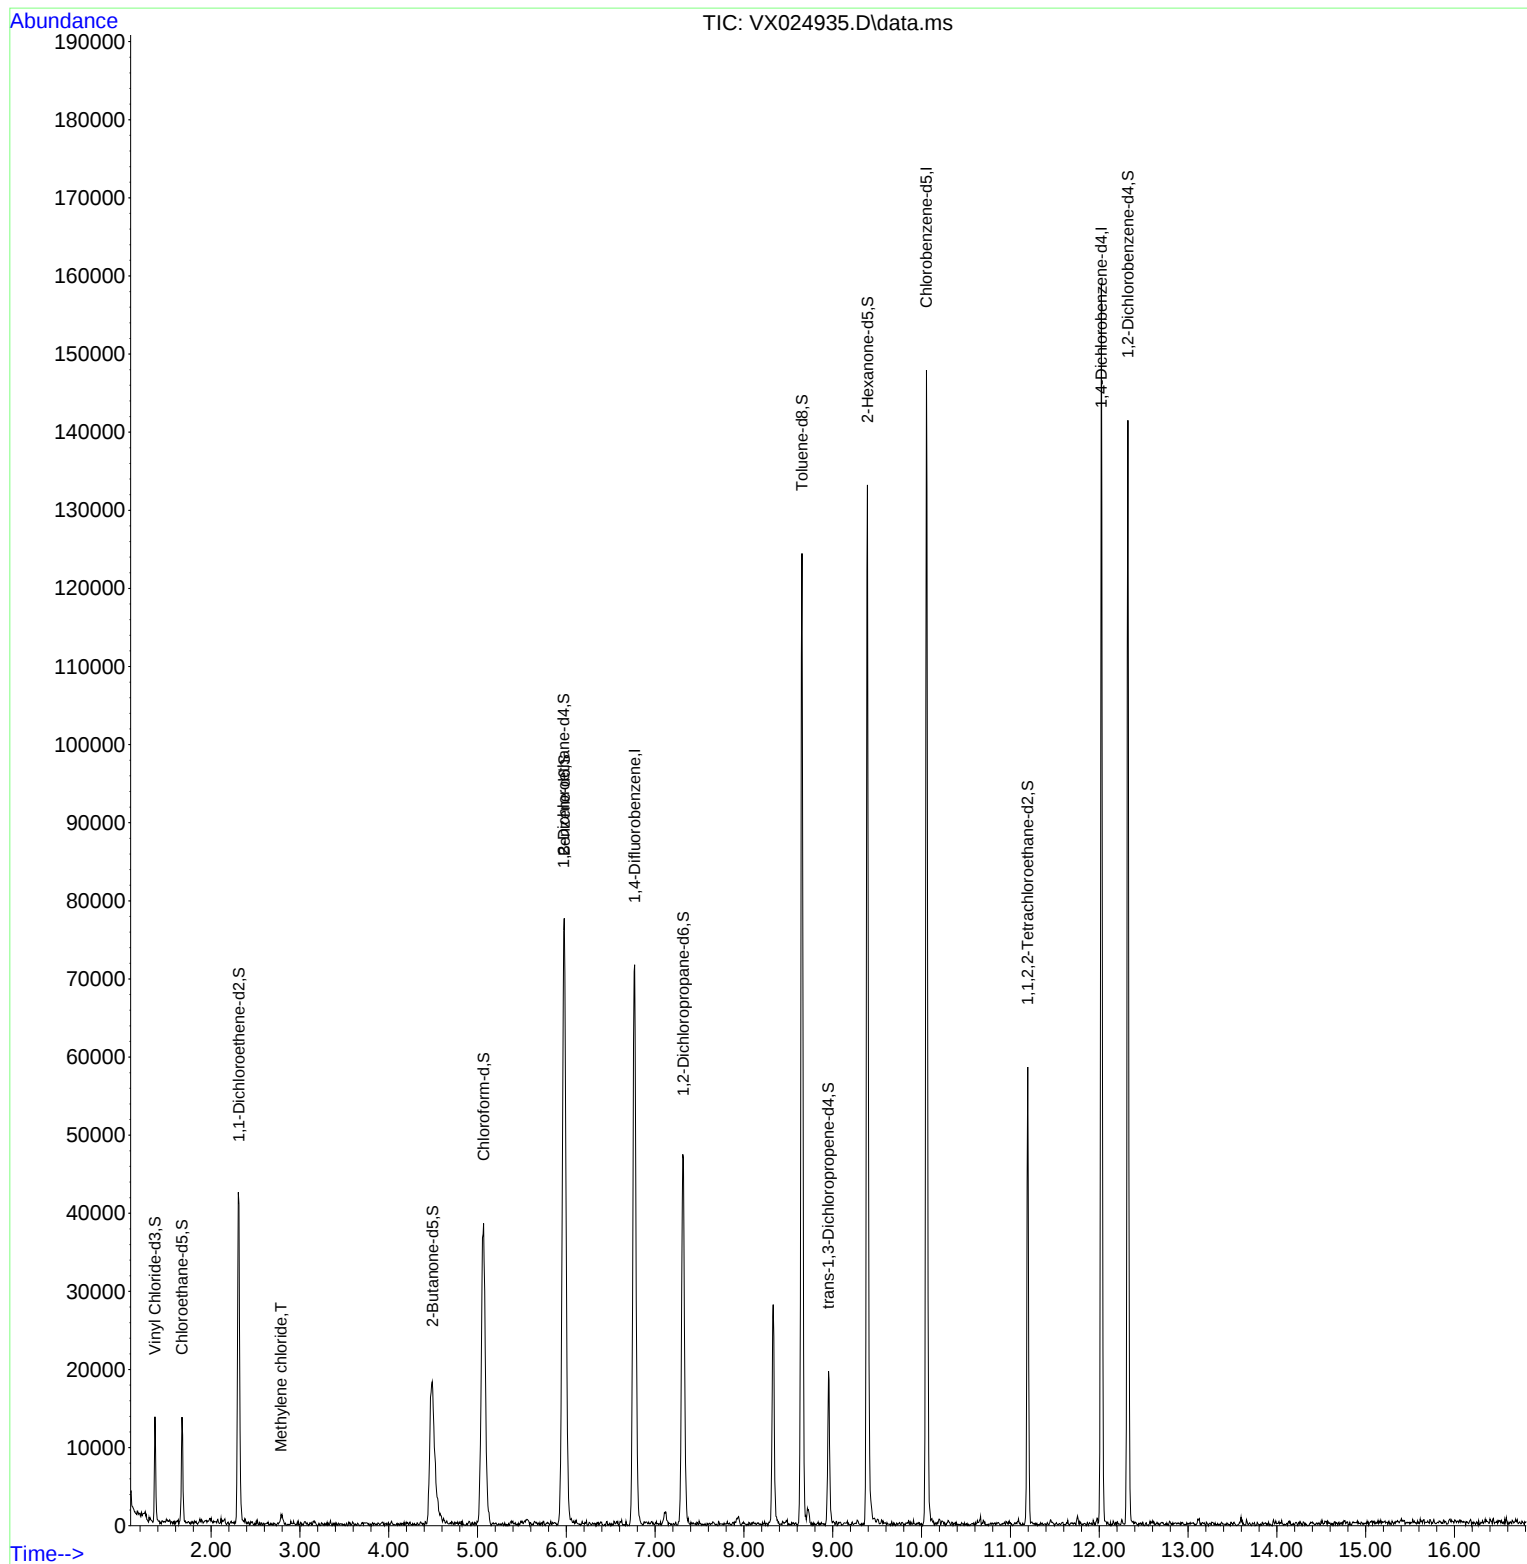

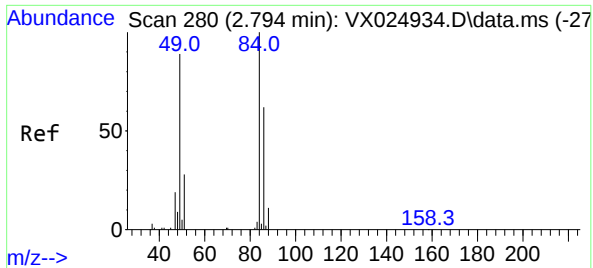

#16
Methylene chloride
Concen: 0.142 ug/L
RT: 2.788 min Scan# 279
Delta R.T. -0.006 min
Lab File: VX024935.D
Acq: 26 Oct 2021 10:39

Instrument :
MSVOA_X
ClientSampleId :
VBLK608

Tgt Ion: 84 Resp: 710

Ion	Ratio	Lower	Upper
84	100		
86	40.6	49.5	91.9#
49	18.9	62.7	116.5#

