

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024940.D
 Acq On : 26 Oct 2021 12:49
 Operator : JC/MD
 Sample : M4304-05
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P063-TW001-01

Quant Time: Oct 27 03:02:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	76271	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	72119	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	7065	3.155	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.200%
7) Chloroethane-d5	1.672	69	7142	3.540	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.800%
11) 1,1-Dichloroethene-d2	2.306	63	20540	2.461	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.200%#
20) 2-Butanone-d5	4.483	46	36111	44.110	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.220%
24) Chloroform-d	5.068	84	44847	4.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
26) 1,2-Dichloroethane-d4	5.970	65	24204	4.108	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
32) Benzene-d6	5.983	84	69009	4.107	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.200%
36) 1,2-Dichloropropane-d6	7.312	67	21645	4.037	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.800%
41) Toluene-d8	8.653	98	64937	3.854	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.000%
43) trans-1,3-Dichloroprop...	8.952	79	9008	3.661	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.200%
46) 2-Hexanone-d5	9.390	63	38429	43.393	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.780%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	18720	4.569	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	12.323	152	24295	4.383	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.600%
Target Compounds					Qvalue	
13) Acetone	2.404	43	1098	1.788	ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024940.D
Acq On : 26 Oct 2021 12:49
Operator : JC/MD
Sample : M4304-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P063-TW001-01

Quant Time: Oct 27 03:02:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 27 02:59:04 2021
Response via : Initial Calibration

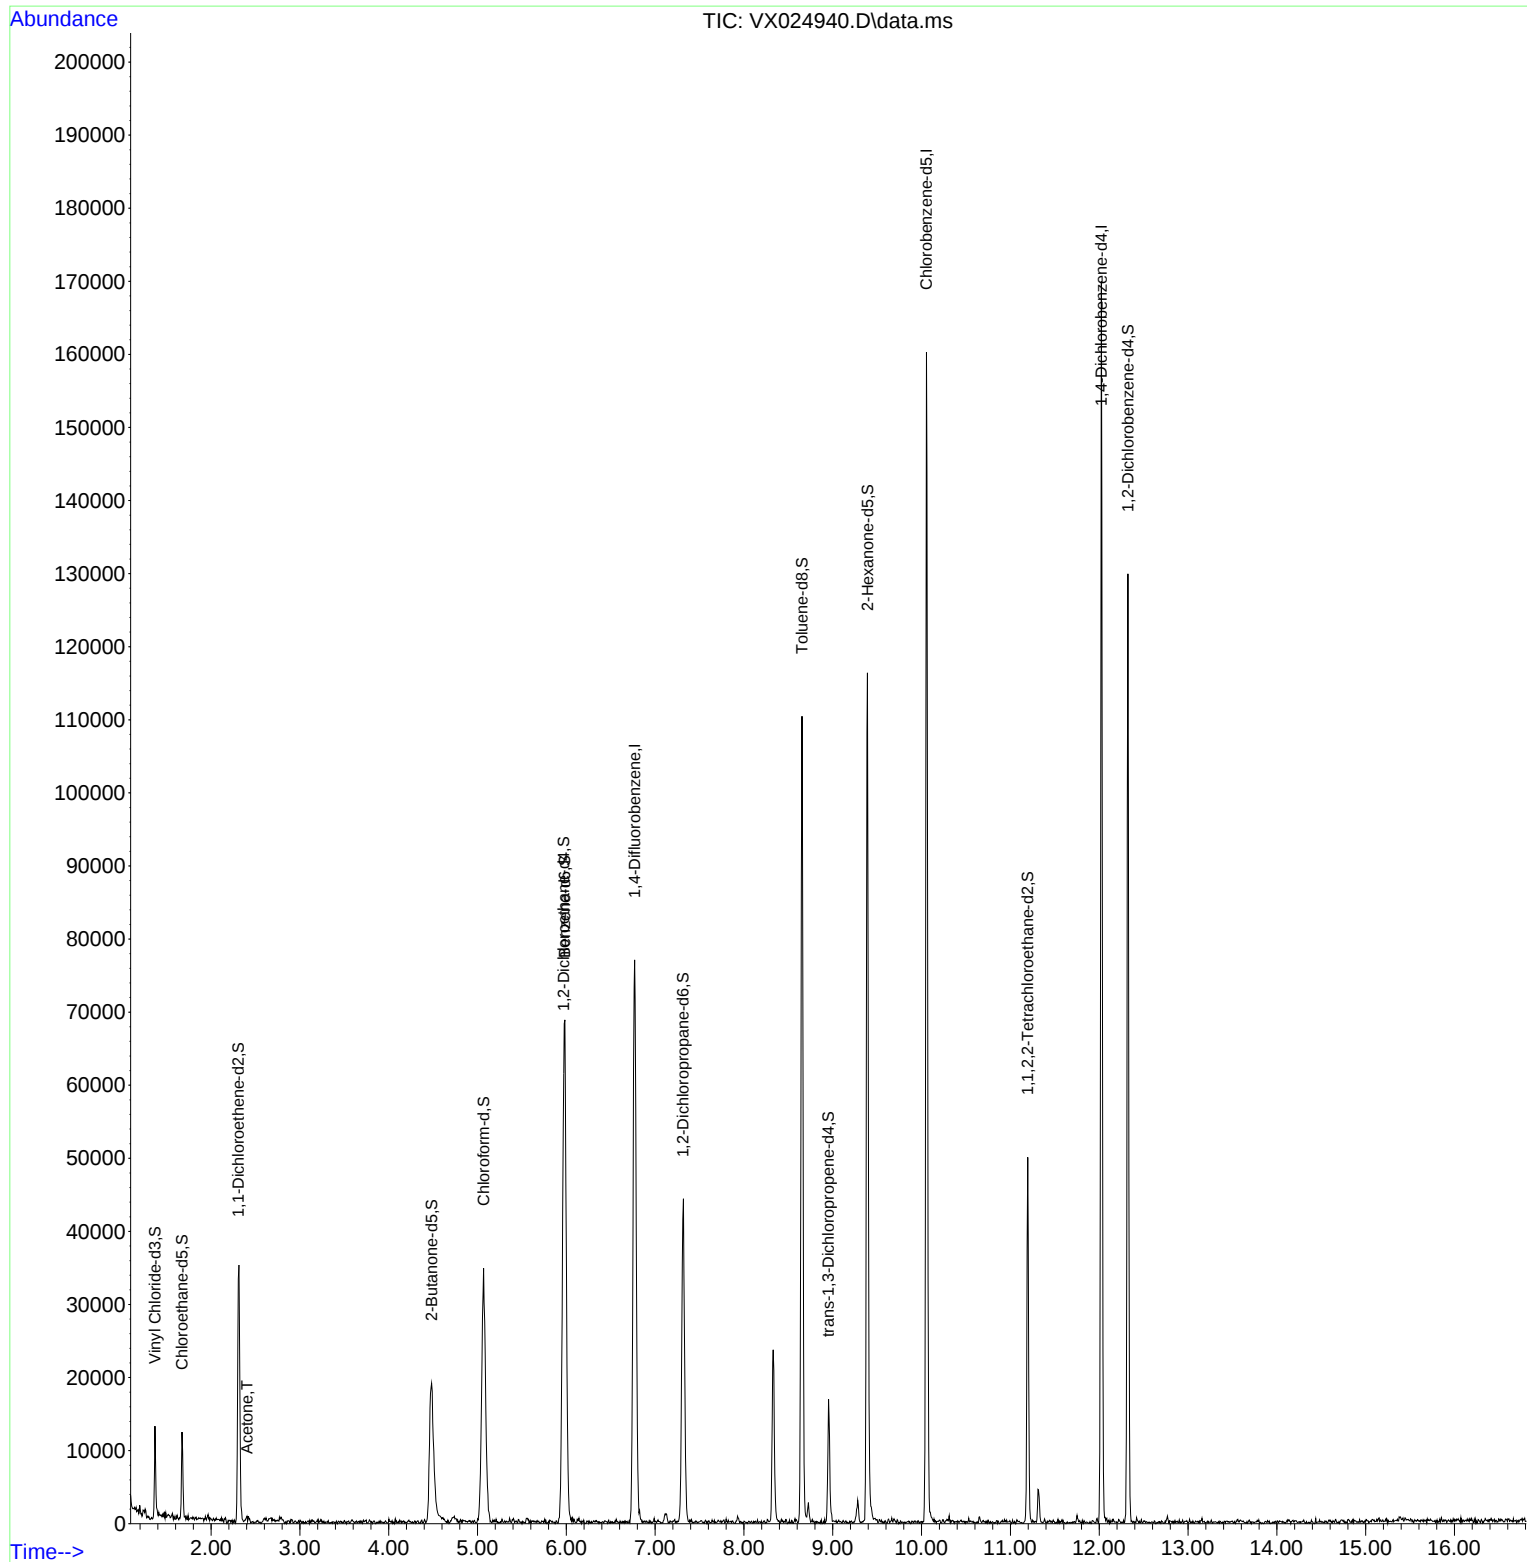

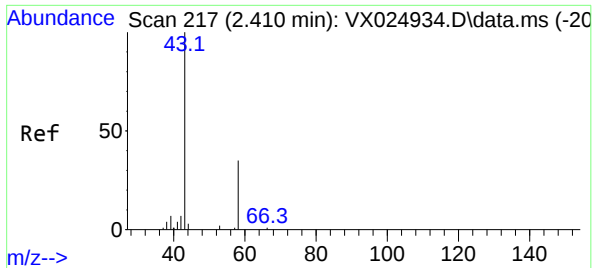

#13
 Acetone
 Concen: 1.788 ug/L
 RT: 2.404 min Scan# 216
 Delta R.T. -0.006 min
 Lab File: VX024940.D
 Acq: 26 Oct 2021 12:49

Instrument :
 MSVOA_X
 ClientSampleId :
 P063-TW001-01

Tgt Ion: 43	Resp: 1098
Ion Ratio	Lower Upper
43	100
58	17.4 0.0 64.2

