

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024945.D
 Acq On : 26 Oct 2021 14:48
 Operator : JC/MD
 Sample : M4304-08
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P067-TW001-01

Quant Time: Oct 27 03:03:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	77079	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	71217	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	34357	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	6899	3.049	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.000%
7) Chloroethane-d5	1.673	69	7065	3.465	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.400%
11) 1,1-Dichloroethene-d2	2.313	63	20434	2.422	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	48.400%#
20) 2-Butanone-d5	4.477	46	35783	43.251	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.500%
24) Chloroform-d	5.068	84	45353	4.163	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
26) 1,2-Dichloroethane-d4	5.964	65	24428	4.103	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
32) Benzene-d6	5.983	84	67996	4.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	7.312	67	20969	3.961	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.200%
41) Toluene-d8	8.653	98	64416	3.872	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.400%
43) trans-1,3-Dichloroprop...	8.952	79	9031	3.717	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	9.391	63	36395	41.617	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.240%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	18173	4.491	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	23322	4.028	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	80.600%
Target Compounds						Qvalue
3) Chloromethane	1.288	50	1300	0.421	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024945.D
Acq On : 26 Oct 2021 14:48
Operator : JC/MD
Sample : M4304-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P067-TW001-01

Quant Time: Oct 27 03:03:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 27 02:59:04 2021
Response via : Initial Calibration

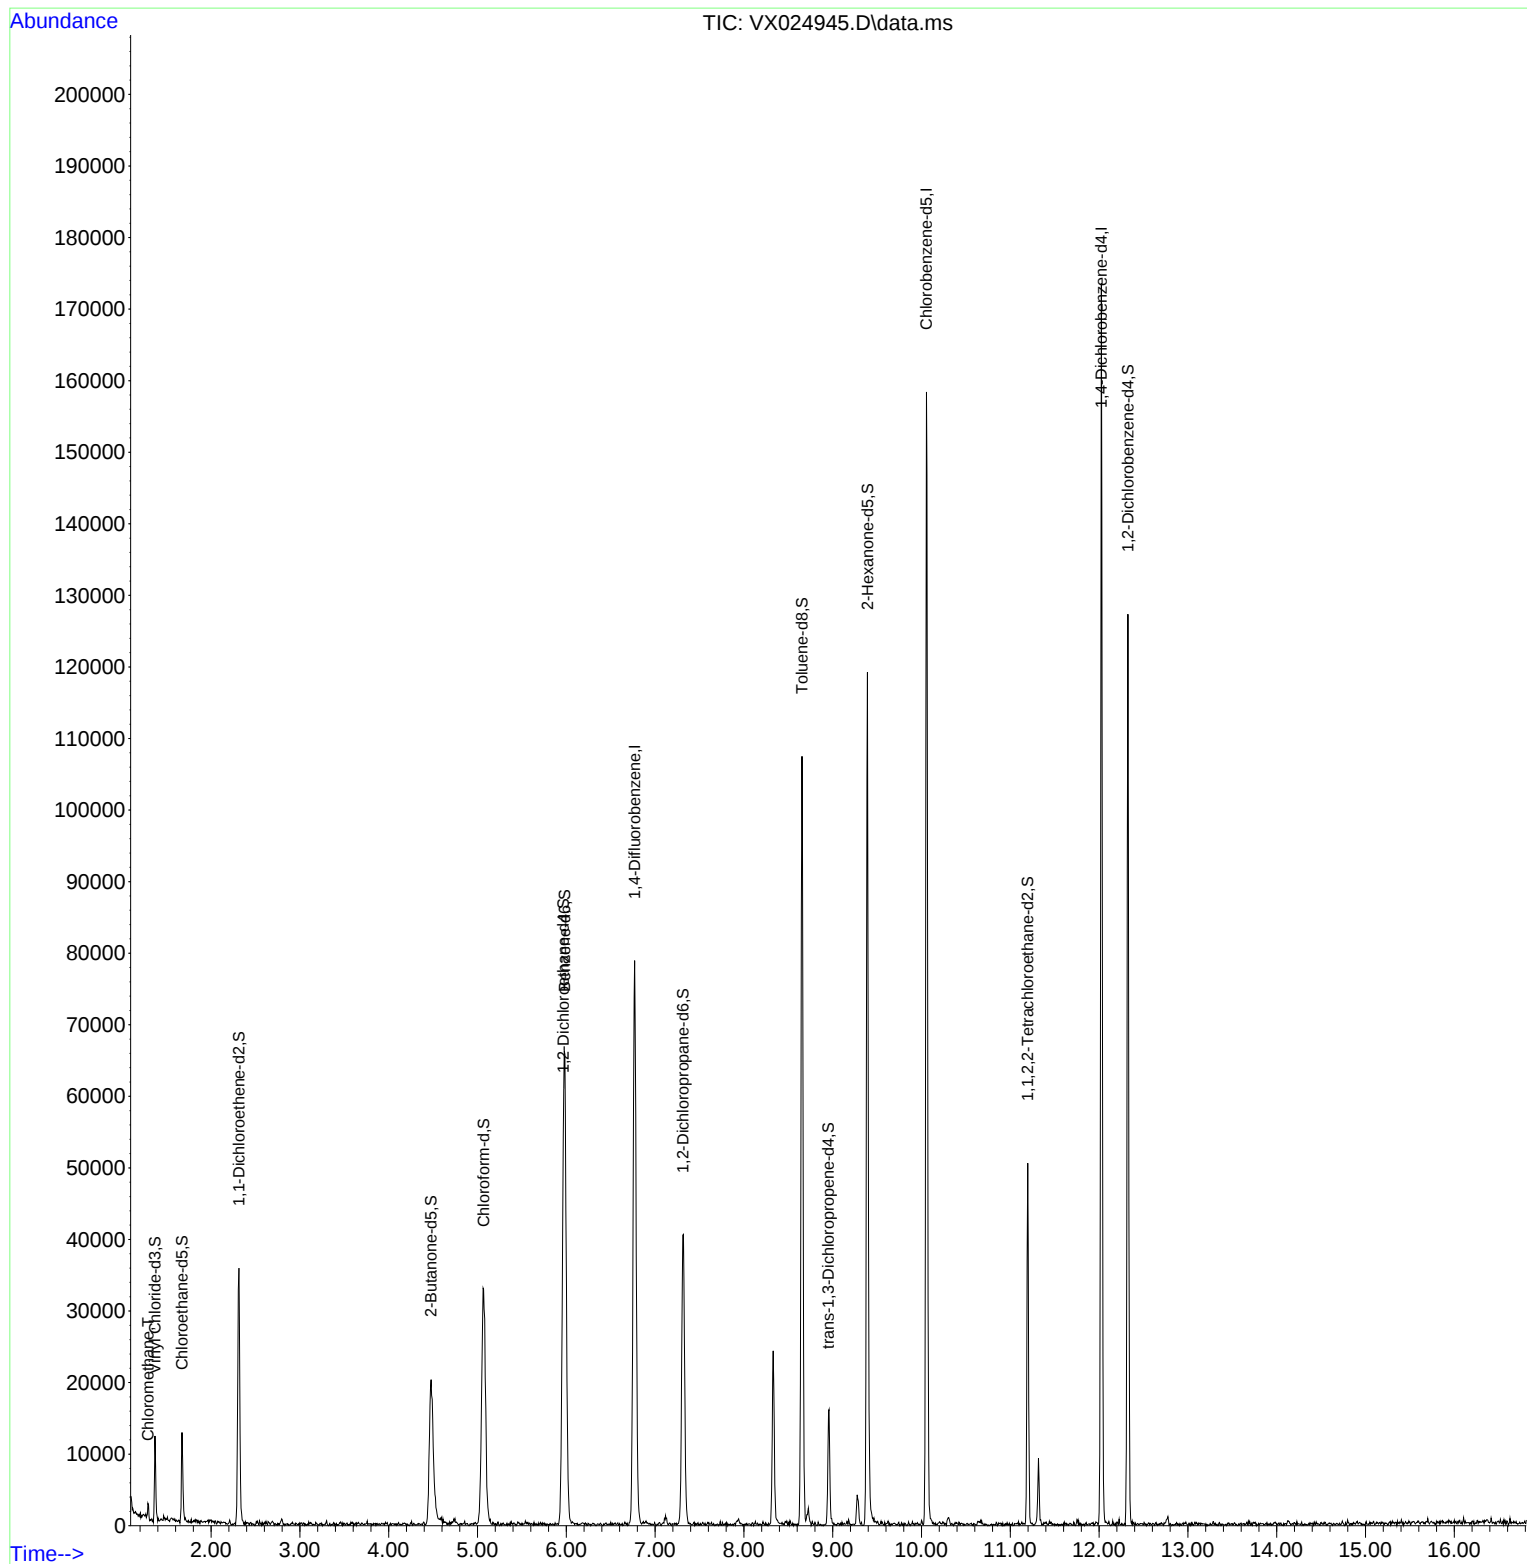

Abundance Scan 33 (1.288 min): VX024934.D\data.ms (-28)

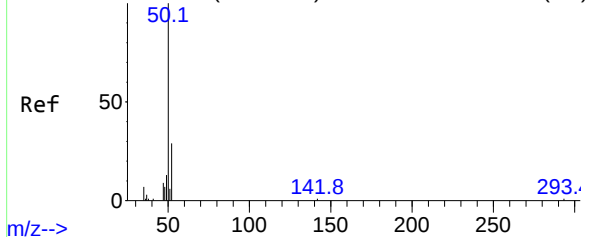

#3
Chloromethane
Concen: 0.421 ug/L
RT: 1.288 min Scan# 33
Delta R.T. -0.000 min
Lab File: VX024945.D
Acq: 26 Oct 2021 14:48

Instrument :
MSVOA_X
ClientSampleId :
P067-TW001-01

Tgt Ion: 50 Resp: 1300
Ion Ratio Lower Upper
50 100
52 33.1 25.5 47.3

