

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024948.D
 Acq On : 26 Oct 2021 16:00
 Operator : JC/MD
 Sample : M4304-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P073-TW001-01

Quant Time: Oct 27 03:04:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 02:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	60894	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	57831	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	26945	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	6489	3.630	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.672	69	7458	4.630	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.600%
11) 1,1-Dichloroethene-d2	2.313	63	20518	3.079	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.600%
20) 2-Butanone-d5	4.483	46	36353	55.619	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.240%
24) Chloroform-d	5.062	84	44490	5.170	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
26) 1,2-Dichloroethane-d4	5.964	65	23300	4.953	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	5.983	84	67930	5.041	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.800%
36) 1,2-Dichloropropane-d6	7.312	67	20336	4.730	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	8.653	98	65237	4.829	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
43) trans-1,3-Dichloroprop...	8.958	79	8763	4.441	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%
46) 2-Hexanone-d5	9.391	63	36358	51.198	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.400%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	17870	5.439	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	24536	5.403	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.000%
Target Compounds						
13) Acetone	2.416	43	1026	2.093	ug/L	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024948.D
Acq On : 26 Oct 2021 16:00
Operator : JC/MD
Sample : M4304-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P073-TW001-01


Quant Time: Oct 27 03:04:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 27 02:59:04 2021
Response via : Initial Calibration

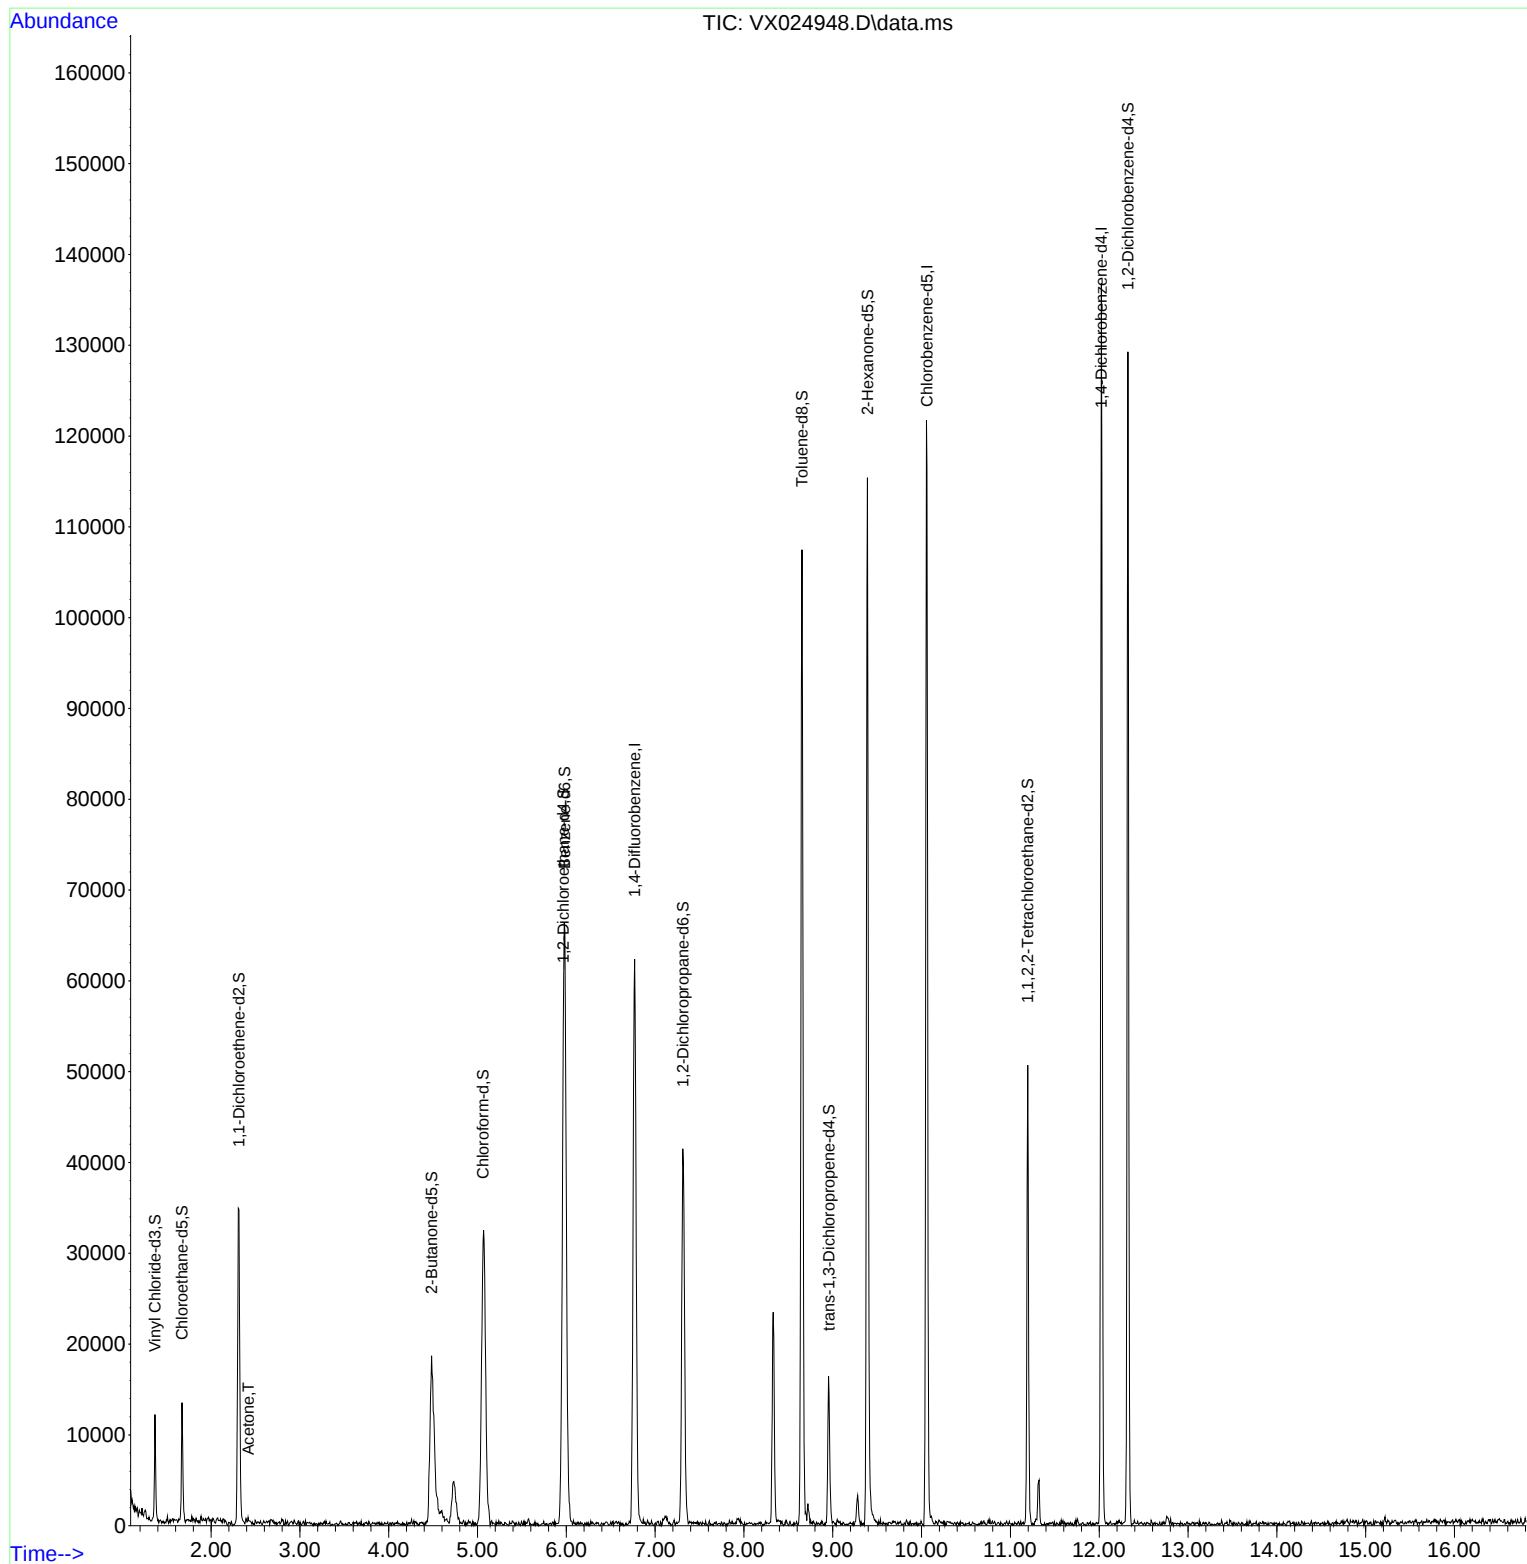

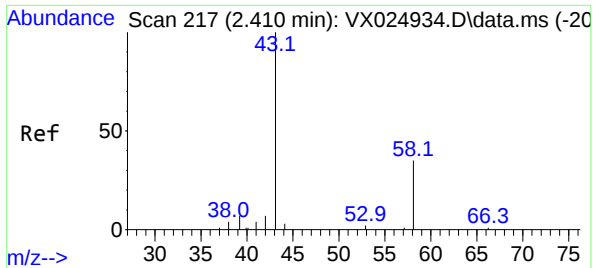

#13
Acetone
Concen: 2.093 ug/L
RT: 2.416 min Scan# 218
Delta R.T. 0.006 min
Lab File: VX024948.D
Acq: 26 Oct 2021 16:00

Instrument :
MSVOA_X
ClientSampleId :
P073-TW001-01

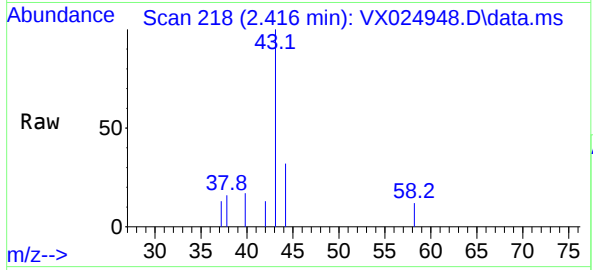

Tgt Ion: 43 Resp: 1026
Ion Ratio Lower Upper
43 100
58 4.2 0.0 64.2

