

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102621\  
 Data File : VX024938.D  
 Acq On : 26 Oct 2021 12:01  
 Operator : JC/MD  
 Sample : M4303-22  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024938.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.367       | 42            | 46          | 51           | rVB      | 13587          | 13419         | 5.95%           | 0.691%        |
| 2         | 1.672       | 92            | 96          | 104          | rVB      | 13299          | 16794         | 7.45%           | 0.864%        |
| 3         | 2.306       | 192           | 200         | 209          | rBV      | 41965          | 67416         | 29.90%          | 3.470%        |
| 4         | 2.794       | 276           | 280         | 285          | rBV2     | 1483           | 2316          | 1.03%           | 0.119%        |
| 5         | 4.501       | 548           | 560         | 573          | rBV3     | 14788          | 64059         | 28.41%          | 3.297%        |
| 6         | 5.074       | 641           | 654         | 671          | rBV2     | 37229          | 117616        | 52.16%          | 6.054%        |
| 7         | 5.976       | 791           | 802         | 816          | rBV4     | 77683          | 225475        | 100.00%         | 11.605%       |
| 8         | 6.769       | 919           | 932         | 943          | rBV2     | 73790          | 178306        | 79.08%          | 9.177%        |
| 9         | 7.318       | 1012          | 1022        | 1031         | rBV      | 47895          | 108481        | 48.11%          | 5.583%        |
| 10        | 8.330       | 1179          | 1188        | 1197         | rBV2     | 27365          | 48148         | 21.35%          | 2.478%        |
| 11        | 8.653       | 1234          | 1241        | 1249         | rBV      | 124430         | 195918        | 86.89%          | 10.084%       |
| 12        | 8.726       | 1249          | 1253        | 1258         | rVB2     | 2060           | 3524          | 1.56%           | 0.181%        |
| 13        | 8.951       | 1285          | 1290        | 1296         | rBV      | 18685          | 29779         | 13.21%          | 1.533%        |
| 14        | 9.390       | 1356          | 1362        | 1373         | rBV      | 130939         | 200544        | 88.94%          | 10.322%       |
| 15        | 10.055      | 1465          | 1471        | 1486         | rVB      | 149794         | 208060        | 92.28%          | 10.709%       |
| 16        | 11.195      | 1653          | 1658        | 1665         | rBV      | 54437          | 70339         | 31.20%          | 3.620%        |
| 17        | 12.024      | 1789          | 1794        | 1800         | rBV      | 161603         | 209714        | 93.01%          | 10.794%       |
| 18        | 12.323      | 1837          | 1843        | 1850         | rVB      | 145397         | 182983        | 81.15%          | 9.418%        |




Sum of corrected areas: 1942891

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102621\  
Data File : VX024938.D  
Acq On : 26 Oct 2021 12:01  
Operator : JC/MD  
Sample : M4303-22  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

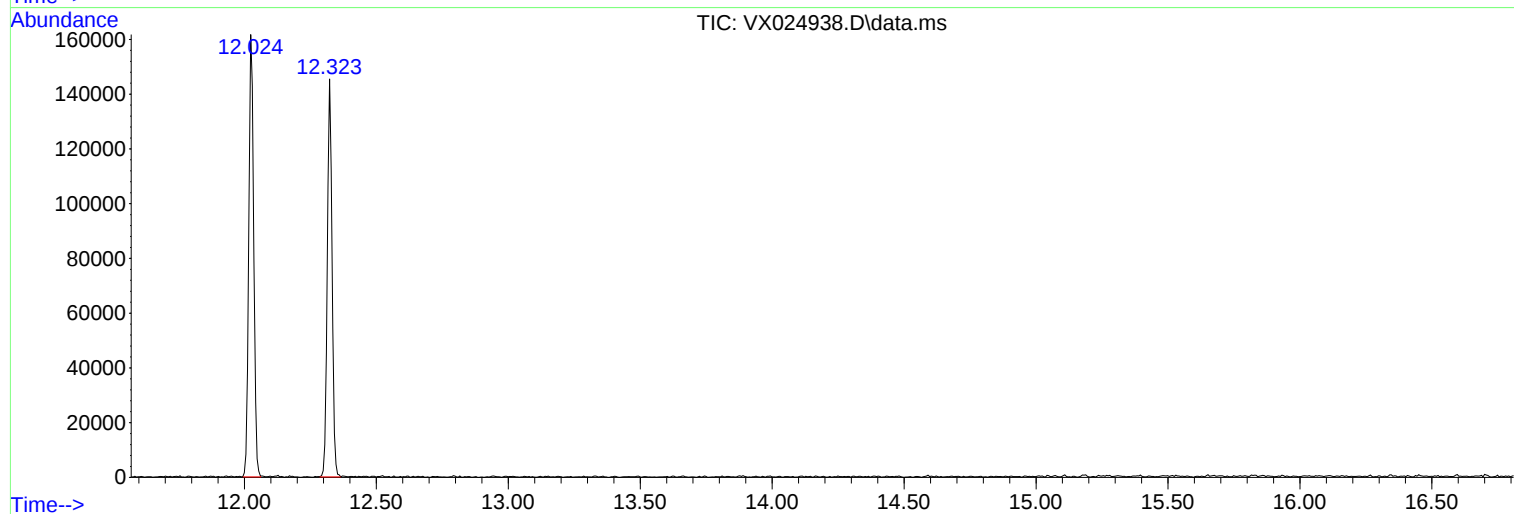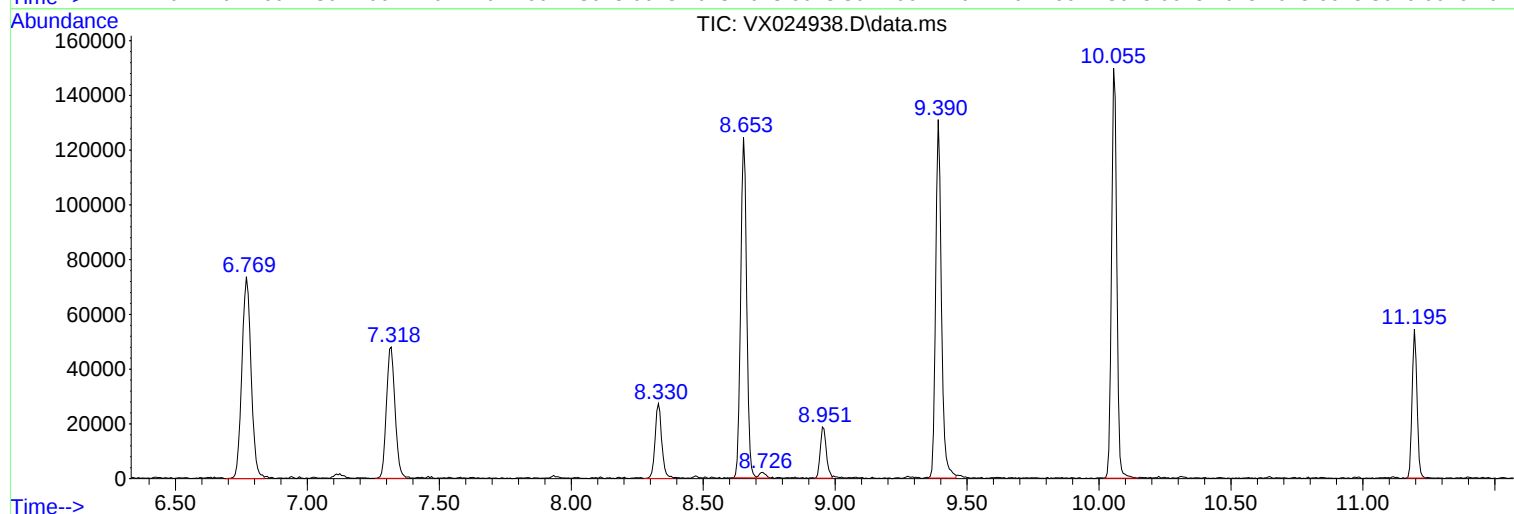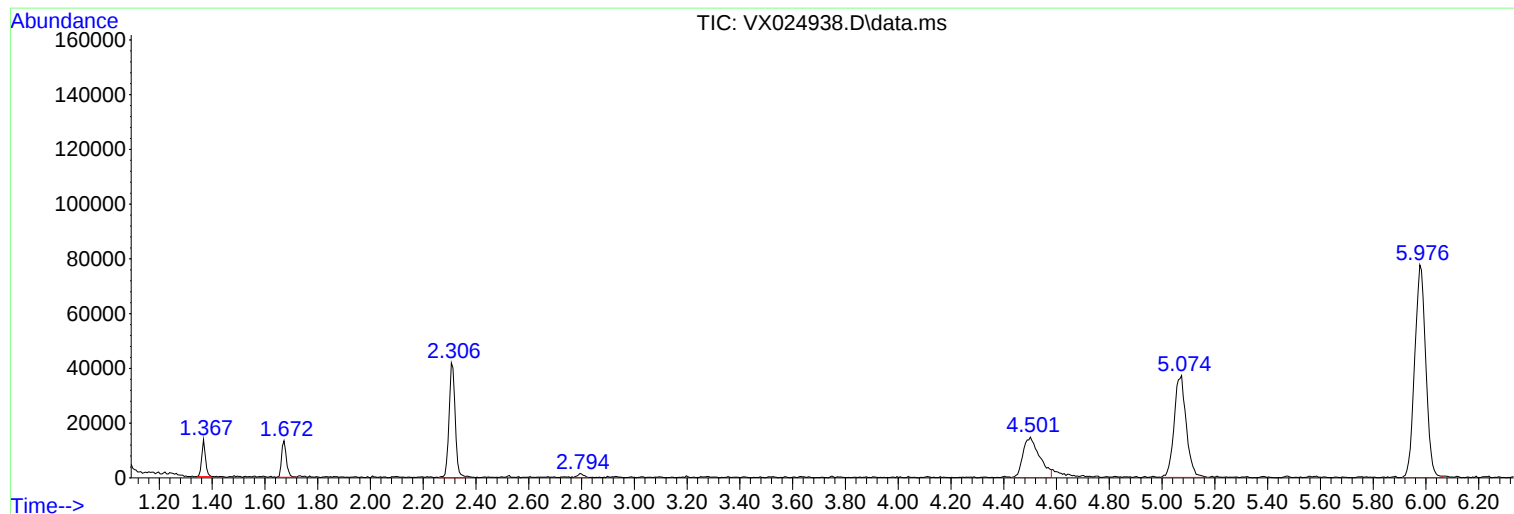

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102621\  
Data File : VX024938.D  
Acq On : 26 Oct 2021 12:01  
Operator : JC/MD  
Sample : M4303-22  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102621\  
Data File : VX024938.D  
Acq On : 26 Oct 2021 12:01  
Operator : JC/MD  
Sample : M4303-22  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----