

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024939.D
 Acq On : 26 Oct 2021 12:25
 Operator : JC/MD
 Sample : M4304-04
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P061-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	55	rVB	12083	13198	6.01%	0.720%
2	1.672	91	96	102	rVB	12606	16165	7.36%	0.881%
3	2.306	195	200	212	rVB	36496	58842	26.79%	3.208%
4	4.477	548	556	570	rBV	17759	65106	29.65%	3.550%
5	5.068	642	653	668	rBV2	33988	106269	48.39%	5.794%
6	5.976	790	802	815	rBV4	70603	202713	92.30%	11.053%
7	6.769	923	932	945	rBV	76916	188069	85.64%	10.255%
8	7.311	1012	1021	1033	rBV2	42253	97025	44.18%	5.290%
9	8.330	1181	1188	1196	rVB	25061	42571	19.38%	2.321%
10	8.653	1235	1241	1248	rBV	110895	174992	79.68%	9.542%
11	8.720	1248	1252	1258	rVB2	2024	4131	1.88%	0.225%
12	8.951	1285	1290	1297	rVB	15379	24297	11.06%	1.325%
13	9.275	1340	1343	1350	rVB2	1560	2220	1.01%	0.121%
14	9.390	1355	1362	1372	rBV	118899	172132	78.38%	9.386%
15	10.055	1466	1471	1483	rBV	157750	219614	100.00%	11.975%
16	11.195	1653	1658	1665	rVB2	47858	64344	29.30%	3.508%
17	11.317	1671	1678	1684	rBV4	2313	3948	1.80%	0.215%
18	12.024	1789	1794	1801	rBV	170211	214816	97.82%	11.713%
19	12.323	1837	1843	1850	rBV	128291	163516	74.46%	8.916%




Sum of corrected areas: 1833968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024939.D
Acq On : 26 Oct 2021 12:25
Operator : JC/MD
Sample : M4304-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P061-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

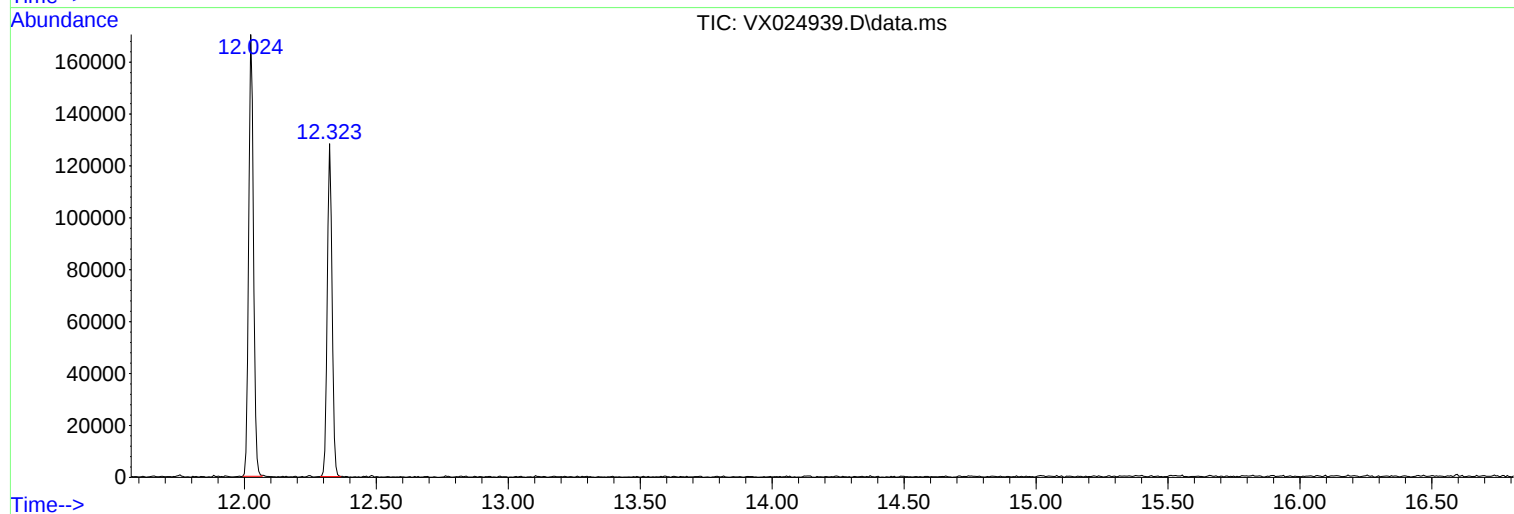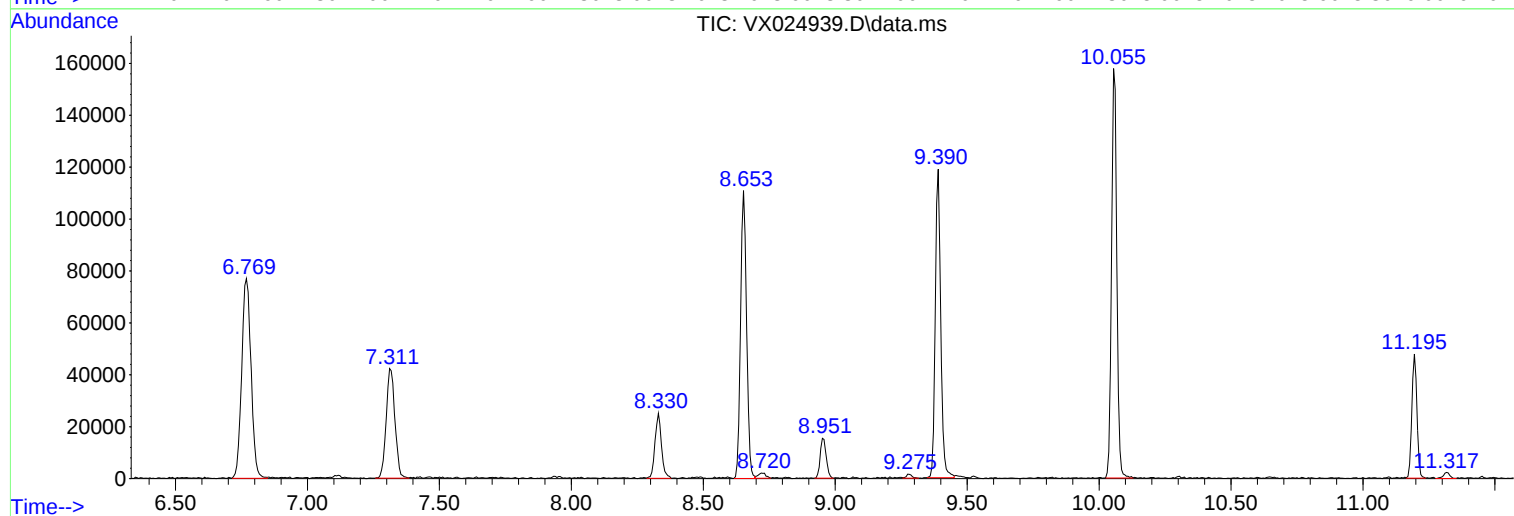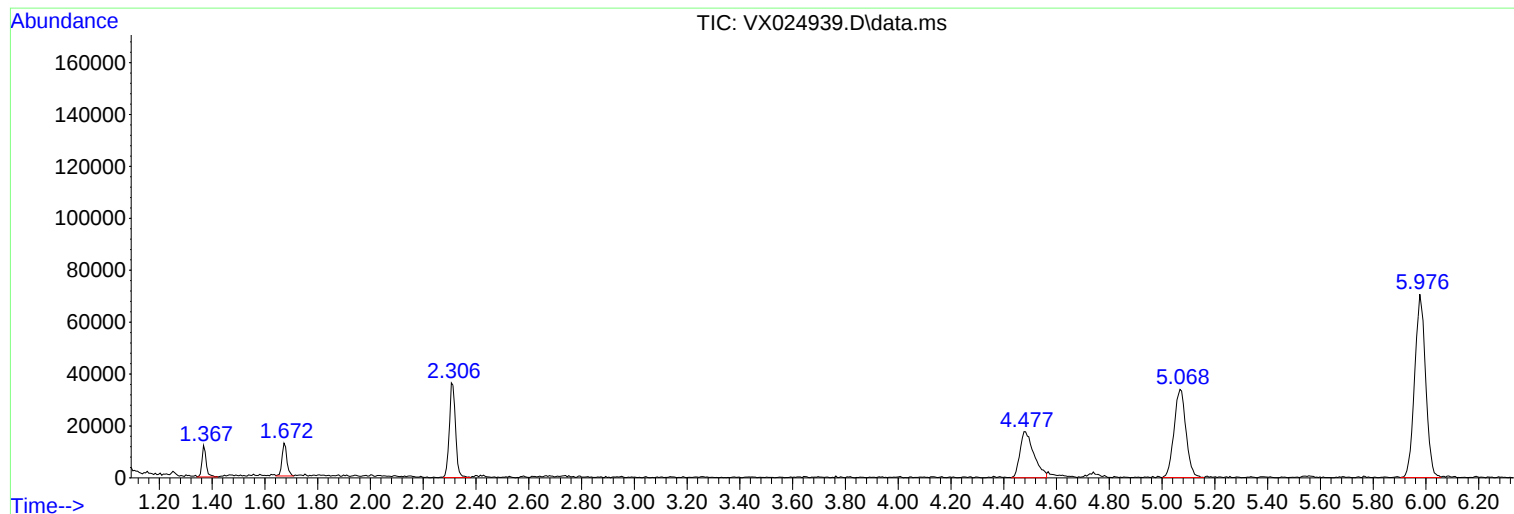

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024939.D
Acq On : 26 Oct 2021 12:25
Operator : JC/MD
Sample : M4304-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P061-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024939.D
Acq On : 26 Oct 2021 12:25
Operator : JC/MD
Sample : M4304-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P061-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
