

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024940.D
 Acq On : 26 Oct 2021 12:49
 Operator : JC/MD
 Sample : M4304-05
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P063-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	41	46	52	rBV	12710	13644	6.26%	0.741%
2	1.672	92	96	101	rBV	11820	13382	6.14%	0.727%
3	2.312	195	201	210	rBV	35286	58114	26.66%	3.156%
4	4.483	546	557	576	rBV2	19140	66745	30.61%	3.625%
5	4.739	589	599	600	rBV	988	2317	1.06%	0.126%
6	5.068	639	653	665	rBV2	34850	105657	48.46%	5.738%
7	5.983	790	803	816	rBV3	68902	203184	93.20%	11.034%
8	6.769	923	932	946	rBV	77022	189897	87.10%	10.313%
9	7.123	984	990	996	rVB4	1283	2772	1.27%	0.151%
10	7.318	1012	1022	1033	rVB	44252	96791	44.40%	5.256%
11	8.330	1180	1188	1197	rBV	23533	41480	19.03%	2.253%
12	8.653	1233	1241	1250	rBV	110376	171292	78.57%	9.302%
13	8.726	1250	1253	1257	rVB2	2698	3401	1.56%	0.185%
14	8.952	1284	1290	1298	rBV2	16921	25806	11.84%	1.401%
15	9.281	1338	1344	1349	rVB2	3042	4676	2.14%	0.254%
16	9.390	1356	1362	1373	rBV	115981	174481	80.03%	9.475%
17	10.055	1465	1471	1484	rBV	160012	218019	100.00%	11.840%
18	11.195	1650	1658	1666	rBV2	50079	66357	30.44%	3.604%
19	11.311	1674	1677	1683	rBV3	4479	6593	3.02%	0.358%
20	12.024	1789	1794	1802	rBV	169916	214647	98.45%	11.657%
21	12.323	1838	1843	1849	rVB	129627	162151	74.37%	8.806%




Sum of corrected areas: 1841406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024940.D
Acq On : 26 Oct 2021 12:49
Operator : JC/MD
Sample : M4304-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P063-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

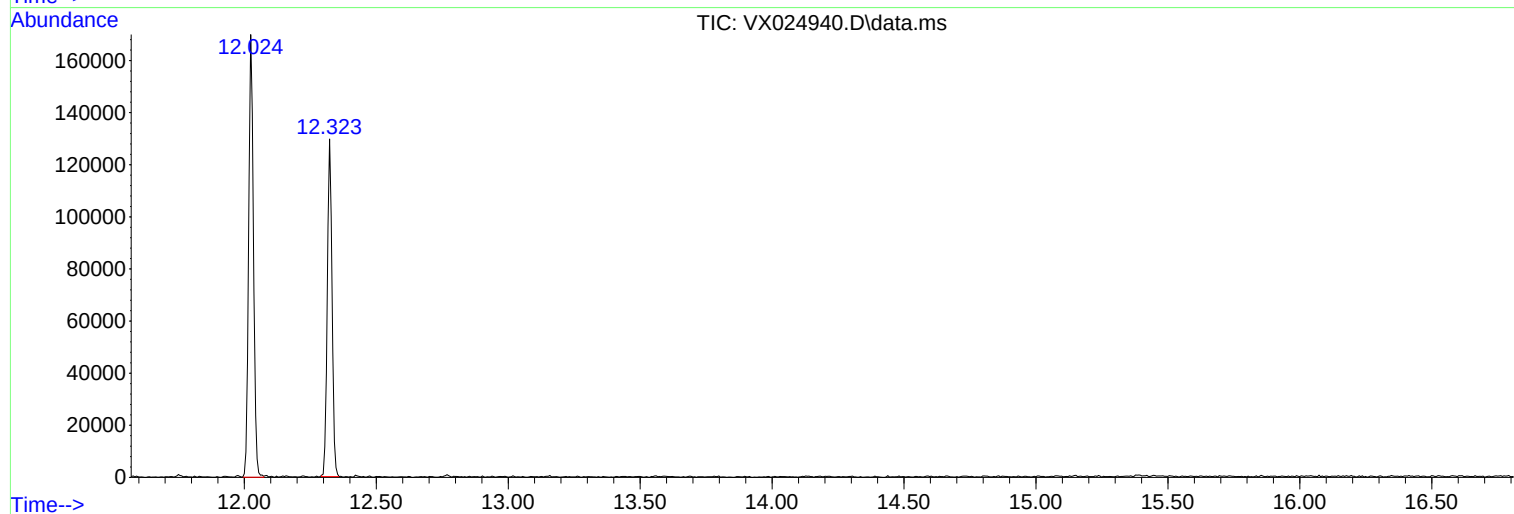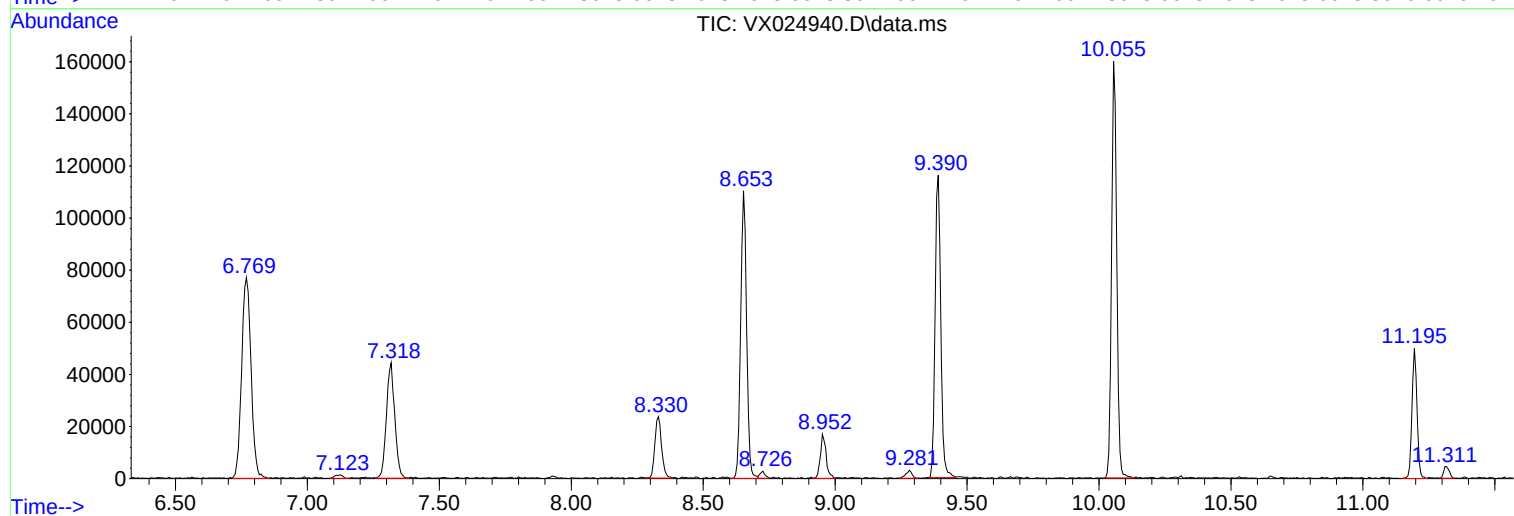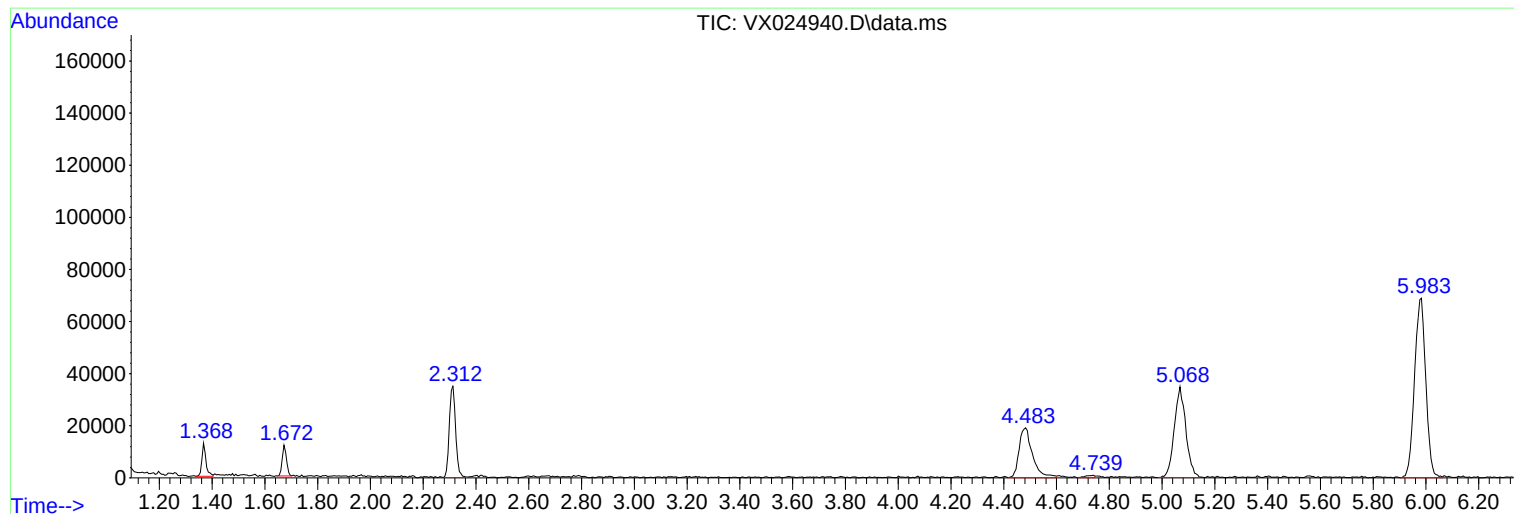

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024940.D
Acq On : 26 Oct 2021 12:49
Operator : JC/MD
Sample : M4304-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P063-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024940.D
Acq On : 26 Oct 2021 12:49
Operator : JC/MD
Sample : M4304-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P063-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
