

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024941.D
 Acq On : 26 Oct 2021 13:13
 Operator : JC/MD
 Sample : VIBLK601
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK601

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	13372	13463	6.28%	0.733%
2	1.673	90	96	101	rBV	12897	16404	7.65%	0.894%
3	2.313	194	201	207	rBV	39543	61703	28.77%	3.362%
4	2.794	274	280	286	rVB3	1937	4115	1.92%	0.224%
5	4.483	547	557	578	rBV	20279	69398	32.36%	3.781%
6	5.068	640	653	666	rVB	34058	109736	51.17%	5.979%
7	5.977	790	802	814	rBV4	73491	214437	100.00%	11.683%
8	6.769	923	932	942	rBV2	69345	168723	78.68%	9.192%
9	7.117	983	989	994	rBV3	1851	2944	1.37%	0.160%
10	7.318	1012	1022	1030	rBV	46095	100624	46.92%	5.482%
11	8.330	1181	1188	1198	rBV2	25140	44835	20.91%	2.443%
12	8.653	1234	1241	1248	rBV	118415	180566	84.20%	9.837%
13	8.714	1248	1251	1257	rVB3	2365	3988	1.86%	0.217%
14	8.952	1286	1290	1298	rBV2	17151	27470	12.81%	1.497%
15	9.275	1340	1343	1349	rVB3	2519	3699	1.72%	0.202%
16	9.391	1356	1362	1374	rBV	126336	186425	86.94%	10.157%
17	10.055	1466	1471	1483	rBV	141621	196545	91.66%	10.708%
18	11.195	1653	1658	1665	rVB	51291	67130	31.31%	3.657%
19	11.317	1675	1678	1683	rBV2	2457	3370	1.57%	0.184%
20	12.024	1789	1794	1804	rVB	153214	191931	89.50%	10.457%
21	12.323	1838	1843	1849	rBV	131849	167982	78.34%	9.152%




Sum of corrected areas: 1835488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024941.D
Acq On : 26 Oct 2021 13:13
Operator : JC/MD
Sample : VIBLK601
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

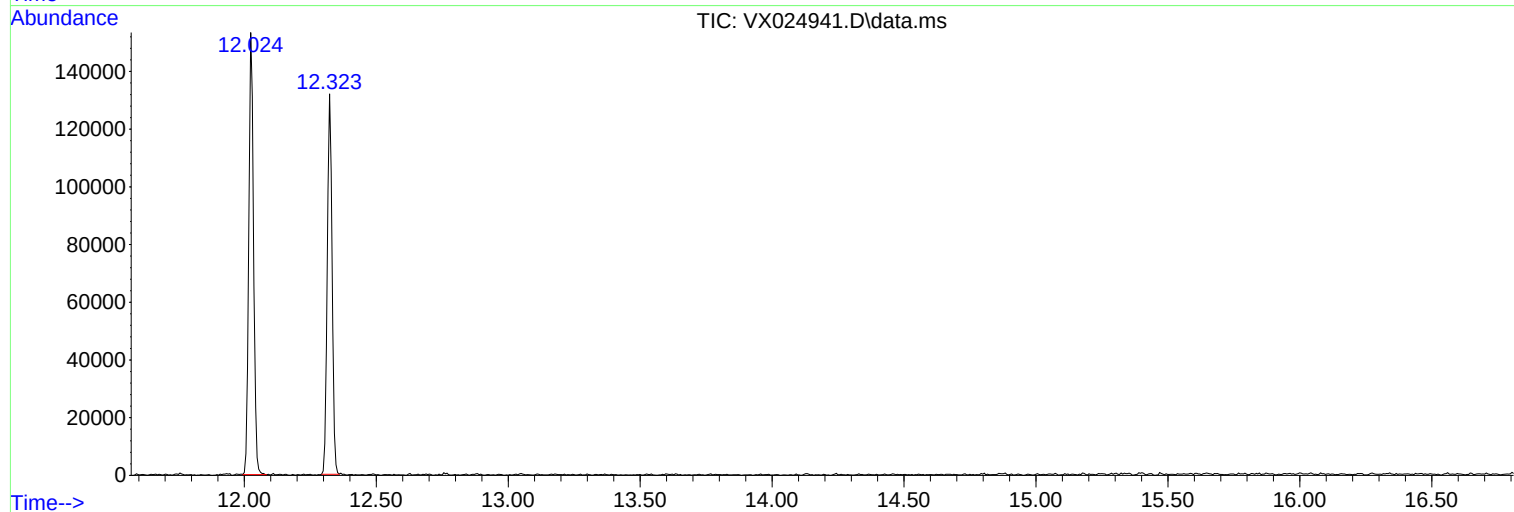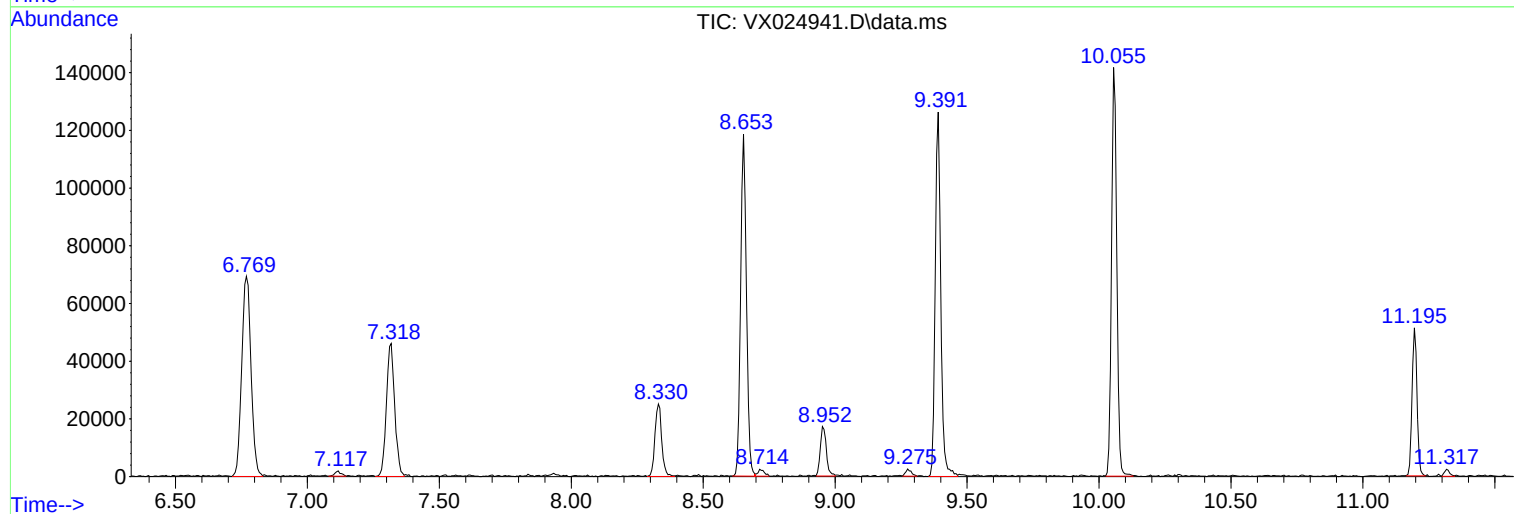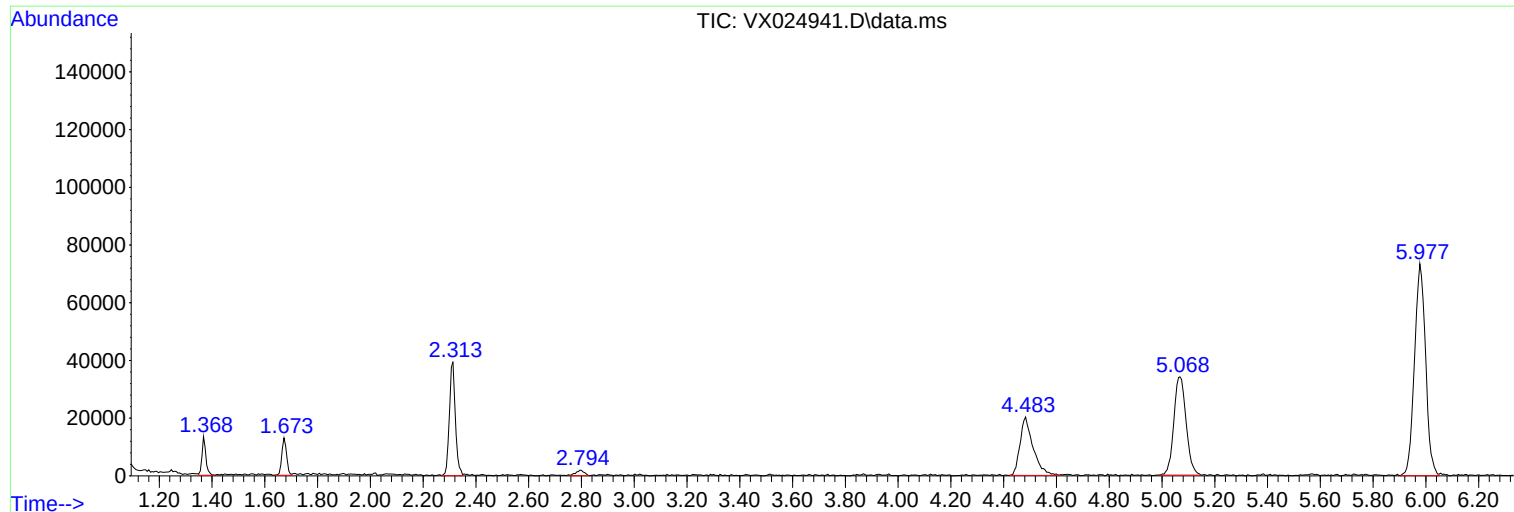

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024941.D
Acq On : 26 Oct 2021 13:13
Operator : JC/MD
Sample : VIBLK601
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024941.D
Acq On : 26 Oct 2021 13:13
Operator : JC/MD
Sample : VIBLK601
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc