

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024943.D
 Acq On : 26 Oct 2021 14:00
 Operator : JC/MD
 Sample : M4304-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P064-TW001-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	12344	12092	5.61%	0.658%
2	1.672	93	96	101	rVB	12214	14813	6.87%	0.807%
3	2.313	193	201	211	rBV	37517	60645	28.14%	3.302%
4	4.483	548	557	570	rBV	19276	66450	30.83%	3.618%
5	4.727	596	597	606	rVB4	1764	3301	1.53%	0.180%
6	5.068	640	653	666	rBV2	34028	106673	49.49%	5.809%
7	5.977	791	802	815	rBV4	67119	202943	94.16%	11.051%
8	6.769	923	932	945	rBV	77356	181787	84.35%	9.899%
9	7.318	1008	1022	1036	rBV2	43247	97287	45.14%	5.297%
10	8.330	1180	1188	1197	rBV2	25446	42919	19.91%	2.337%
11	8.653	1234	1241	1249	rBV	112397	174643	81.03%	9.510%
12	8.720	1249	1252	1257	rVB2	2334	3730	1.73%	0.203%
13	8.952	1285	1290	1299	rBV	16378	25976	12.05%	1.414%
14	9.391	1356	1362	1373	rBV	124021	176777	82.02%	9.626%
15	10.055	1464	1471	1484	rBV	153463	215527	100.00%	11.736%
16	11.195	1652	1658	1665	rBV	55276	67007	31.09%	3.649%
17	11.317	1674	1678	1682	rBV4	2337	3631	1.68%	0.198%
18	12.024	1789	1794	1805	rVB	167546	214308	99.43%	11.669%
19	12.323	1837	1843	1851	rBV	131492	165987	77.01%	9.038%




Sum of corrected areas: 1836496

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024943.D
Acq On : 26 Oct 2021 14:00
Operator : JC/MD
Sample : M4304-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P064-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

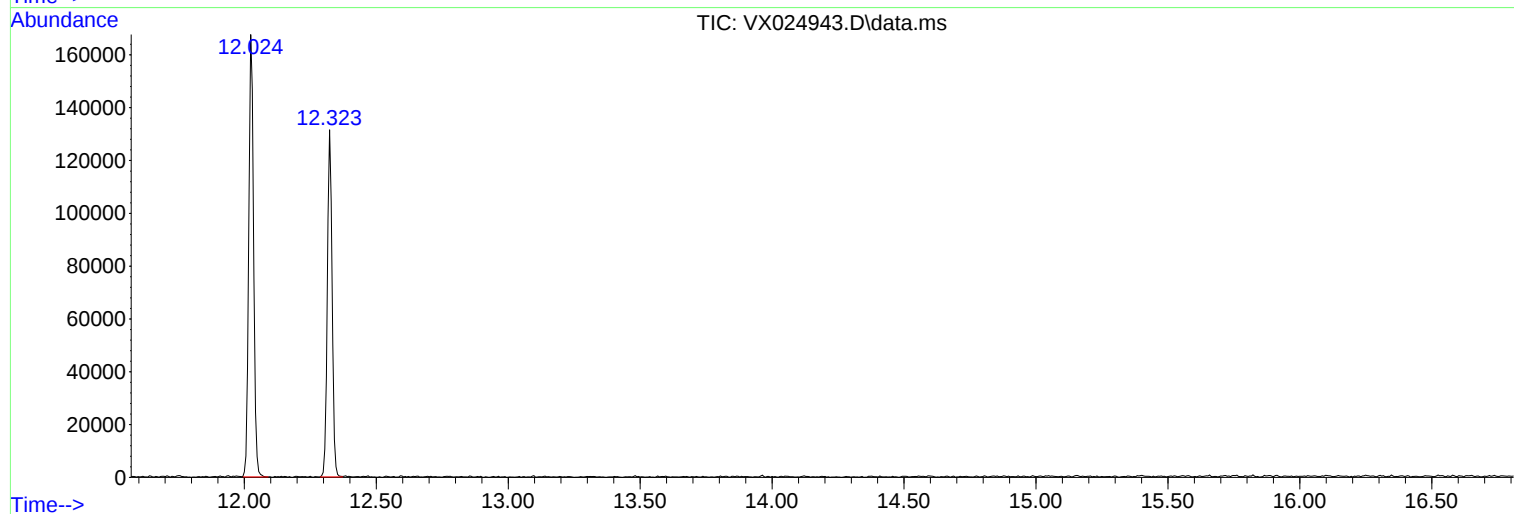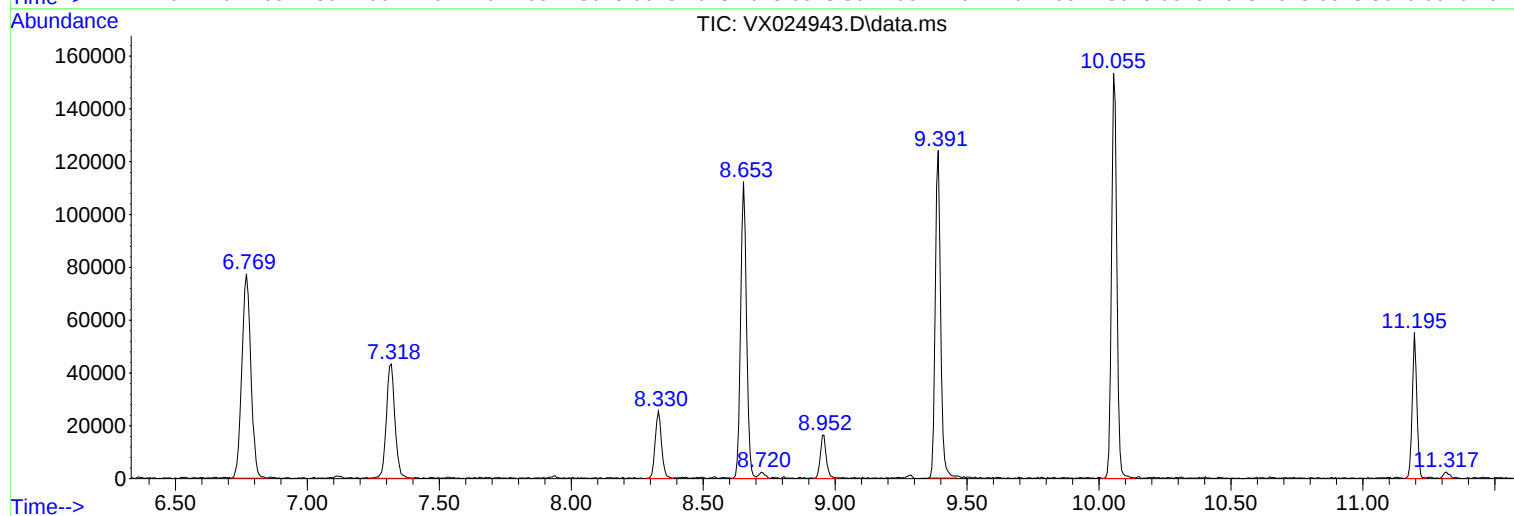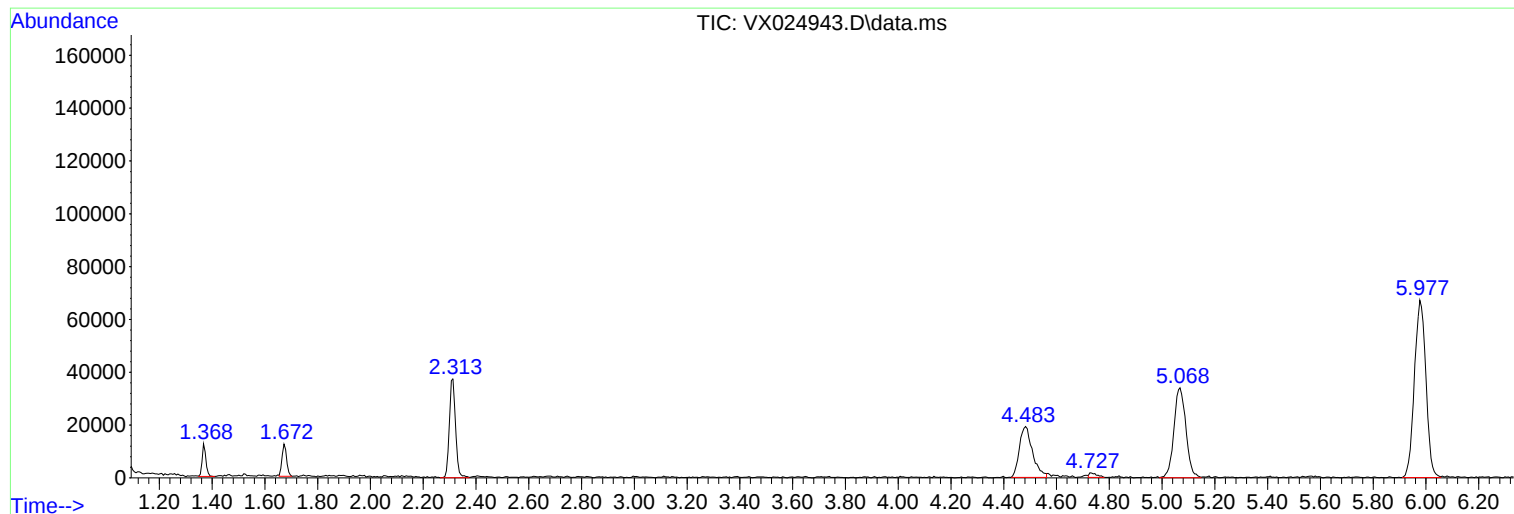

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024943.D
Acq On : 26 Oct 2021 14:00
Operator : JC/MD
Sample : M4304-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P064-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024943.D
Acq On : 26 Oct 2021 14:00
Operator : JC/MD
Sample : M4304-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P064-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
