

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024944.D
 Acq On : 26 Oct 2021 14:24
 Operator : JC/MD
 Sample : M4304-07
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P066-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	51	rBV	12697	12896	6.37%	0.717%
2	1.672	92	96	103	rVB	13730	15326	7.57%	0.852%
3	2.312	194	201	211	rBV	37344	59958	29.61%	3.334%
4	2.800	279	281	287	rVB2	2184	2599	1.28%	0.145%
5	4.477	546	556	571	rBV	20915	67147	33.16%	3.734%
6	5.068	644	653	664	rBV	33849	103835	51.28%	5.774%
7	5.976	791	802	813	rBV2	69018	202479	100.00%	11.259%
8	6.769	920	932	944	rBV2	73990	175490	86.67%	9.758%
9	7.116	984	989	995	rVB2	1061	2380	1.18%	0.132%
10	7.312	1014	1021	1034	rBV	42388	95116	46.98%	5.289%
11	8.330	1181	1188	1195	rVB	23442	40632	20.07%	2.259%
12	8.653	1235	1241	1248	rBV	111677	172973	85.43%	9.618%
13	8.720	1248	1252	1261	rVB	2186	3986	1.97%	0.222%
14	8.958	1285	1291	1296	rBV	15549	25061	12.38%	1.393%
15	9.275	1340	1343	1349	rVB	3950	5028	2.48%	0.280%
16	9.390	1354	1362	1369	rBV	118695	175418	86.64%	9.754%
17	10.055	1465	1471	1477	rBV	140663	200134	98.84%	11.128%
18	11.195	1653	1658	1665	rVB2	49545	64088	31.65%	3.564%
19	11.317	1673	1678	1684	rBB2	7034	8998	4.44%	0.500%
20	12.024	1788	1794	1803	rVB	157283	200631	99.09%	11.156%
21	12.323	1836	1843	1852	rBV	129874	164250	81.12%	9.133%




Sum of corrected areas: 1798425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024944.D
Acq On : 26 Oct 2021 14:24
Operator : JC/MD
Sample : M4304-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P066-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

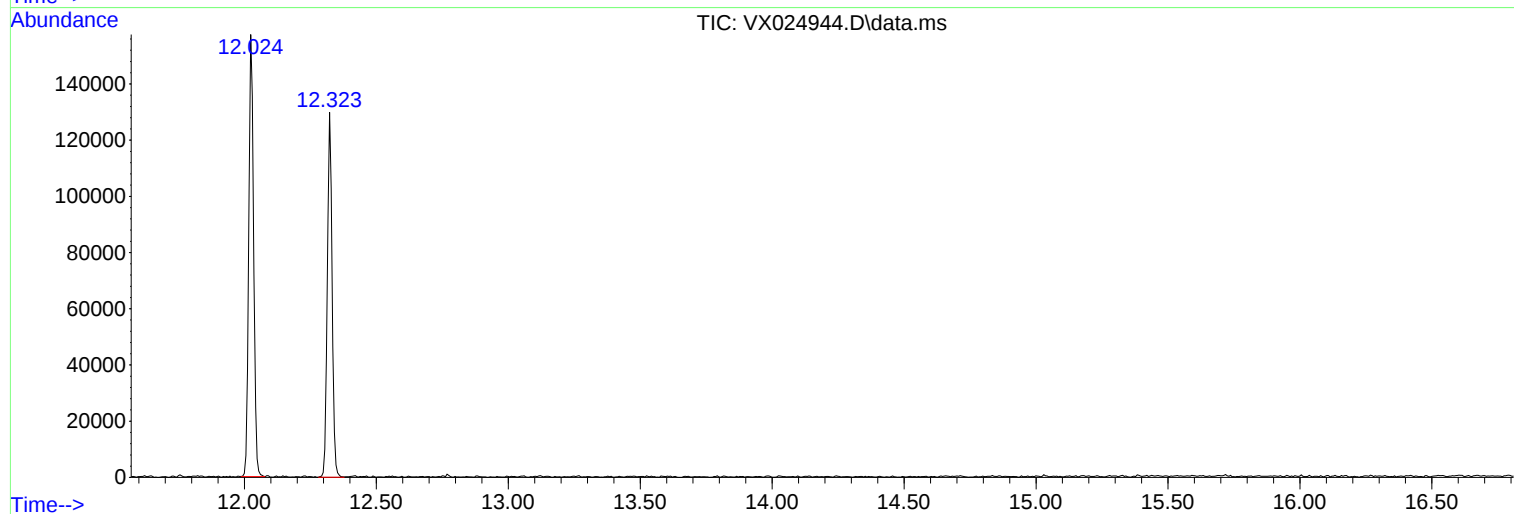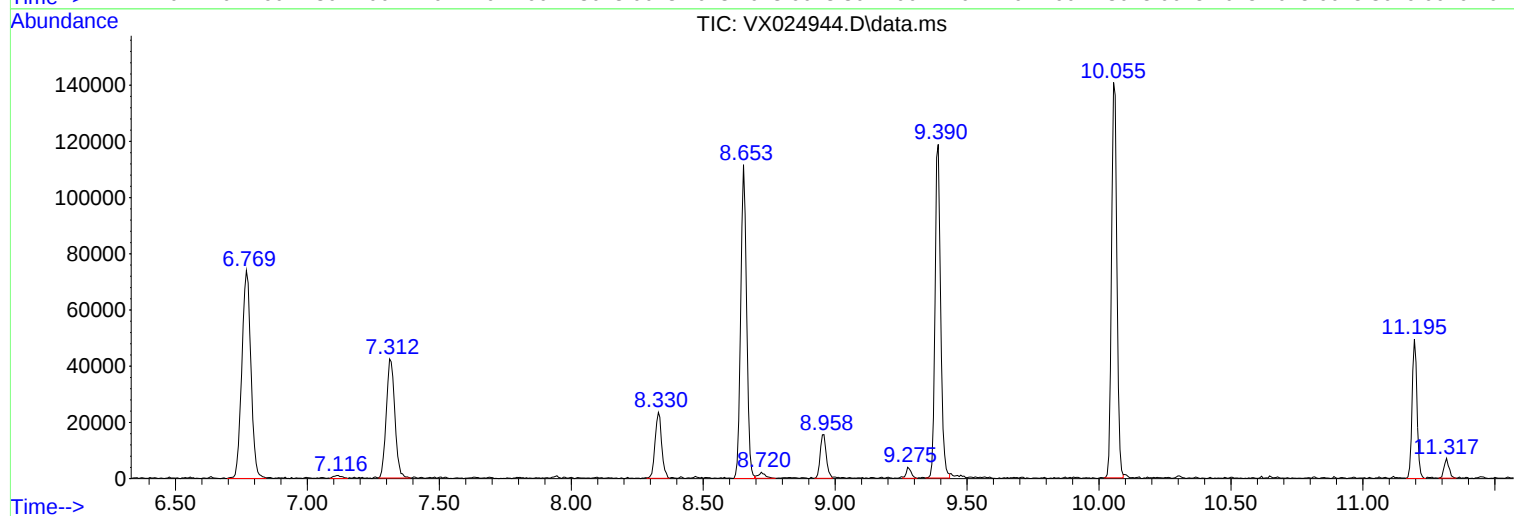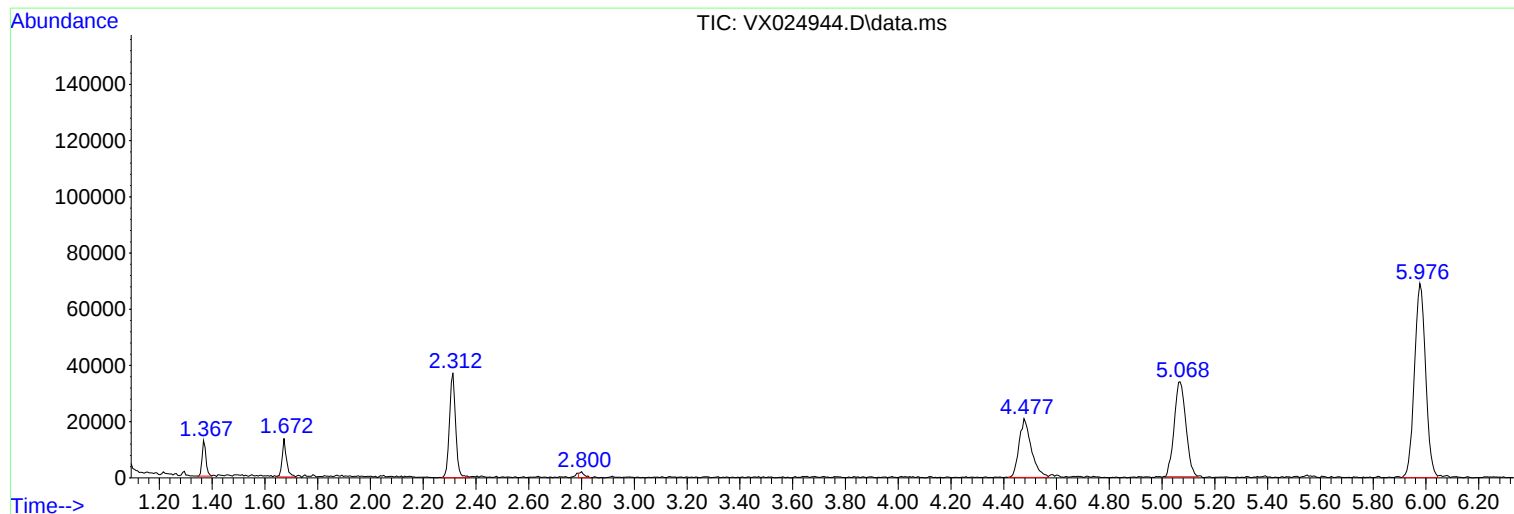

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024944.D
Acq On : 26 Oct 2021 14:24
Operator : JC/MD
Sample : M4304-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P066-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024944.D
Acq On : 26 Oct 2021 14:24
Operator : JC/MD
Sample : M4304-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P066-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
