

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024945.D
 Acq On : 26 Oct 2021 14:48
 Operator : JC/MD
 Sample : M4304-08
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P067-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	30	33	36	rVB2	2410	2443	1.12%	0.134%
2	1.368	43	46	51	rBV	12075	12722	5.81%	0.698%
3	1.673	92	96	105	rBV	12682	15872	7.25%	0.871%
4	2.313	195	201	212	rVB	35845	57272	26.16%	3.144%
5	4.477	545	556	571	rBV	20339	65986	30.14%	3.622%
6	5.062	640	652	669	rVB3	33002	102204	46.69%	5.611%
7	5.977	791	802	815	rBV4	66231	196443	89.73%	10.784%
8	6.769	919	932	945	rBV	78963	189665	86.64%	10.412%
9	7.318	1012	1022	1034	rVB	40452	92696	42.34%	5.089%
10	8.330	1182	1188	1200	rBV	24208	39532	18.06%	2.170%
11	8.653	1234	1241	1248	rBV	107421	167317	76.43%	9.185%
12	8.726	1248	1253	1258	rVB3	2478	4390	2.01%	0.241%
13	8.958	1281	1291	1299	rBV2	16247	26092	11.92%	1.432%
14	9.275	1338	1343	1349	rBV3	4182	6934	3.17%	0.381%
15	9.391	1355	1362	1375	rBV	119215	172474	78.78%	9.468%
16	10.055	1465	1471	1484	rBV	158277	218918	100.00%	12.018%
17	11.195	1653	1658	1665	rBV	50454	62945	28.75%	3.455%
18	11.317	1668	1678	1681	rBV3	9355	11487	5.25%	0.631%
19	12.024	1788	1794	1801	rBV	173418	216965	99.11%	11.911%
20	12.323	1838	1843	1850	rBV	127221	159238	72.74%	8.742%




Sum of corrected areas: 1821595

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024945.D
Acq On : 26 Oct 2021 14:48
Operator : JC/MD
Sample : M4304-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P067-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

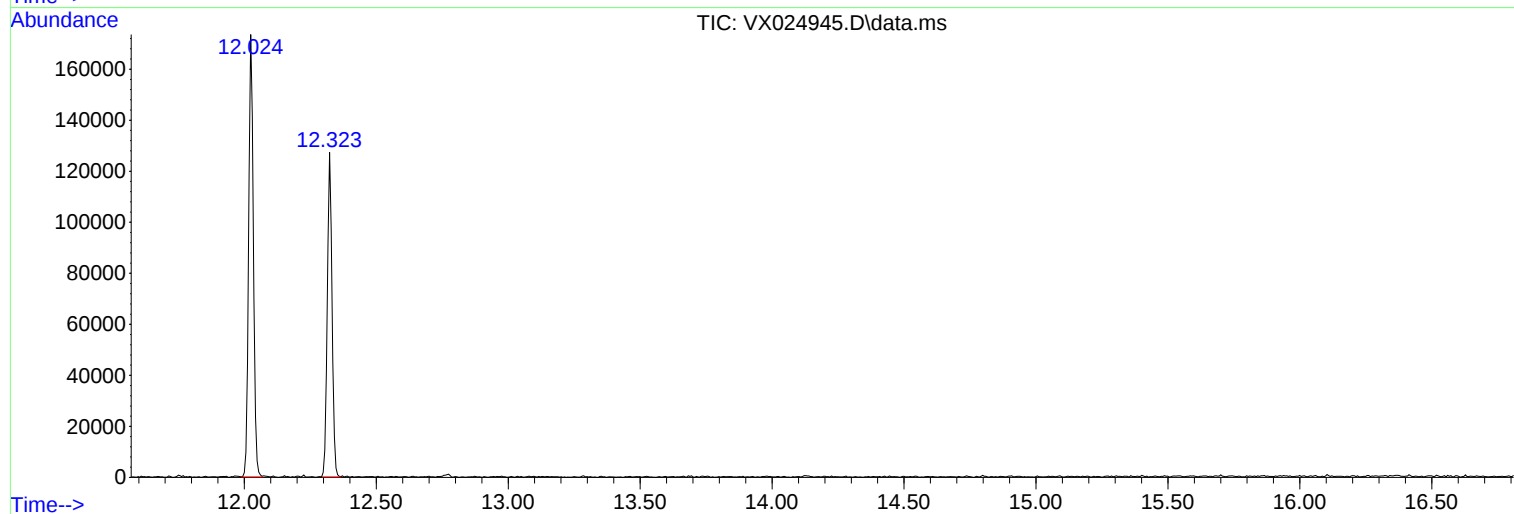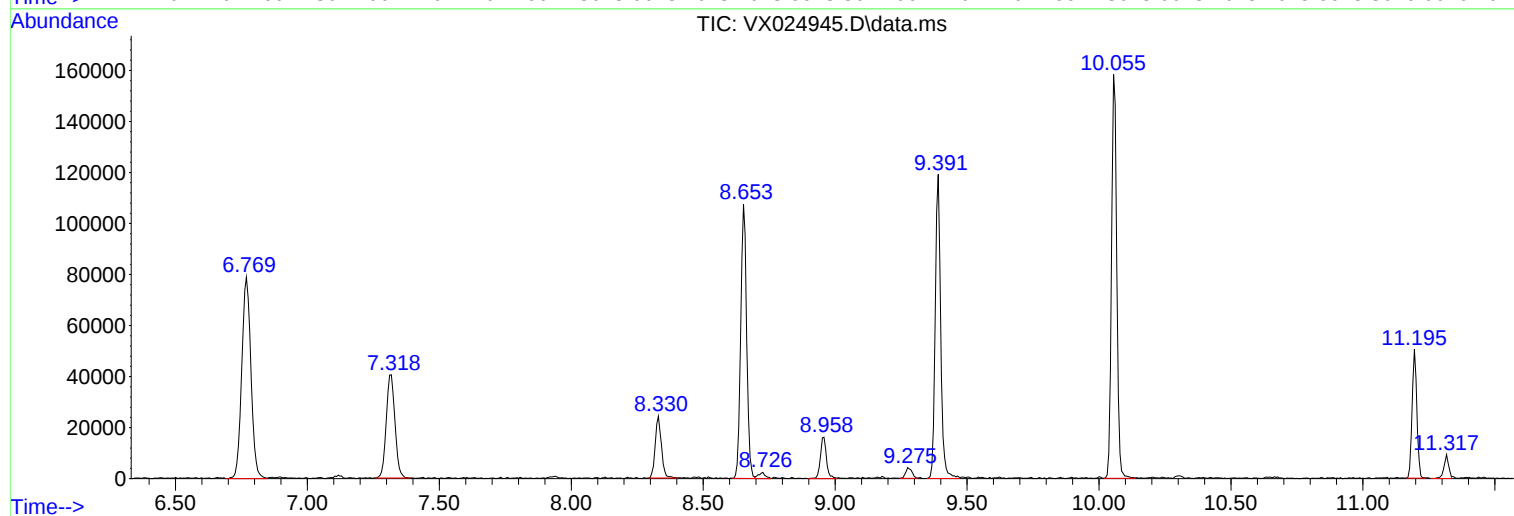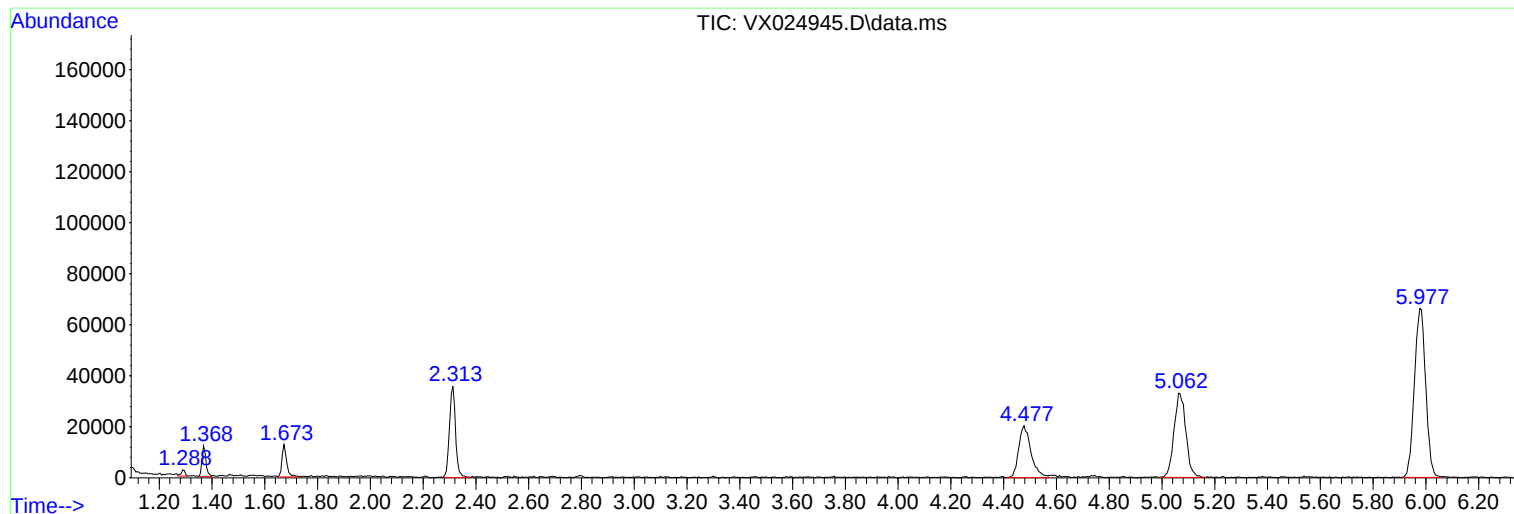

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024945.D
Acq On : 26 Oct 2021 14:48
Operator : JC/MD
Sample : M4304-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P067-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024945.D
Acq On : 26 Oct 2021 14:48
Operator : JC/MD
Sample : M4304-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P067-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
