

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024946.D
 Acq On : 26 Oct 2021 15:12
 Operator : JC/MD
 Sample : M4304-09
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P068-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	50	rBV	10810	10978	5.24%	0.613%
2	1.673	92	96	103	rVB	13007	14262	6.81%	0.797%
3	2.313	195	201	208	rVB	34390	55659	26.56%	3.110%
4	2.520	230	235	241	rBV	1217	2124	1.01%	0.119%
5	4.477	547	556	570	rBV	19393	62472	29.82%	3.491%
6	4.727	590	597	606	rVB5	4303	11803	5.63%	0.659%
7	5.062	640	652	666	rBV	35082	101463	48.43%	5.669%
8	5.977	791	802	816	rVB4	67170	194002	92.59%	10.840%
9	6.769	921	932	942	rBV2	73061	182085	86.91%	10.174%
10	7.318	1014	1022	1031	rVB2	40970	91971	43.90%	5.139%
11	8.330	1181	1188	1197	rBV2	22973	40400	19.28%	2.257%
12	8.653	1234	1241	1248	rBV	104487	165478	78.98%	9.246%
13	8.732	1248	1254	1260	rVB	2155	4362	2.08%	0.244%
14	8.952	1285	1290	1300	rBV	15963	25532	12.19%	1.427%
15	9.281	1339	1344	1353	rVB2	4464	6718	3.21%	0.375%
16	9.391	1356	1362	1371	rBV	114822	167244	79.82%	9.345%
17	10.055	1465	1471	1479	rBV	154110	209521	100.00%	11.707%
18	11.195	1653	1658	1663	rBV	48795	61689	29.44%	3.447%
19	11.317	1673	1678	1683	rVB3	8377	11459	5.47%	0.640%
20	12.024	1789	1794	1802	rBV	165306	209510	99.99%	11.706%
21	12.323	1838	1843	1851	rVB	128592	158886	75.83%	8.878%
22	12.768	1910	1916	1919	rBV2	1738	2130	1.02%	0.119%




Sum of corrected areas: 1789748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024946.D
Acq On : 26 Oct 2021 15:12
Operator : JC/MD
Sample : M4304-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P068-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

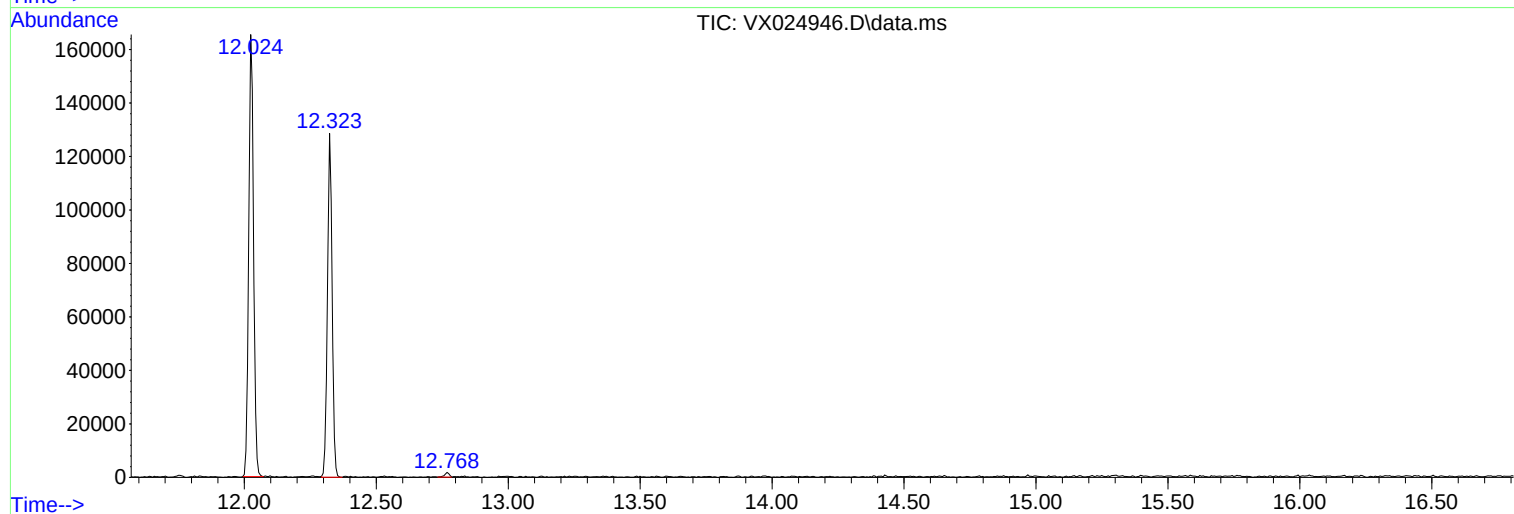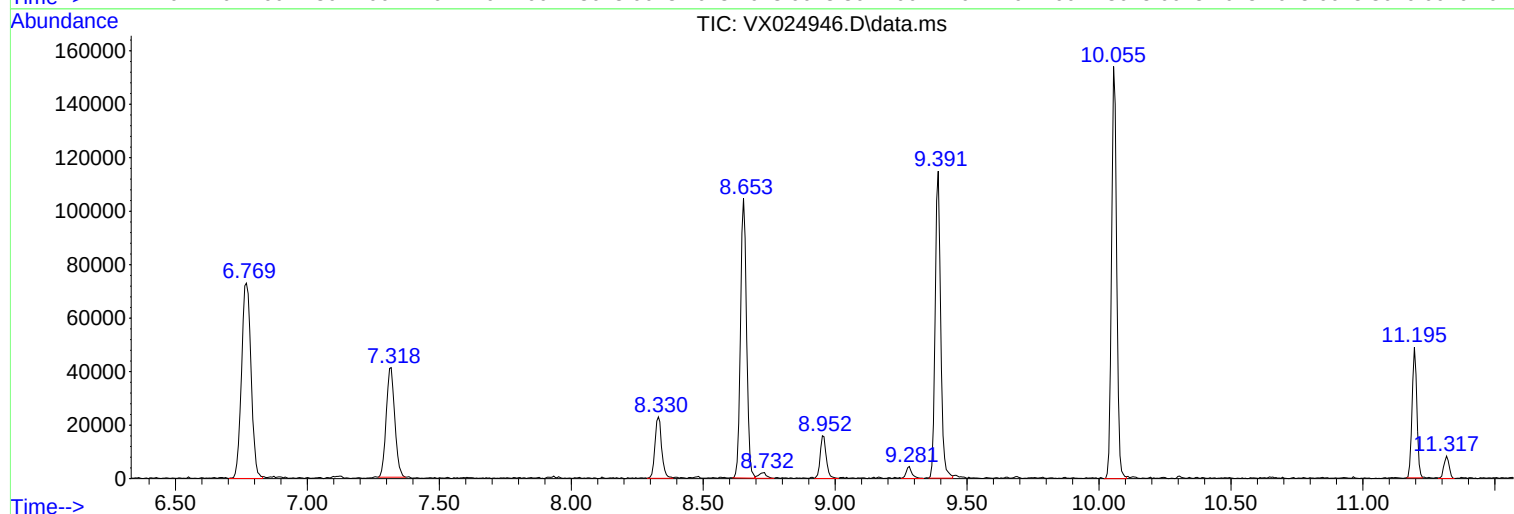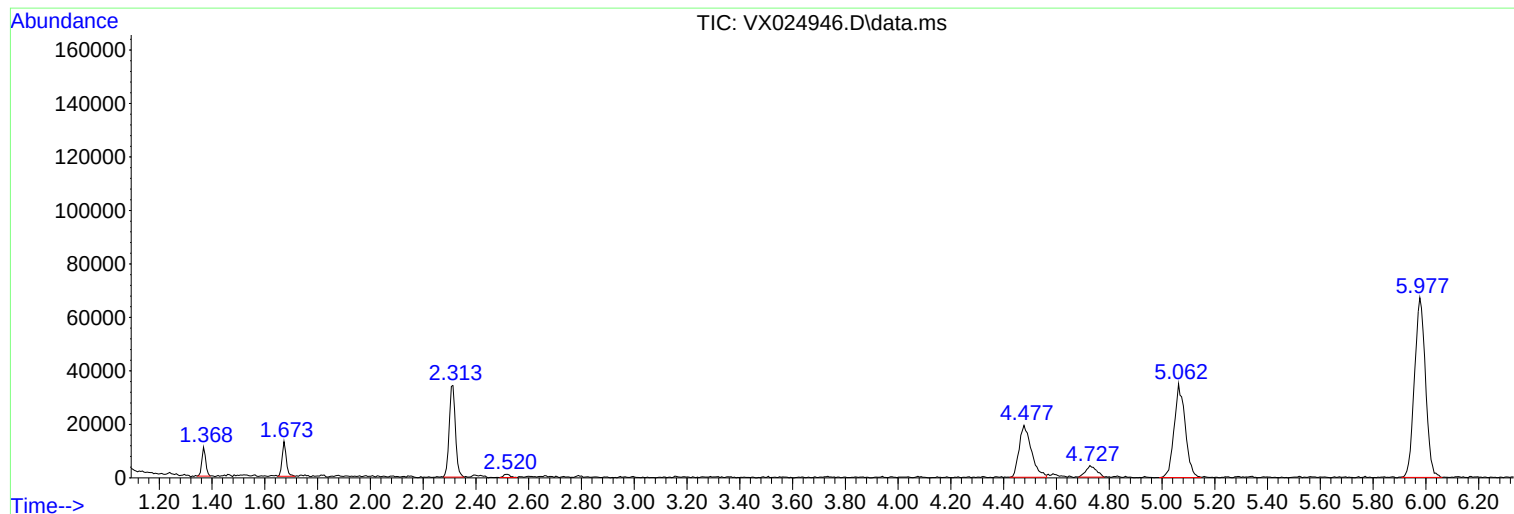

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024946.D
Acq On : 26 Oct 2021 15:12
Operator : JC/MD
Sample : M4304-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P068-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024946.D
Acq On : 26 Oct 2021 15:12
Operator : JC/MD
Sample : M4304-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P068-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
