

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024948.D
 Acq On : 26 Oct 2021 16:00
 Operator : JC/MD
 Sample : M4304-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P073-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	40	46	53	rVB	11923	12513	6.32%	0.736%
2	1.672	91	96	102	rVB	13185	14896	7.52%	0.877%
3	2.306	189	200	212	rBV	34990	58718	29.66%	3.456%
4	4.483	546	557	571	rBV	18557	62951	31.80%	3.705%
5	4.733	589	598	606	rBV4	4590	14653	7.40%	0.862%
6	5.068	640	653	665	rVB3	32468	102966	52.01%	6.060%
7	5.977	790	802	814	rBV4	66192	197990	100.00%	11.653%
8	6.769	924	932	946	rVB	62137	147745	74.62%	8.696%
9	7.312	1013	1021	1031	rVB	41313	90966	45.94%	5.354%
10	8.330	1182	1188	1194	rBV	23127	38361	19.38%	2.258%
11	8.653	1233	1241	1247	rBV	107438	168601	85.16%	9.923%
12	8.720	1250	1252	1258	rVB3	2230	2949	1.49%	0.174%
13	8.952	1284	1290	1297	rBV	16381	25256	12.76%	1.486%
14	9.281	1337	1344	1349	rBV2	3330	5670	2.86%	0.334%
15	9.391	1356	1362	1381	rBV	115368	173177	87.47%	10.193%
16	10.055	1466	1471	1478	rBV	121752	174452	88.11%	10.268%
17	11.195	1651	1658	1666	rVB	50633	64462	32.56%	3.794%
18	11.323	1675	1679	1684	rVB2	4960	7408	3.74%	0.436%
19	12.024	1789	1794	1802	rVB	136597	174388	88.08%	10.264%
20	12.323	1837	1843	1850	rVB	129273	160924	81.28%	9.471%


Sum of corrected areas: 1699046

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024948.D
Acq On : 26 Oct 2021 16:00
Operator : JC/MD
Sample : M4304-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P073-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

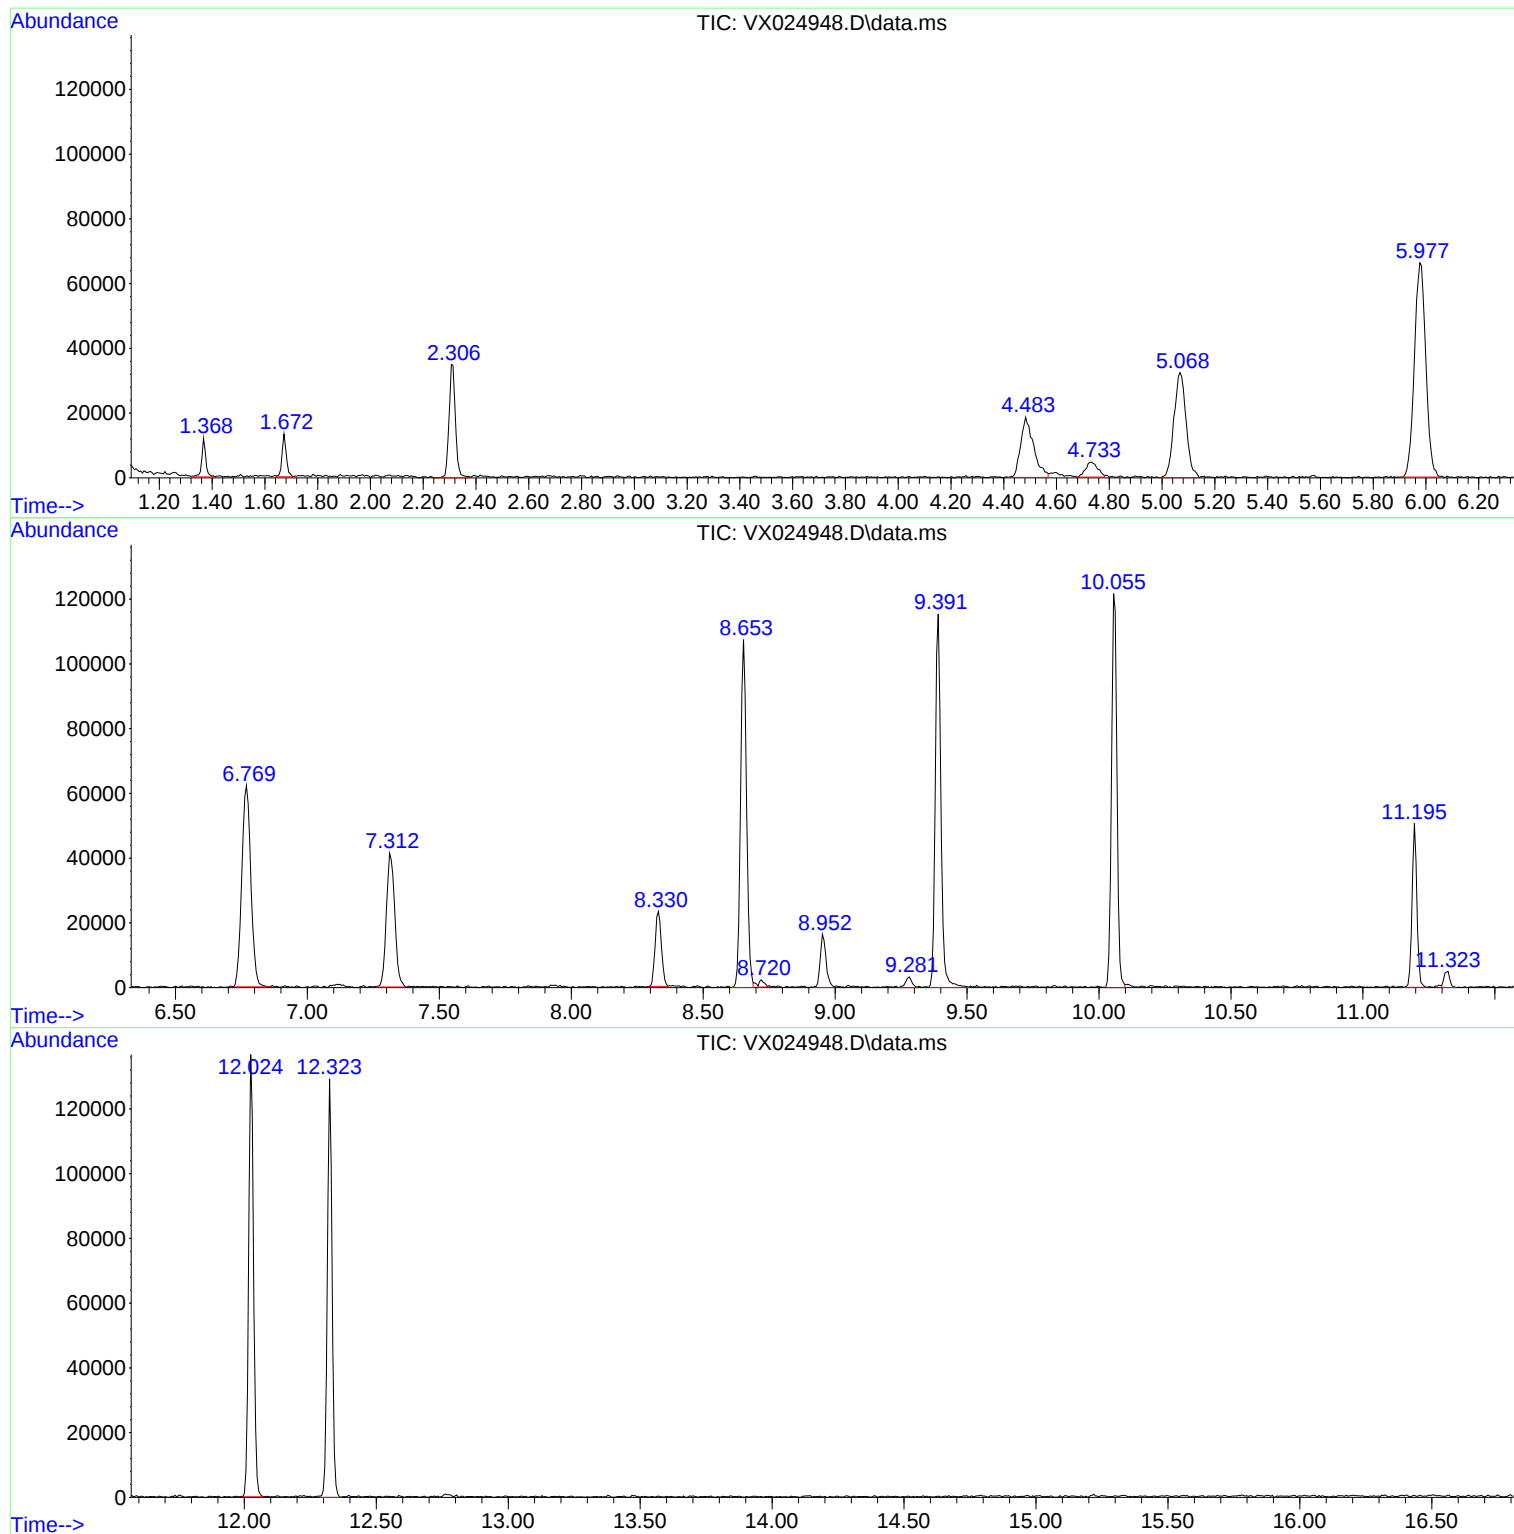

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024948.D
Acq On : 26 Oct 2021 16:00
Operator : JC/MD
Sample : M4304-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P073-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024948.D
Acq On : 26 Oct 2021 16:00
Operator : JC/MD
Sample : M4304-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P073-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
