

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024952.D
 Acq On : 26 Oct 2021 17:35
 Operator : JC/MD
 Sample : M4319-02
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P024-TW002-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	51	rBV	11788	11873	5.76%	0.674%
2	1.672	88	96	101	rBV	12695	14858	7.21%	0.843%
3	2.306	193	200	210	rBV	34837	55841	27.08%	3.170%
4	4.477	548	556	567	rBV	19900	61217	29.69%	3.475%
5	5.062	640	652	666	rBV2	31892	101824	49.38%	5.780%
6	5.977	791	802	813	rBV3	64807	191757	92.99%	10.886%
7	6.769	922	932	943	rBV3	72665	175712	85.21%	9.975%
8	7.117	982	989	993	rBV4	1164	2729	1.32%	0.155%
9	7.318	1013	1022	1031	rBV	42009	90912	44.09%	5.161%
10	8.330	1181	1188	1198	rVB2	24036	40263	19.53%	2.286%
11	8.653	1234	1241	1248	rBV	107072	165895	80.45%	9.418%
12	8.720	1249	1252	1257	rVB2	1751	3039	1.47%	0.173%
13	8.952	1284	1290	1299	rBV3	16356	25457	12.35%	1.445%
14	9.281	1338	1344	1349	rBV2	3142	5134	2.49%	0.291%
15	9.391	1353	1362	1373	rBV	117551	170882	82.87%	9.701%
16	10.055	1465	1471	1480	rBV	145860	203219	98.55%	11.537%
17	11.195	1653	1658	1666	rBV	48434	62977	30.54%	3.575%
18	11.317	1673	1678	1682	rVB4	4139	6258	3.03%	0.355%
19	12.024	1789	1794	1801	rBV	160080	206212	100.00%	11.707%
20	12.323	1836	1843	1851	rBV	130451	163274	79.18%	9.269%
21	16.371	2501	2507	2510	rBV	1637	2177	1.06%	0.124%




Sum of corrected areas: 1761510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024952.D
Acq On : 26 Oct 2021 17:35
Operator : JC/MD
Sample : M4319-02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P024-TW002-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

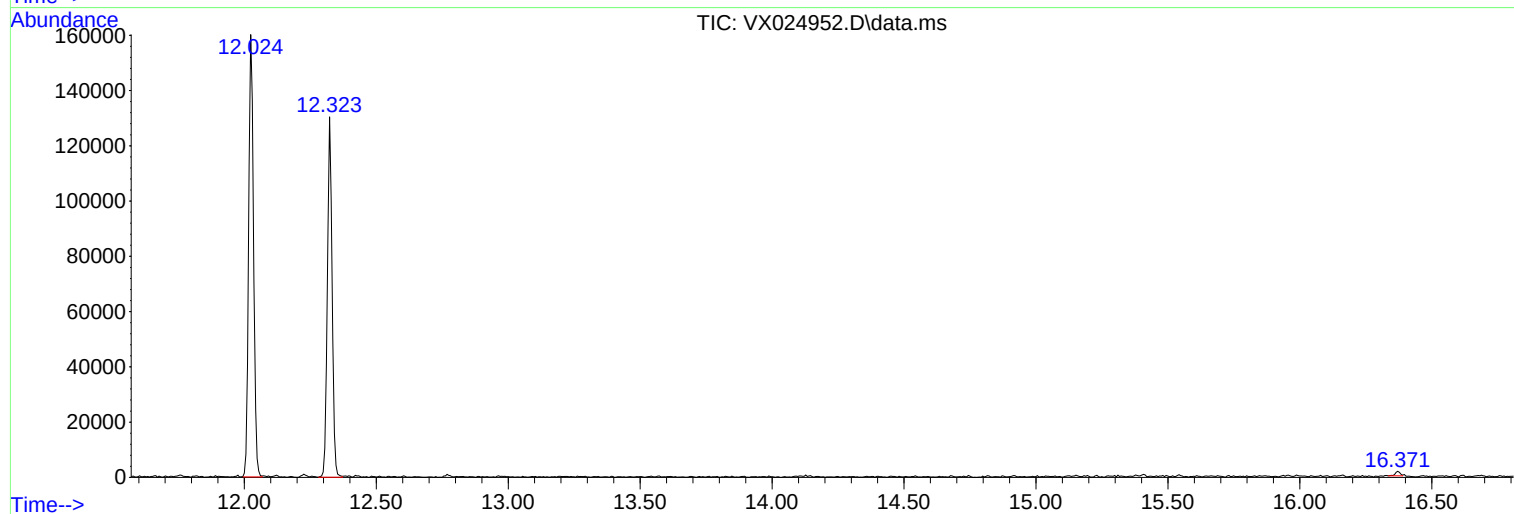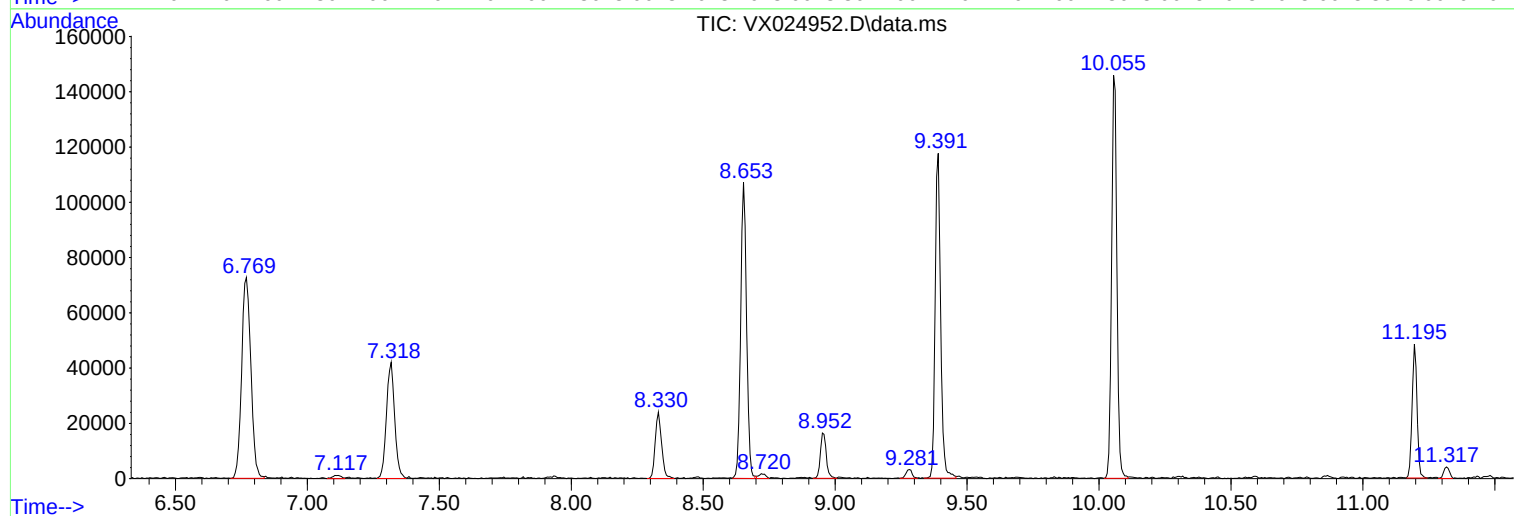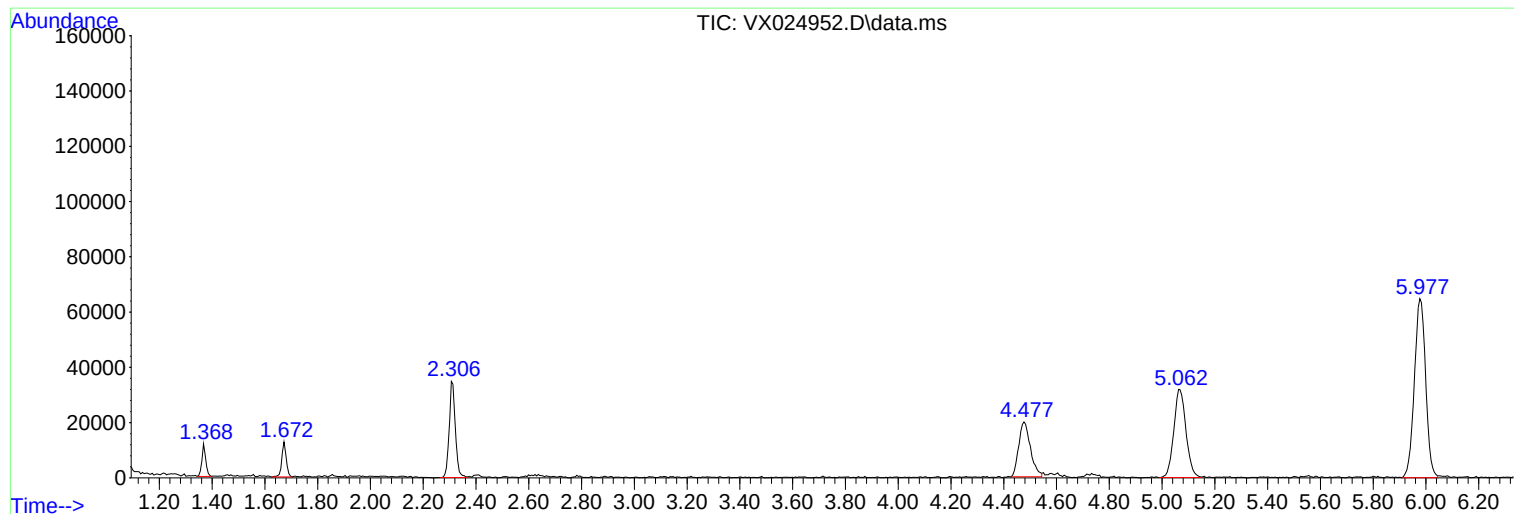

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024952.D
Acq On : 26 Oct 2021 17:35
Operator : JC/MD
Sample : M4319-02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P024-TW002-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024952.D
Acq On : 26 Oct 2021 17:35
Operator : JC/MD
Sample : M4319-02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P024-TW002-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc