

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024954.D
 Acq On : 26 Oct 2021 18:23
 Operator : JC/MD
 Sample : M4319-04
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P038-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	11	13	17	rVB	4585	4090	2.02%	0.236%
2	1.367	42	46	50	rBV	10477	10735	5.30%	0.619%
3	1.672	92	96	104	rVB	11362	14127	6.98%	0.814%
4	2.312	195	201	208	rBV	32926	53514	26.44%	3.084%
5	2.404	212	216	220	rBV4	1409	2263	1.12%	0.130%
6	4.477	547	556	568	rBV	20327	62291	30.78%	3.590%
7	4.733	590	598	602	rBV3	1500	3640	1.80%	0.210%
8	5.068	641	653	666	rBV2	30790	99172	49.00%	5.715%
9	5.976	790	802	813	rBV3	63669	188889	93.33%	10.886%
10	6.769	922	932	941	rBV2	72324	176082	87.00%	10.148%
11	7.318	1012	1022	1033	rVB	40949	90109	44.52%	5.193%
12	8.330	1182	1188	1195	rBV	23790	39810	19.67%	2.294%
13	8.653	1233	1241	1248	rBV	100982	162476	80.28%	9.364%
14	8.720	1250	1252	1259	rVB3	1745	2961	1.46%	0.171%
15	8.951	1286	1290	1297	rVB	15499	24028	11.87%	1.385%
16	9.281	1340	1344	1351	rVB2	4402	6380	3.15%	0.368%
17	9.390	1356	1362	1375	rVB	114954	167656	82.84%	9.662%
18	10.055	1466	1471	1478	rBV	143024	202384	100.00%	11.664%
19	11.195	1653	1658	1664	rBV	47874	59787	29.54%	3.446%
20	11.317	1674	1678	1683	rBV2	5385	7213	3.56%	0.416%
21	12.024	1789	1794	1803	rVB	155095	202085	99.85%	11.646%
22	12.323	1838	1843	1850	rVB	122414	155480	76.82%	8.960%


Sum of corrected areas: 1735172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024954.D
Acq On : 26 Oct 2021 18:23
Operator : JC/MD
Sample : M4319-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P038-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

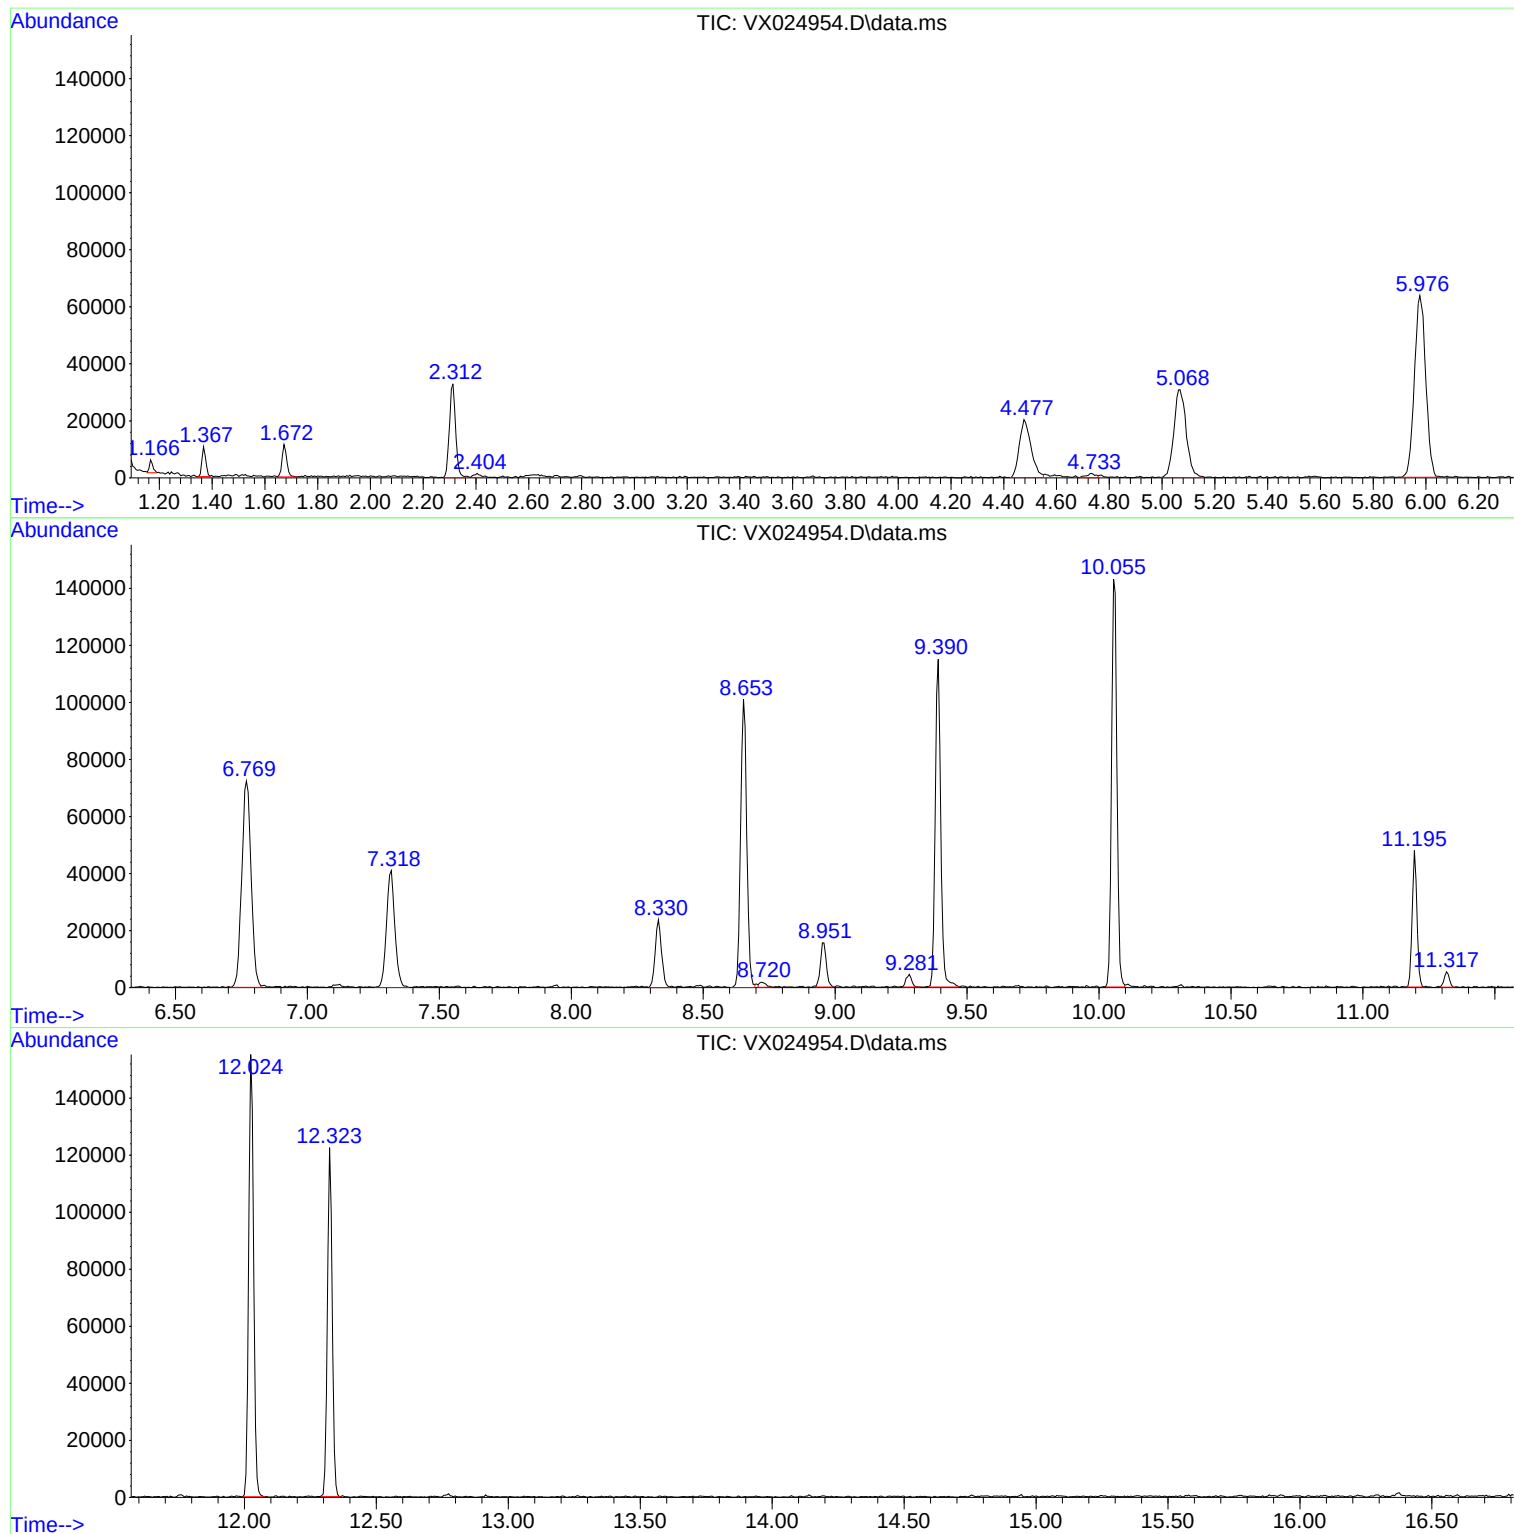

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024954.D
Acq On : 26 Oct 2021 18:23
Operator : JC/MD
Sample : M4319-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P038-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024954.D
Acq On : 26 Oct 2021 18:23
Operator : JC/MD
Sample : M4319-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P038-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
