

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024957.D
 Acq On : 26 Oct 2021 19:34
 Operator : JC/MD
 Sample : M4319-07
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P044-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	54	rVB	11107	11065	5.58%	0.624%
2	1.672	92	96	102	rVB	11783	13618	6.87%	0.768%
3	2.312	192	201	210	rBV	32311	53190	26.81%	2.998%
4	4.489	546	558	569	rBV3	22000	75089	37.85%	4.232%
5	5.062	642	652	666	rBV2	32214	97529	49.17%	5.497%
6	5.391	694	706	707	rBV2	1733	4076	2.05%	0.230%
7	5.976	792	802	814	rVB4	62057	180448	90.97%	10.170%
8	6.769	922	932	942	rBV2	70607	168794	85.09%	9.513%
9	7.135	983	992	1003	rBV3	32792	72008	36.30%	4.058%
10	7.318	1012	1022	1033	rVB3	39474	88272	44.50%	4.975%
11	8.330	1182	1188	1195	rVB2	22975	38168	19.24%	2.151%
12	8.653	1234	1241	1249	rBV	100567	156811	79.05%	8.838%
13	8.726	1249	1253	1258	rVB3	1970	3278	1.65%	0.185%
14	8.951	1286	1290	1301	rBV	15013	23304	11.75%	1.313%
15	9.281	1340	1344	1350	rVB2	4260	5975	3.01%	0.337%
16	9.390	1356	1362	1373	rBV	114730	164129	82.74%	9.250%
17	10.055	1465	1471	1478	rBV	143013	197473	99.55%	11.130%
18	11.195	1653	1658	1666	rVB	47020	60423	30.46%	3.405%
19	11.317	1672	1678	1684	rVB2	6814	9085	4.58%	0.512%
20	12.024	1789	1794	1801	rBV	156328	198368	100.00%	11.180%
21	12.323	1838	1843	1852	rBV	116315	153192	77.23%	8.634%




Sum of corrected areas: 1774295

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024957.D
Acq On : 26 Oct 2021 19:34
Operator : JC/MD
Sample : M4319-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P044-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

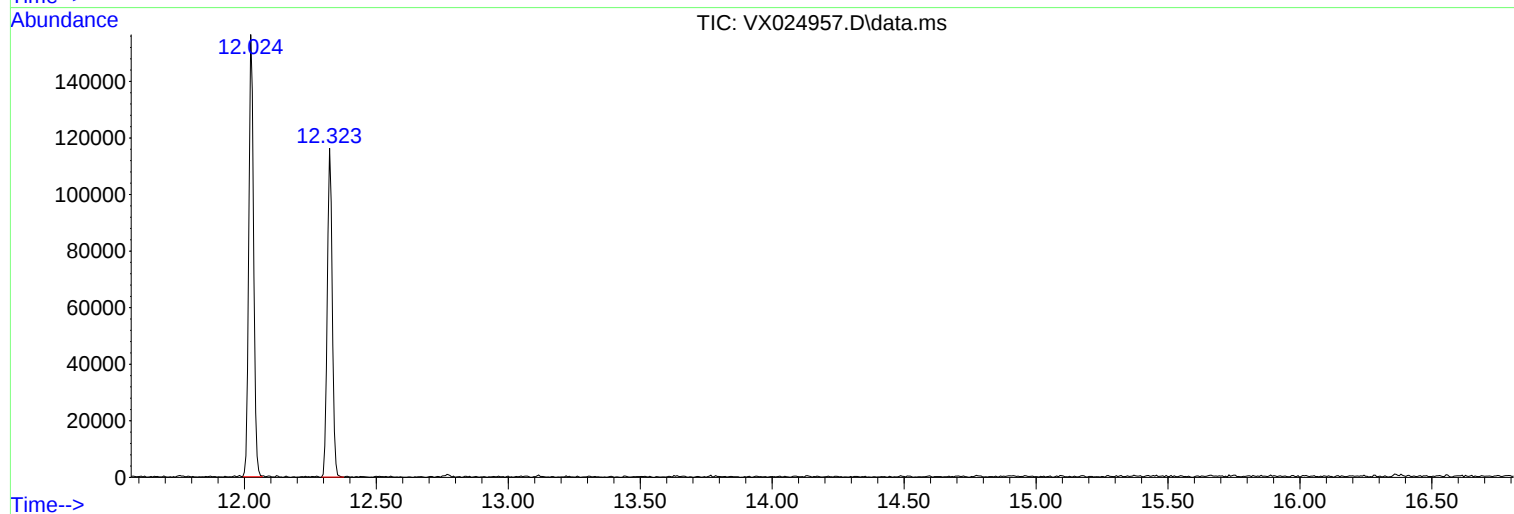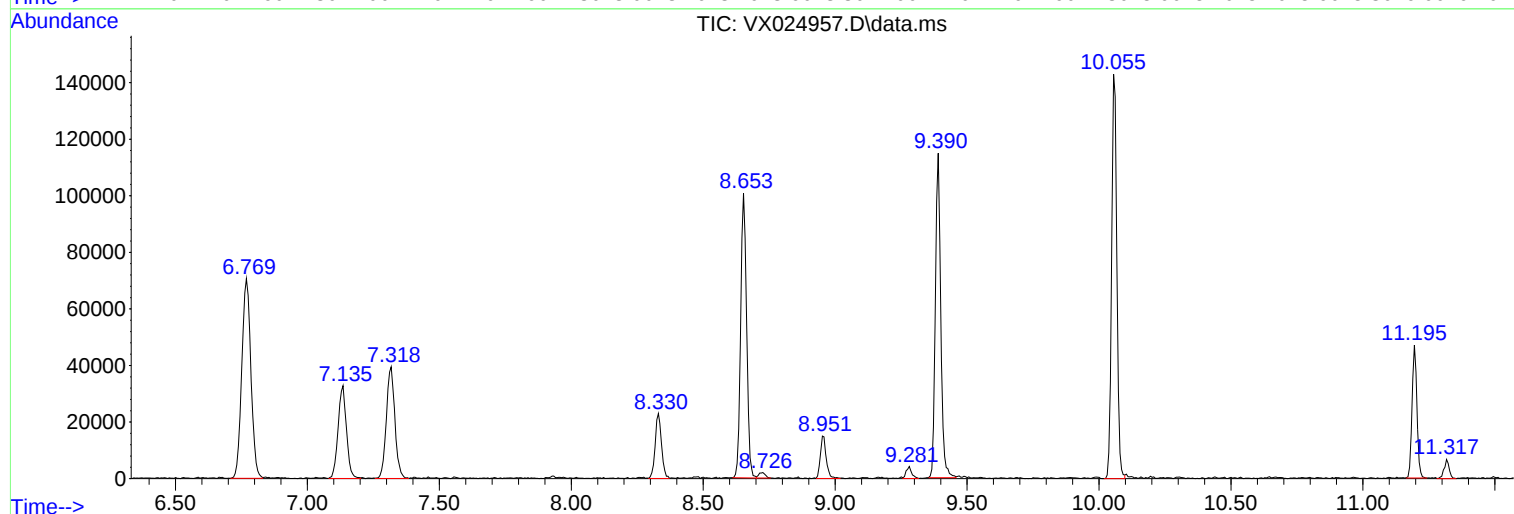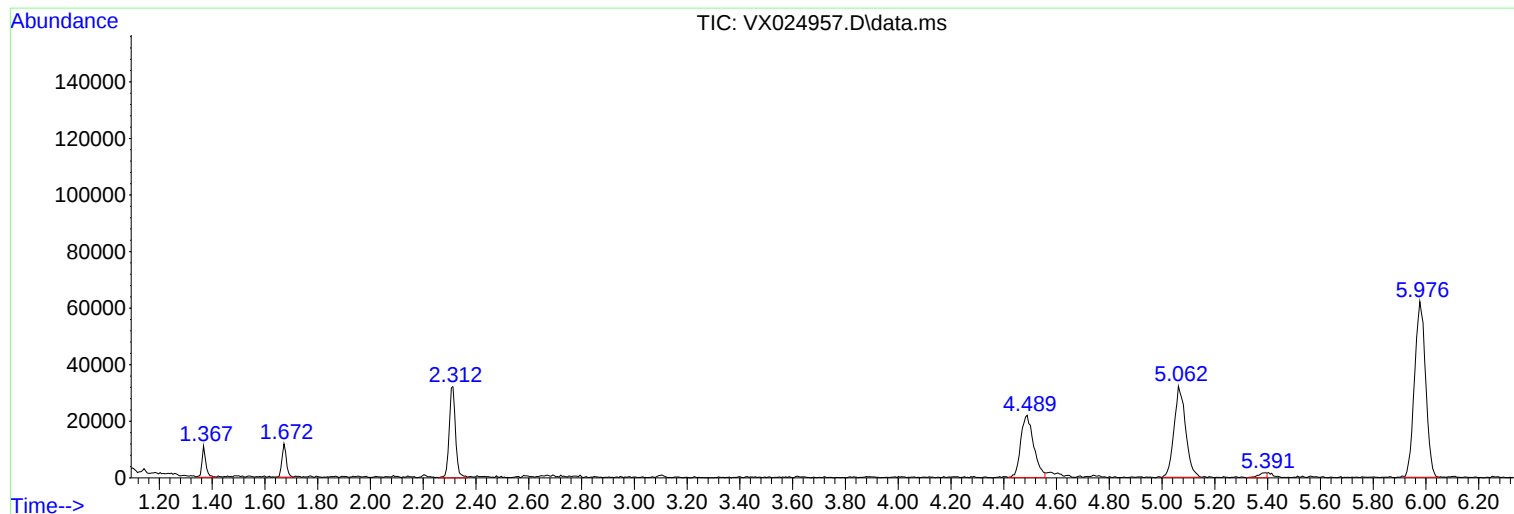

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024957.D
Acq On : 26 Oct 2021 19:34
Operator : JC/MD
Sample : M4319-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P044-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024957.D
Acq On : 26 Oct 2021 19:34
Operator : JC/MD
Sample : M4319-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P044-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
