

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024958.D
 Acq On : 26 Oct 2021 19:58
 Operator : JC/MD
 Sample : M4319-08
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P051-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	51	rVB	11830	11415	5.54%	0.664%
2	1.672	92	96	101	rBV	11313	13401	6.50%	0.779%
3	2.312	194	201	209	rBV	35789	55539	26.94%	3.229%
4	4.477	547	556	568	rBV2	18194	61493	29.83%	3.575%
5	5.068	641	653	667	rBV2	32263	98940	47.99%	5.752%
6	5.976	789	802	818	rBV4	61098	185918	90.17%	10.808%
7	6.769	922	932	944	rBV	73322	176933	85.82%	10.286%
8	7.318	1011	1022	1032	rBV2	40883	88756	43.05%	5.160%
9	8.330	1182	1188	1199	rBV	23790	40046	19.42%	2.328%
10	8.653	1234	1241	1249	rBV	103109	158692	76.97%	9.225%
11	8.726	1249	1253	1258	rVB	3063	3694	1.79%	0.215%
12	8.951	1284	1290	1299	rBV2	13628	23288	11.30%	1.354%
13	9.275	1338	1343	1351	rVB2	2627	4601	2.23%	0.267%
14	9.390	1356	1362	1369	rBV	112020	166847	80.92%	9.699%
15	10.055	1465	1471	1479	rBV	152499	206178	100.00%	11.986%
16	11.195	1653	1658	1664	rBV2	46390	60581	29.38%	3.522%
17	11.317	1674	1678	1682	rVB3	5193	6417	3.11%	0.373%
18	12.024	1786	1794	1802	rBV	158361	204035	98.96%	11.861%
19	12.323	1838	1843	1850	rBV	120546	153413	74.41%	8.918%




Sum of corrected areas: 1720187

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024958.D
Acq On : 26 Oct 2021 19:58
Operator : JC/MD
Sample : M4319-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P051-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

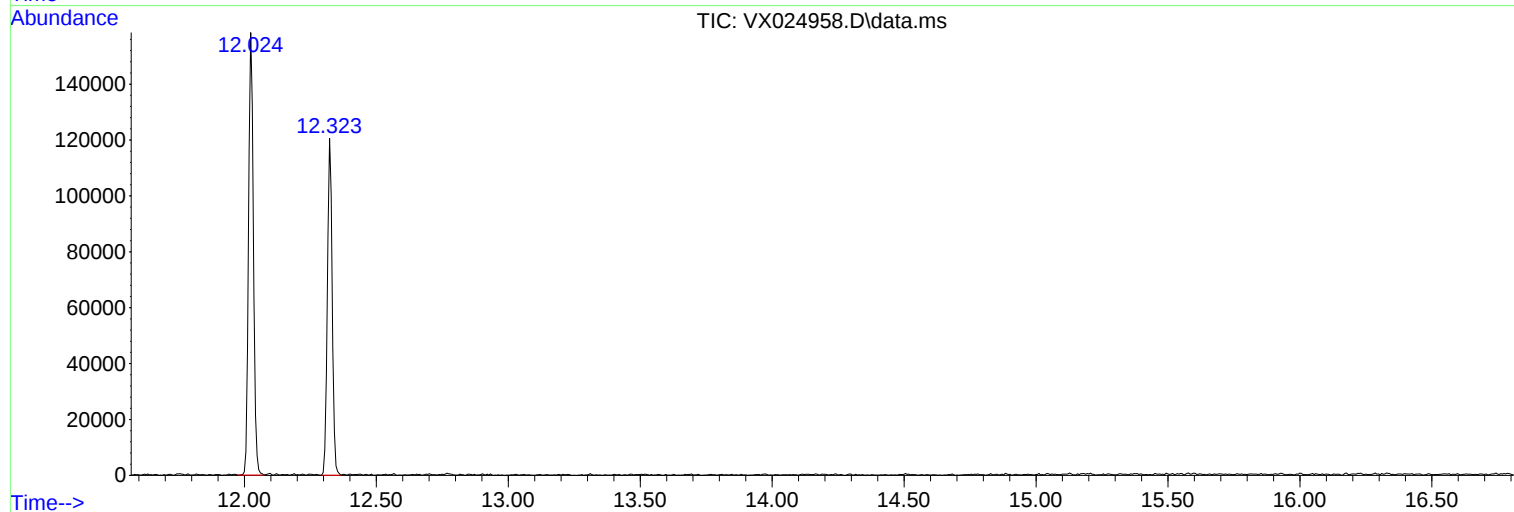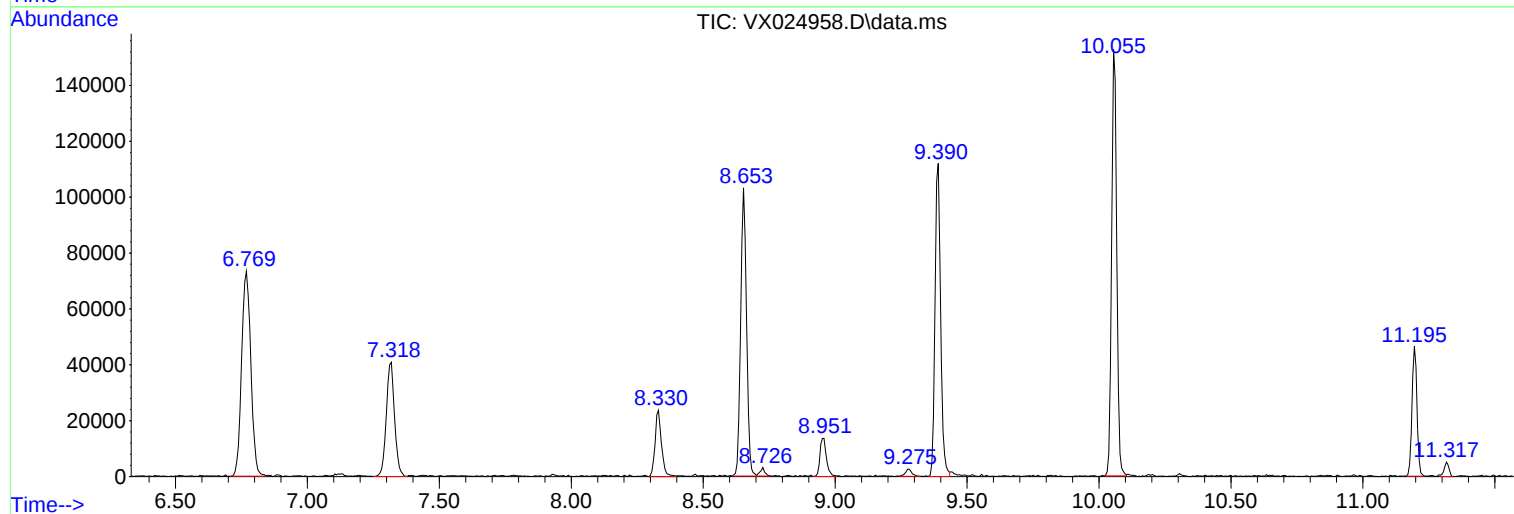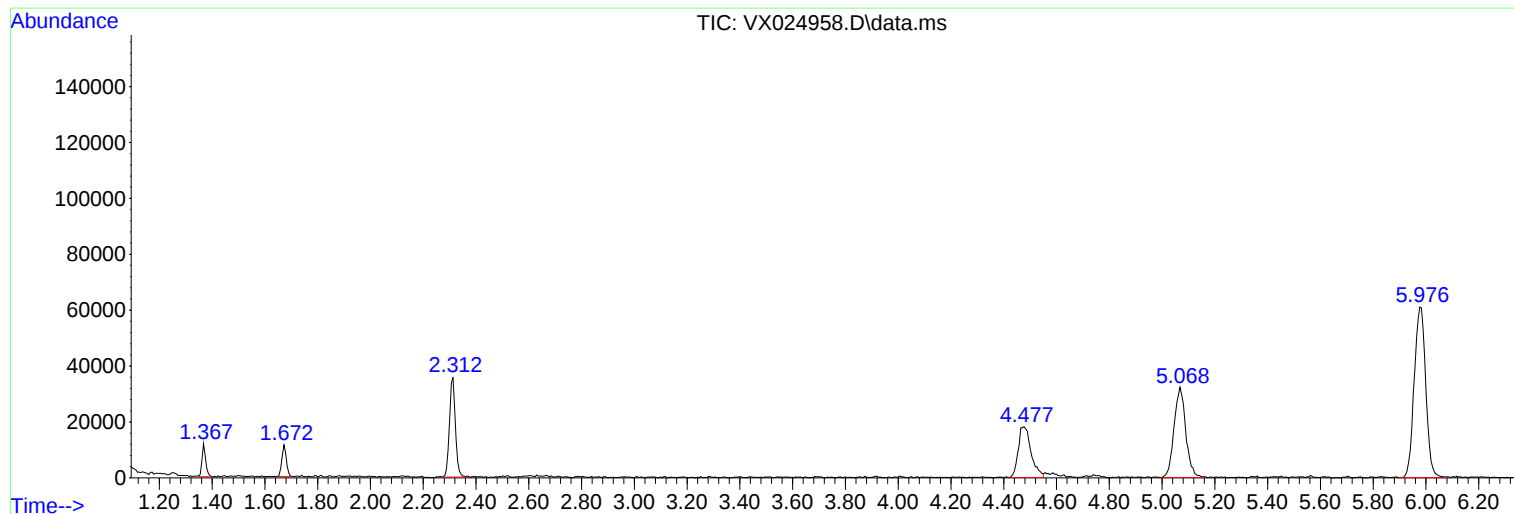

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024958.D
Acq On : 26 Oct 2021 19:58
Operator : JC/MD
Sample : M4319-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P051-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024958.D
Acq On : 26 Oct 2021 19:58
Operator : JC/MD
Sample : M4319-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P051-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc