

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024960.D
 Acq On : 26 Oct 2021 20:46
 Operator : JC/MD
 Sample : M4319-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P058-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024960.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	10929	11097	5.27%	0.649%
2	1.672	91	96	103	rVB	11069	14397	6.83%	0.842%
3	2.313	192	201	209	rBV	34035	54605	25.91%	3.192%
4	4.477	548	556	569	rBV	16924	58045	27.54%	3.394%
5	4.605	575	577	590	rVB4	2176	3974	1.89%	0.232%
6	5.068	641	653	666	rBV2	31652	97795	46.40%	5.718%
7	5.977	792	802	815	rVB3	61554	181024	85.89%	10.583%
8	6.769	921	932	942	rBV3	74164	175237	83.15%	10.245%
9	7.318	1012	1022	1031	rBV	39121	87122	41.34%	5.094%
10	8.330	1182	1188	1194	rBV3	20665	37230	17.66%	2.177%
11	8.653	1234	1241	1249	rBV	99206	156678	74.34%	9.160%
12	8.714	1249	1251	1258	rVB3	1607	2715	1.29%	0.159%
13	8.958	1284	1291	1297	rBV	16234	23839	11.31%	1.394%
14	9.281	1339	1344	1349	rBV2	4033	5817	2.76%	0.340%
15	9.391	1354	1362	1374	rBV	113210	166077	78.80%	9.710%
16	10.055	1466	1471	1478	rBV	150529	207939	98.66%	12.157%
17	11.195	1652	1658	1666	rBV2	47621	60705	28.80%	3.549%
18	11.317	1673	1678	1684	rBV4	4376	6954	3.30%	0.407%
19	12.024	1788	1794	1803	rBV	165955	210758	100.00%	12.322%
20	12.323	1838	1843	1851	rVB	113806	148439	70.43%	8.678%




Sum of corrected areas: 1710447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024960.D
Acq On : 26 Oct 2021 20:46
Operator : JC/MD
Sample : M4319-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P058-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

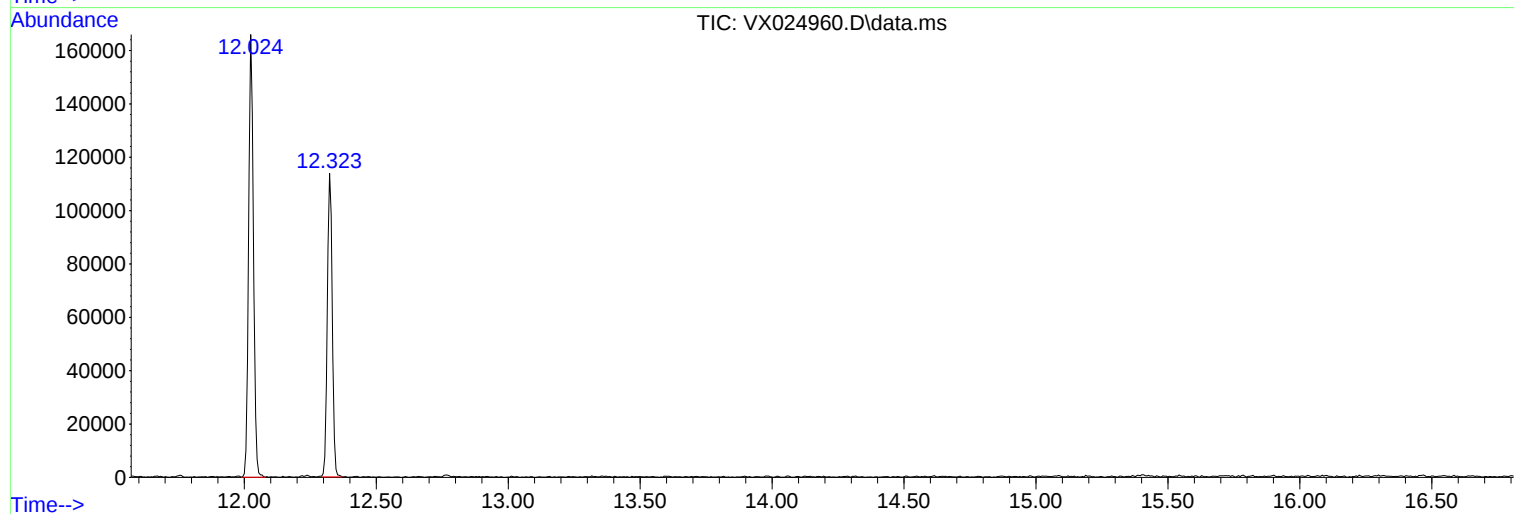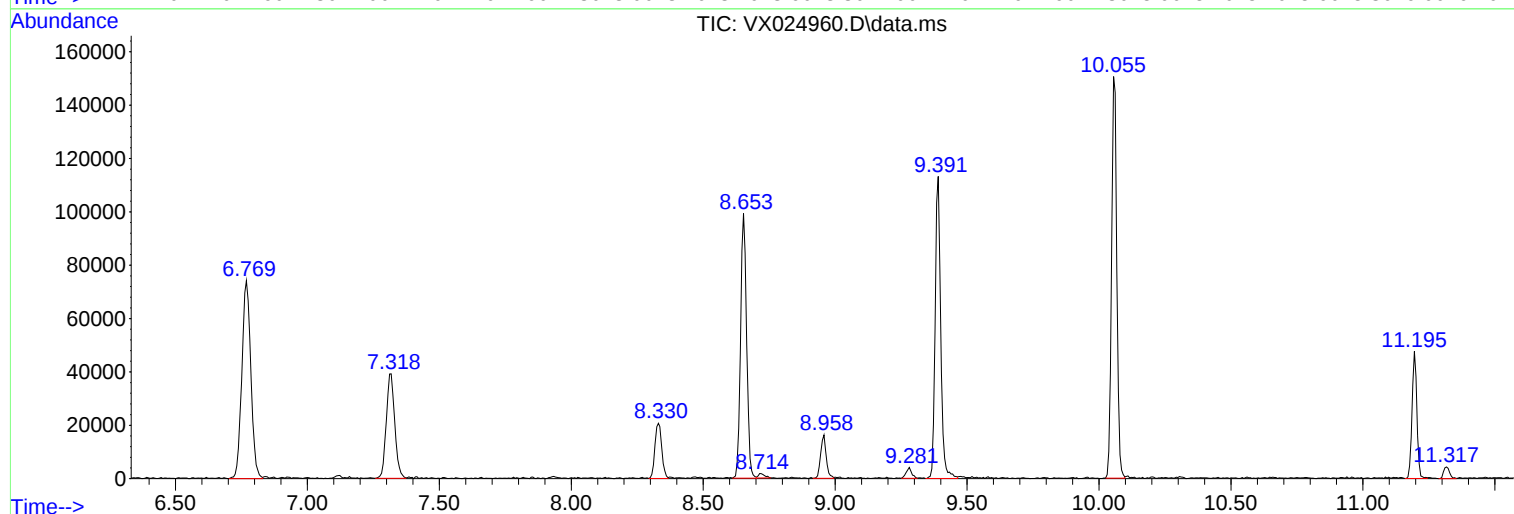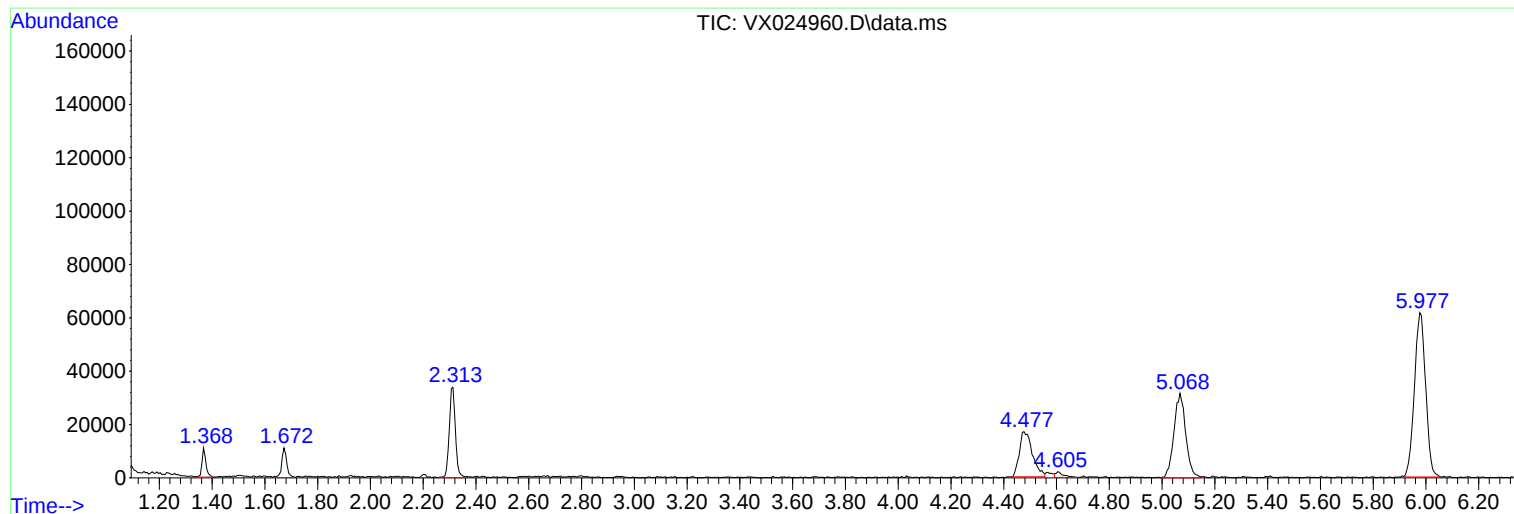

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024960.D
Acq On : 26 Oct 2021 20:46
Operator : JC/MD
Sample : M4319-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P058-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
Data File : VX024960.D
Acq On : 26 Oct 2021 20:46
Operator : JC/MD
Sample : M4319-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P058-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
