
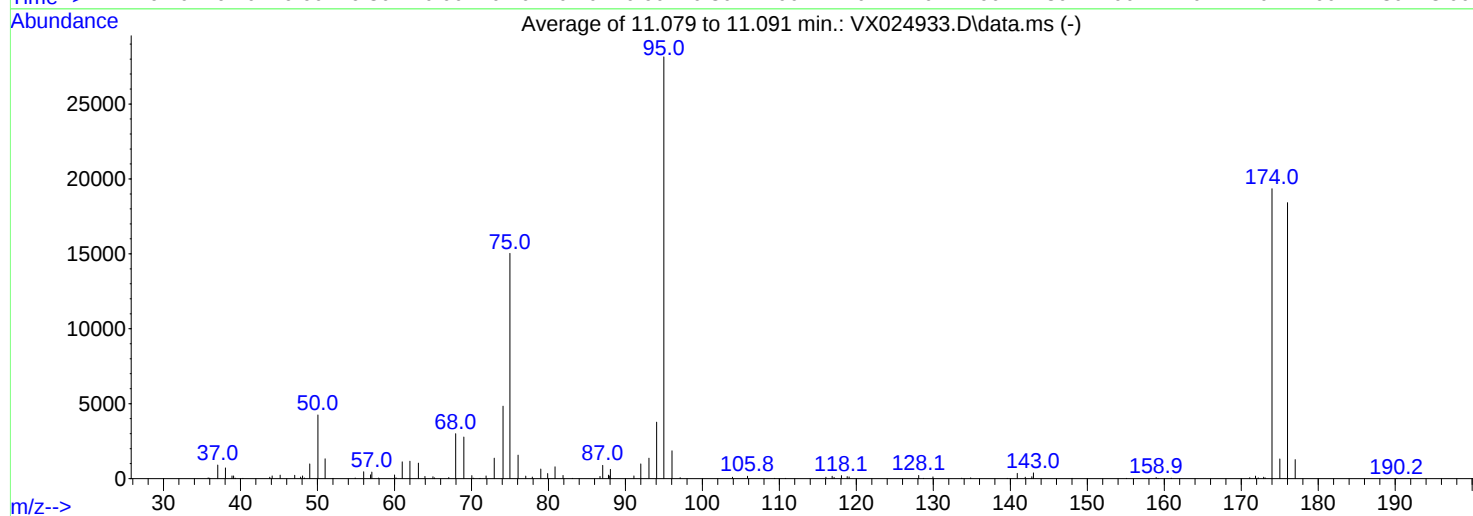


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102621\
 Data File : VX024933.D
 Acq On : 26 Oct 2021 09:41
 Operator : JC/MD
 Sample : BFB610
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB610

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Oct 28 03:09:30 2021

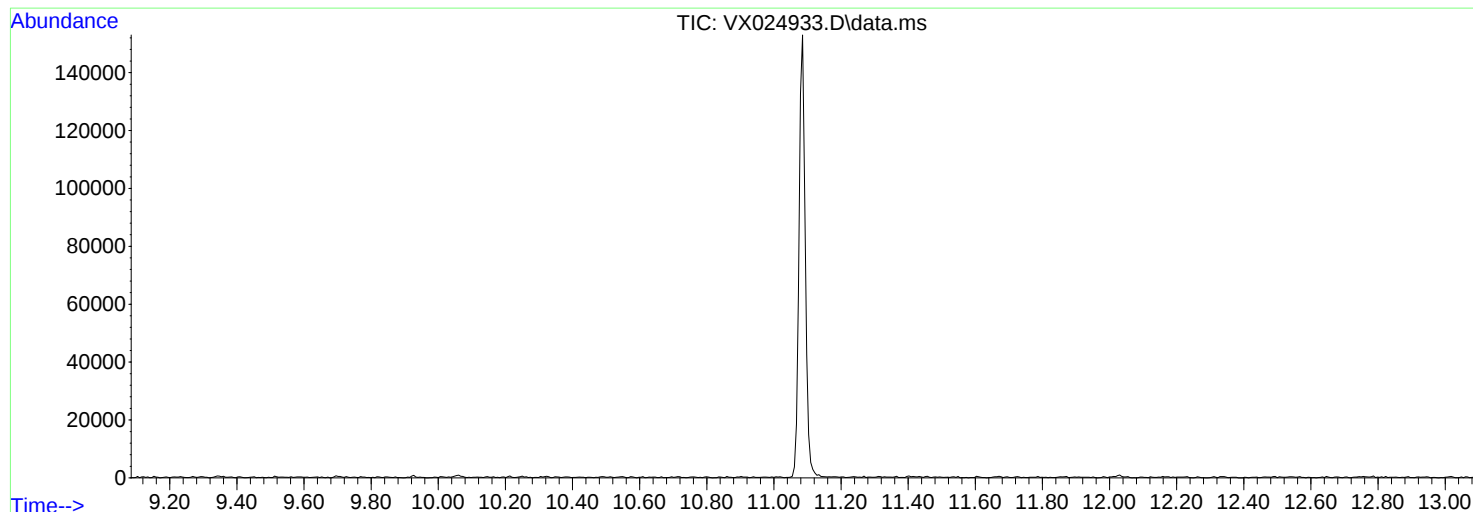

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	4254	PASS
75	95	30	80	53.4	15032	PASS
95	95	100	100	100.0	28147	PASS
96	95	5	9	6.6	1863	PASS
173	174	0.00	2	0.5	96	PASS
174	95	50	120	68.7	19344	PASS
175	174	5	9	6.8	1315	PASS
176	174	95	105	95.2	18415	PASS
177	176	5	10	6.9	1273	PASS

m/z	Abundance
38.30	56.0
39.90	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610

m/z	Abundance
37.10	1068.0
38.00	680.0
38.90	283.0
44.10	197.0
45.10	303.0
47.10	366.0
47.80	328.0
48.30	142.0
49.00	956.0
50.00	5014.0
51.00	1247.0
56.00	546.0
56.90	769.0
57.90	74.0
60.00	339.0
61.10	1370.0
62.10	1237.0
63.20	1139.0
63.90	134.0
65.00	280.0
67.00	124.0
68.00	3012.0
69.00	3118.0
70.00	374.0
71.90	240.0
73.00	1562.0
74.10	5480.0
75.00	15714.0
76.00	2079.0
77.00	110.0
79.00	734.0
79.90	259.0
80.90	1212.0
81.90	234.0
83.10	67.0
87.00	1055.0
87.80	703.0
88.10	798.0
91.10	283.0
92.00	1185.0
93.10	1518.0
94.10	4338.0
95.00	29752.0
96.20	1753.0
105.80	200.0
116.10	62.0
116.80	261.0
118.10	181.0
118.80	216.0
119.10	232.0
128.10	158.0
129.80	97.0
134.80	81.0
140.90	272.0
142.00	128.0
142.80	389.0
155.10	72.0
158.90	138.0
171.10	59.0
172.00	166.0
172.90	288.0
174.00	17728.0
175.00	1183.0
176.00	17008.0
177.00	1463.0
190.20	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610

m/z	Abundance
35.80	155.0
37.10	1023.0
38.10	819.0
39.10	544.0
44.10	338.0
45.20	253.0
46.90	219.0
48.00	273.0
49.00	1329.0
50.10	4960.0
51.00	1624.0
52.00	55.0
55.00	75.0
56.00	471.0
57.10	868.0
58.00	55.0
60.00	398.0
60.90	1054.0
61.90	1583.0
63.00	1415.0
64.00	218.0
65.20	156.0
67.10	115.0
68.00	3582.0
69.00	3016.0
70.10	228.0
71.90	299.0
73.00	1550.0
74.10	5696.0
75.00	19080.0
76.10	1687.0
77.00	239.0
78.00	196.0
79.00	715.0
79.90	527.0
80.80	781.0
81.90	291.0
87.10	1239.0
88.00	1053.0
91.10	173.0
91.90	1058.0
93.00	1595.0
94.00	4192.0
95.00	32824.0
96.00	2298.0
97.10	186.0
103.90	173.0
105.90	196.0
109.40	56.0
116.00	138.0
117.10	266.0
118.10	299.0
118.80	216.0
128.00	330.0
129.90	70.0
134.90	71.0
140.90	496.0
141.90	166.0
143.00	625.0
148.00	78.0
159.00	81.0
171.10	137.0
171.80	191.0
174.00	23744.0
175.00	1562.0
176.00	22072.0
177.00	1520.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610

m/z	Abundance
36.00	83.0
36.90	621.0
38.00	654.0
38.90	278.0
39.30	106.0
40.30	68.0
43.80	304.0
45.10	139.0
47.00	79.0
48.10	259.0
49.10	662.0
50.10	2787.0
51.00	1107.0
54.80	64.0
56.00	347.0
57.00	443.0
60.20	175.0
61.00	934.0
62.00	660.0
63.20	539.0
63.90	89.0
65.00	116.0
67.90	2421.0
69.00	2204.0
70.30	97.0
71.10	57.0
72.80	973.0
74.00	3319.0
75.00	10303.0
76.10	954.0
77.10	154.0
77.80	128.0
79.00	477.0
79.90	227.0
80.90	386.0
82.00	112.0
86.70	452.0
87.10	378.0
87.90	555.0
91.10	92.0
92.10	712.0
93.00	1002.0
94.10	2771.0
95.00	21864.0
96.00	1538.0
103.90	104.0
105.90	96.0
110.80	51.0
116.00	83.0
116.90	214.0
117.90	135.0
119.00	117.0
128.20	154.0
128.70	53.0
130.00	172.0
133.70	83.0
139.60	59.0
140.90	285.0
143.00	533.0
159.20	81.0
160.90	85.0
171.70	142.0
172.20	157.0
173.10	175.0
174.00	16560.0
175.00	1199.0
176.00	16164.0
177.10	836.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610