
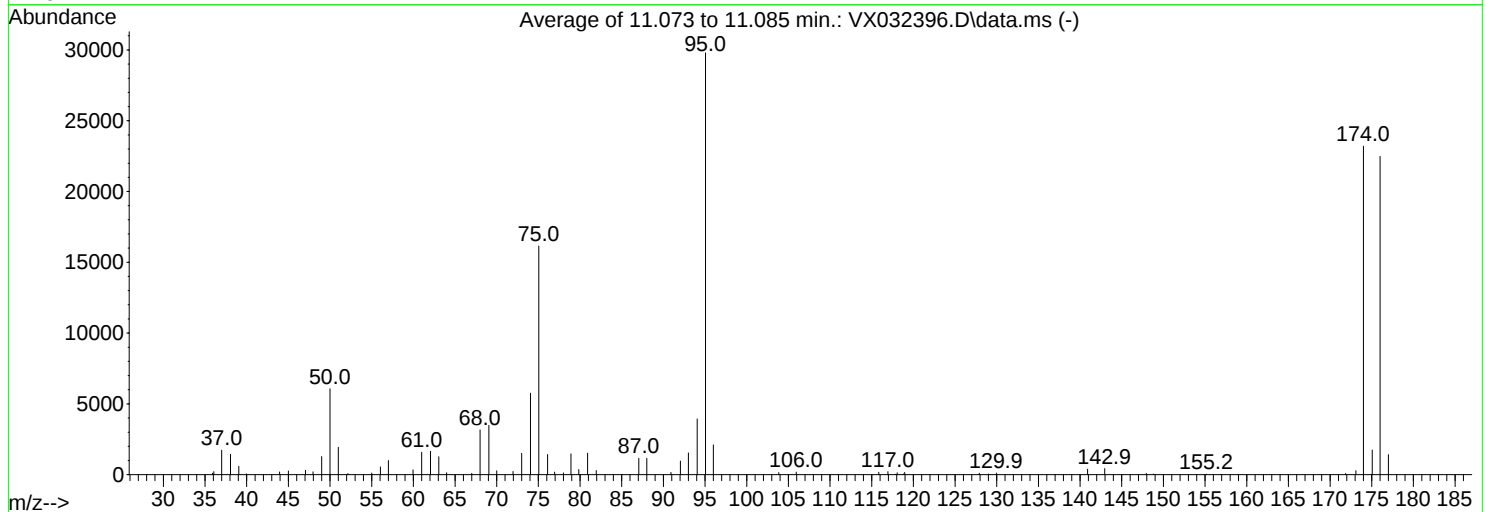


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102622\  
 Data File : VX032396.D  
 Acq On : 26 Oct 2022 09:26  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X102622W.M  
 Title : SW846 8260  
 Last Update : Thu Oct 27 08:28:06 2022

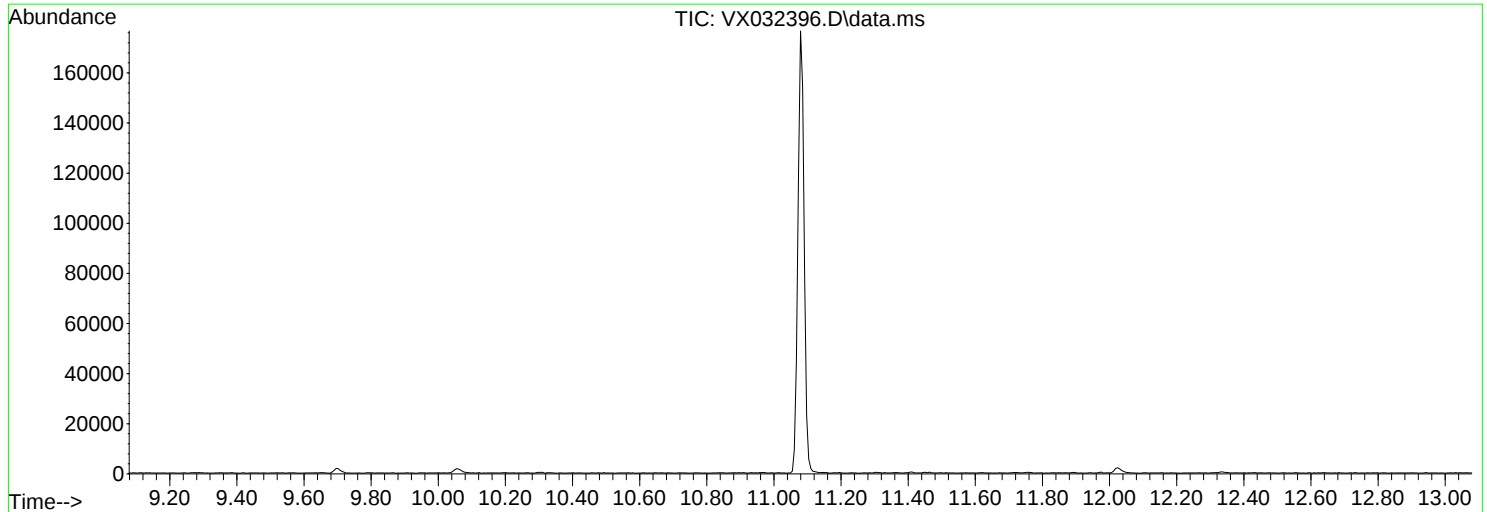

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.4         | 6068       | PASS                |
| 75             | 95              | 30              | 60              | 54.2         | 16147      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 29795      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 2097       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 282        | PASS                |
| 174            | 95              | 50              | 100             | 77.9         | 23207      | PASS                |
| 175            | 174             | 5               | 9               | 7.5          | 1745       | PASS                |
| 176            | 174             | 95              | 101             | 96.9         | 22485      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 1411       | PASS                |