

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038523.D
Acq On : 26 Oct 2023 17:19
Operator : JC/MD
Sample : 05063-03 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	547	559	582	rBV	262279	741327	68.19%	10.250%
2	5.385	691	705	722	rBV2	133017	392735	36.12%	5.430%
3	5.556	722	733	754	rVV	186908	541657	49.82%	7.489%
4	5.958	787	799	816	rBV2	136678	361772	33.28%	5.002%
5	6.763	918	931	951	rBV	298026	715315	65.79%	9.890%
6	7.123	982	990	1009	rBV	249732	557704	51.30%	7.711%
7	8.647	1234	1240	1251	rBV	665393	1087191	100.00%	15.032%
8	10.055	1465	1471	1489	rBV	704048	946016	87.01%	13.080%
9	11.079	1634	1639	1653	rBV	631696	845029	77.73%	11.684%
10	12.024	1788	1794	1807	rBV	827340	1043889	96.02%	14.433%




Sum of corrected areas: 7232635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038523.D
Acq On : 26 Oct 2023 17:19
Operator : JC/MD
Sample : 05063-03 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

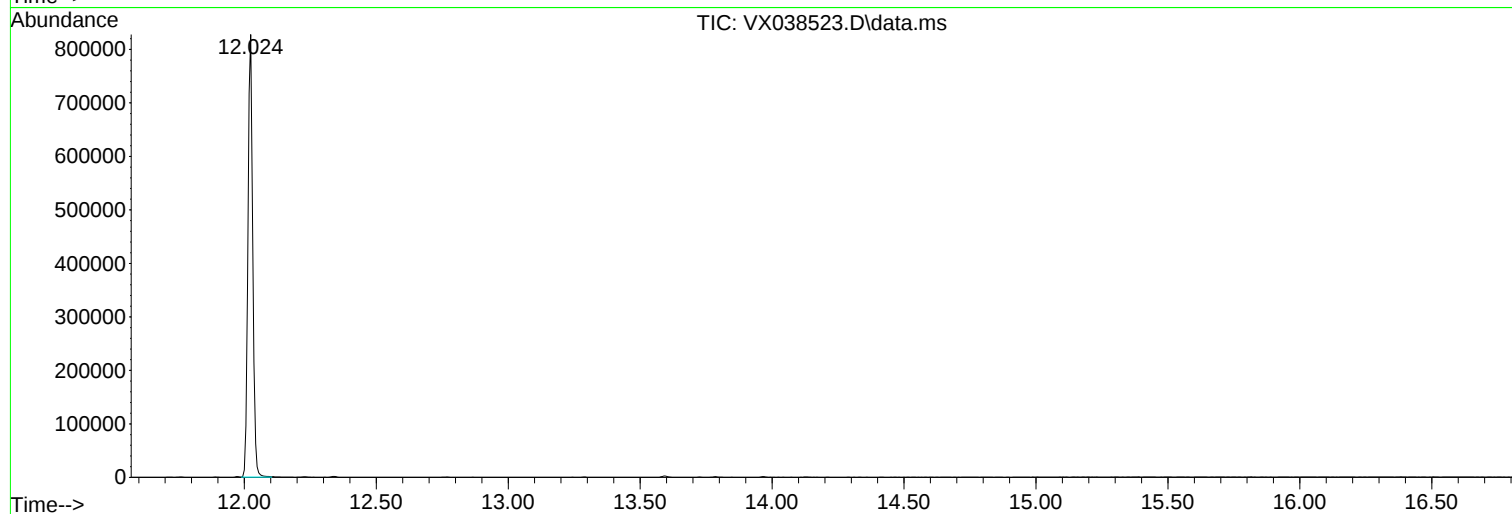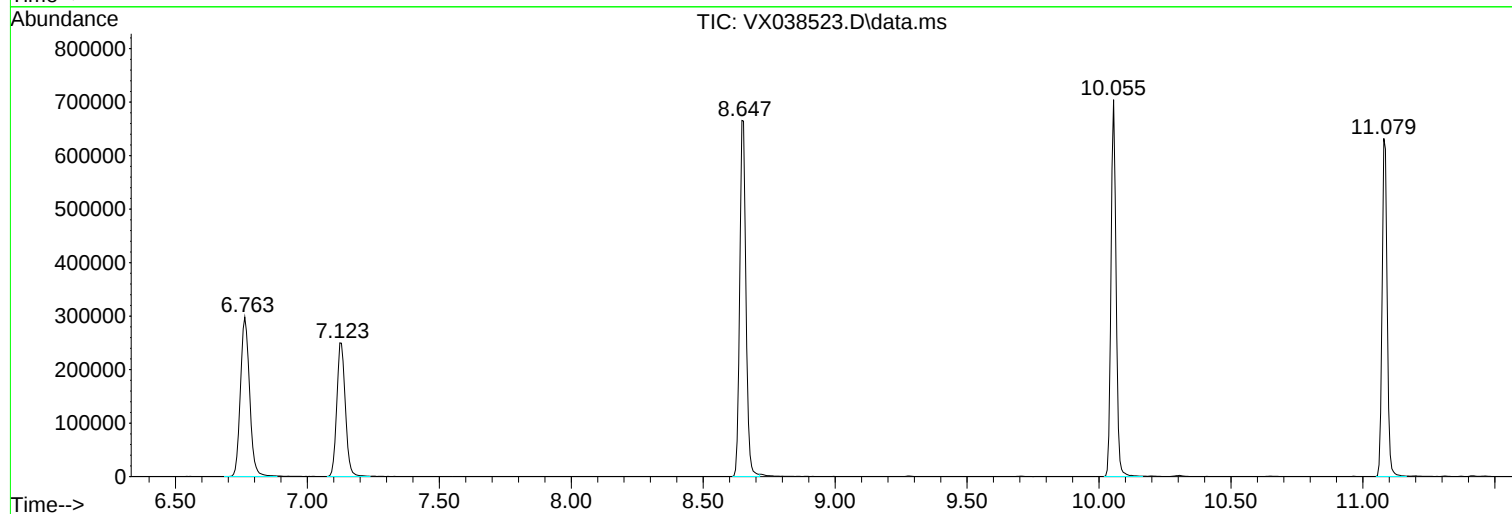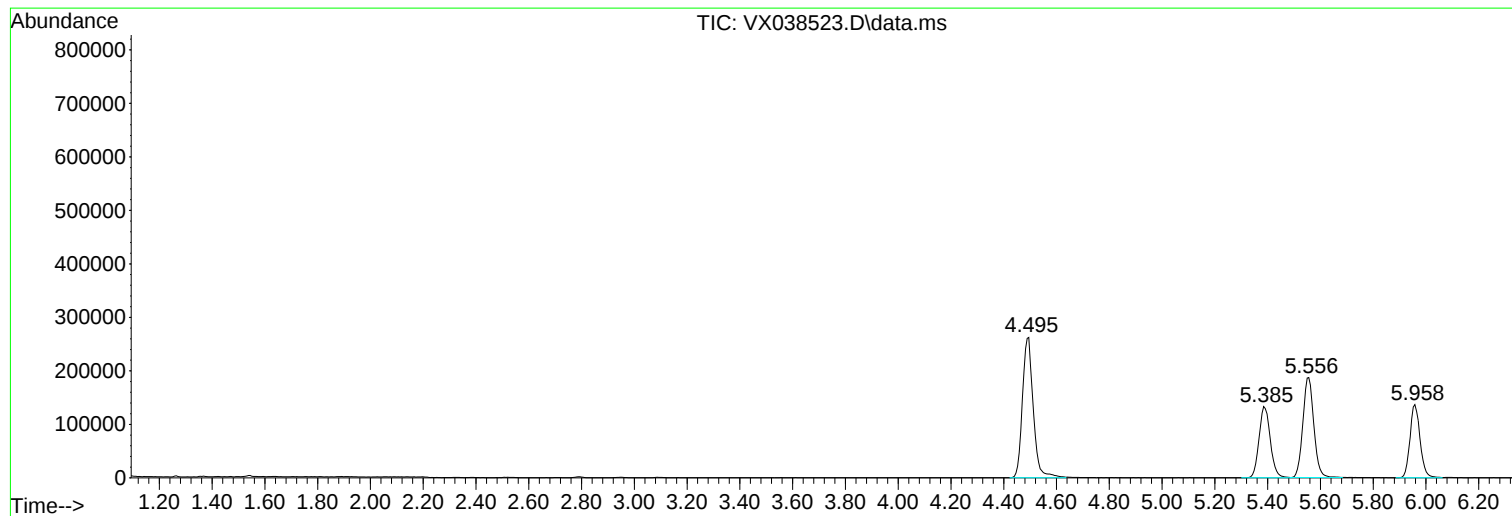

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038523.D
Acq On : 26 Oct 2023 17:19
Operator : JC/MD
Sample : 05063-03 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038523.D
Acq On : 26 Oct 2023 17:19
Operator : JC/MD
Sample : 05063-03 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------