

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
 Data File : VX038525.D
 Acq On : 26 Oct 2023 18:05
 Operator : JC/MD
 Sample : 05097-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-22

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	57	rVB	23475	25309	2.35%	0.418%
2	4.489	549	558	566	rBV	45378	129053	11.97%	2.131%
3	4.568	567	571	583	rVB	10945	32466	3.01%	0.536%
4	5.385	694	705	721	rBV	130934	385999	35.79%	6.375%
5	5.556	721	733	749	rVV	182666	523041	48.49%	8.639%
6	5.958	788	799	820	rBV	133569	355056	32.92%	5.864%
7	6.763	921	931	950	rBV	292689	701576	65.05%	11.587%
8	8.647	1234	1240	1260	rBV	669147	1078587	100.00%	17.814%
9	10.055	1465	1471	1490	rBV	693704	939172	87.07%	15.511%
10	11.079	1634	1639	1655	rBV	623856	841268	78.00%	13.894%
11	12.024	1788	1794	1811	rBV	816392	1043220	96.72%	17.230%




Sum of corrected areas: 6054747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038525.D
Acq On : 26 Oct 2023 18:05
Operator : JC/MD
Sample : 05097-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

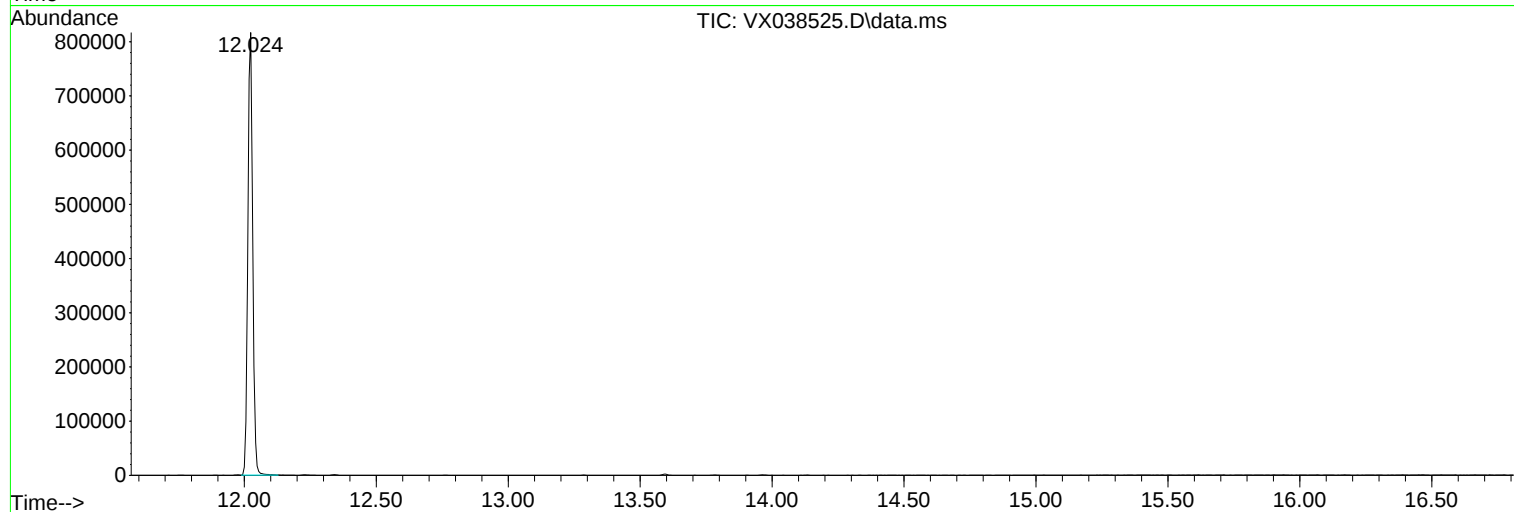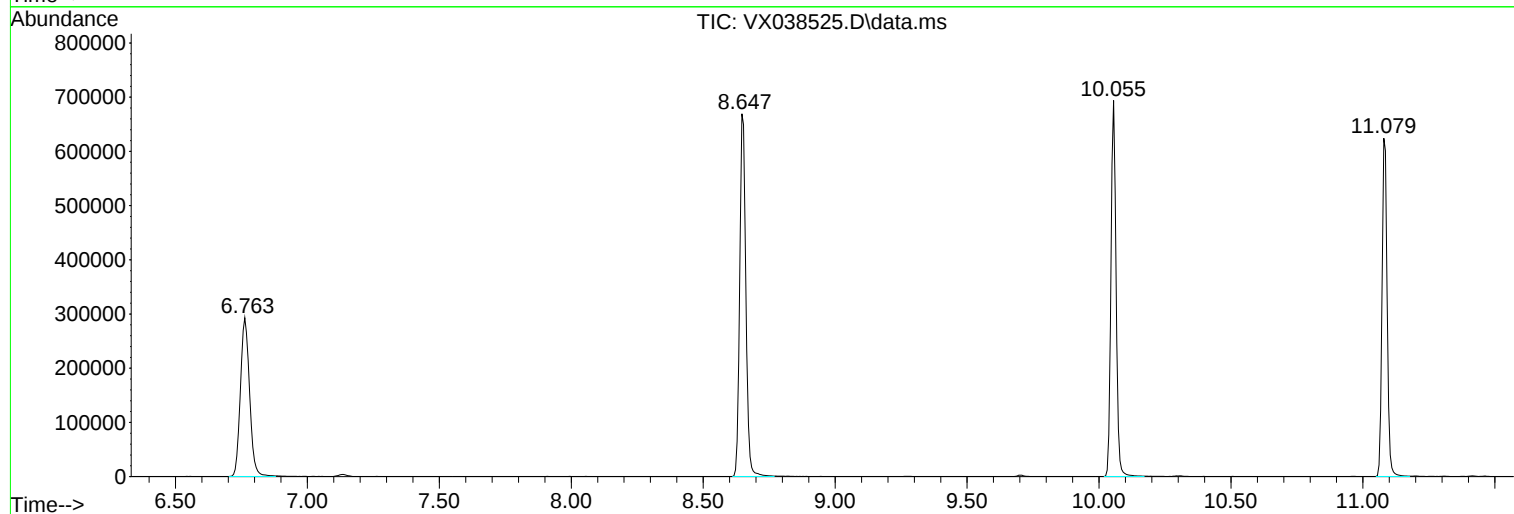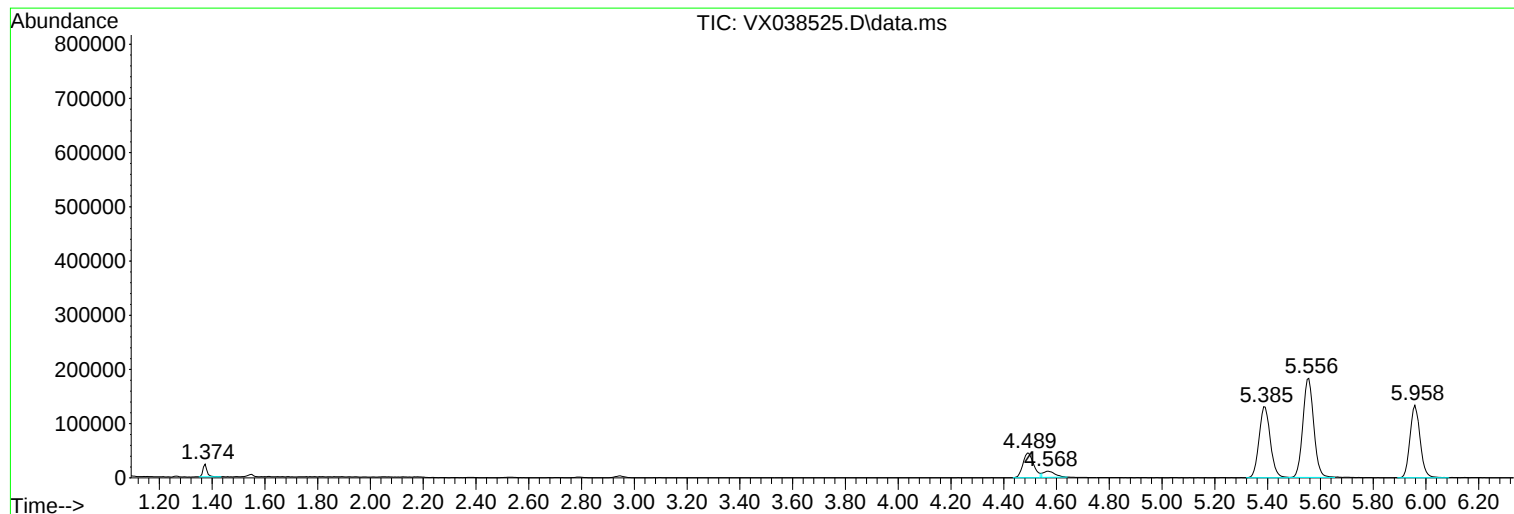

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038525.D
Acq On : 26 Oct 2023 18:05
Operator : JC/MD
Sample : 05097-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038525.D
Acq On : 26 Oct 2023 18:05
Operator : JC/MD
Sample : 05097-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------