

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
 Data File : VX038526.D
 Acq On : 26 Oct 2023 18:29
 Operator : JC/MD
 Sample : 05097-02 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LEA-7i

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.501	549	560	565	rBV2	6995	19327	1.79%	0.302%
2	4.568	565	571	586	rVB2	5362	17812	1.65%	0.278%
3	5.391	693	706	722	rBV2	130926	385869	35.80%	6.021%
4	5.556	722	733	746	rBV	183201	520726	48.31%	8.125%
5	5.958	789	799	816	rBV	131010	347769	32.27%	5.426%
6	6.763	921	931	956	rBV	290199	697818	64.75%	10.888%
7	7.129	981	991	1008	rBV	248204	545924	50.65%	8.518%
8	8.647	1234	1240	1258	rBV	668981	1077777	100.00%	16.817%
9	10.055	1465	1471	1491	rBV	674397	928905	86.19%	14.494%
10	11.079	1634	1639	1652	rBV	635080	833667	77.35%	13.008%
11	12.024	1788	1794	1806	rBV	812946	1033322	95.88%	16.123%




Sum of corrected areas: 6408916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038526.D
Acq On : 26 Oct 2023 18:29
Operator : JC/MD
Sample : 05097-02 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-7i

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

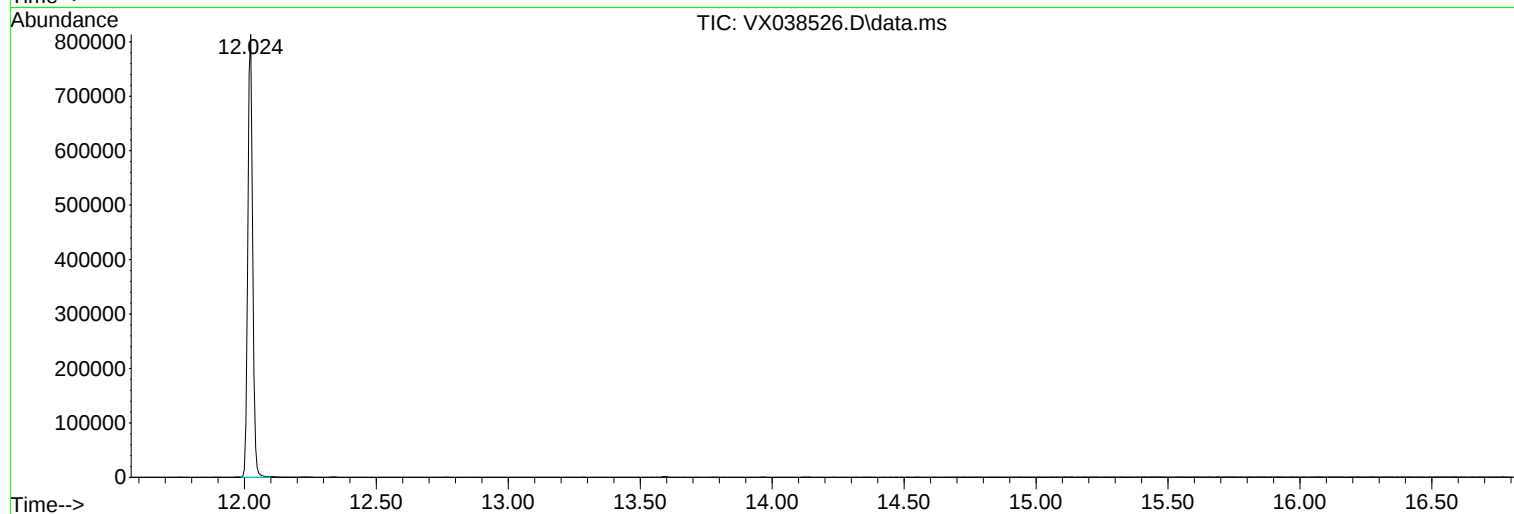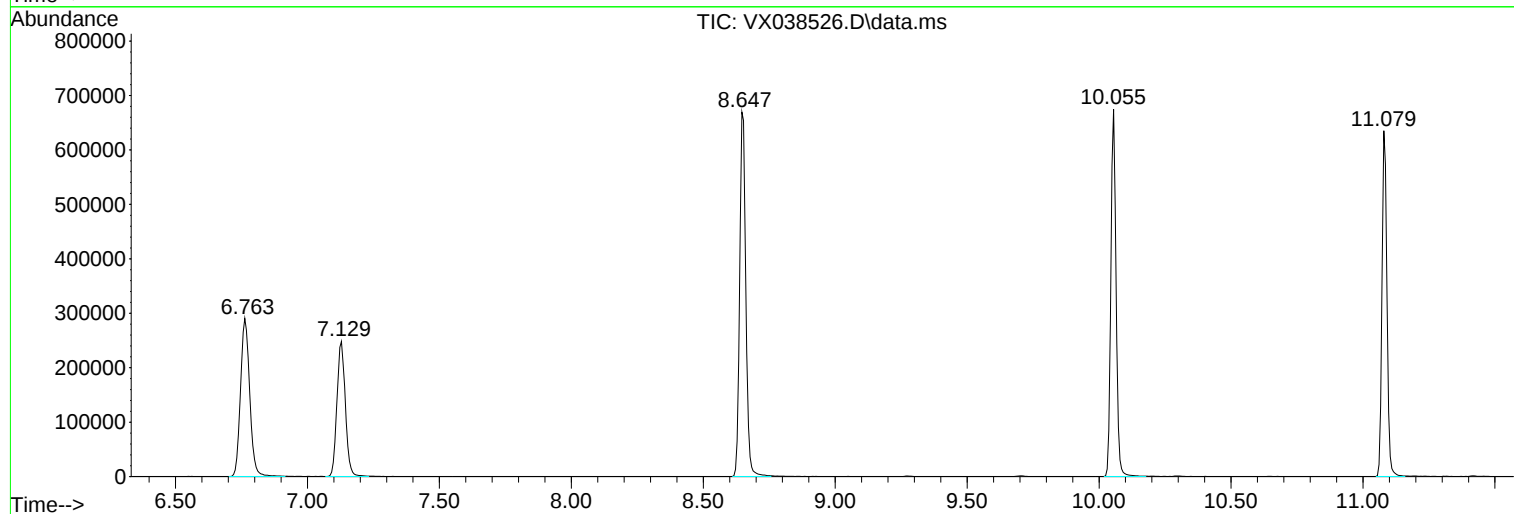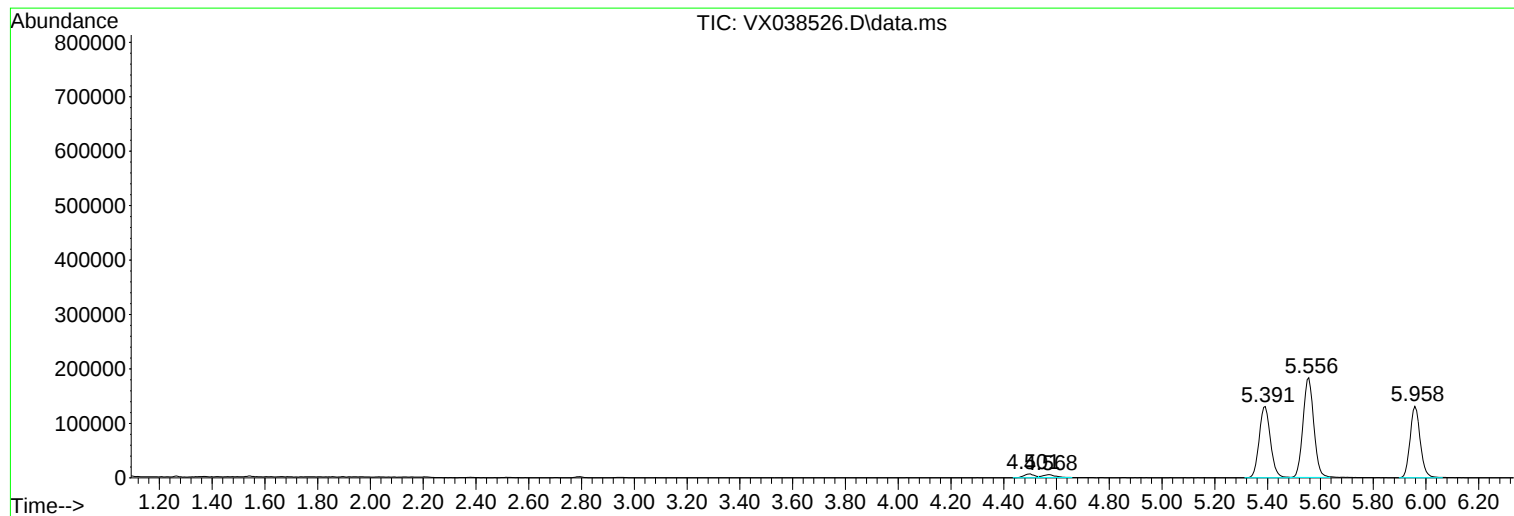

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038526.D
Acq On : 26 Oct 2023 18:29
Operator : JC/MD
Sample : 05097-02 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-7i

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102623\
Data File : VX038526.D
Acq On : 26 Oct 2023 18:29
Operator : JC/MD
Sample : 05097-02 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-7i

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------