



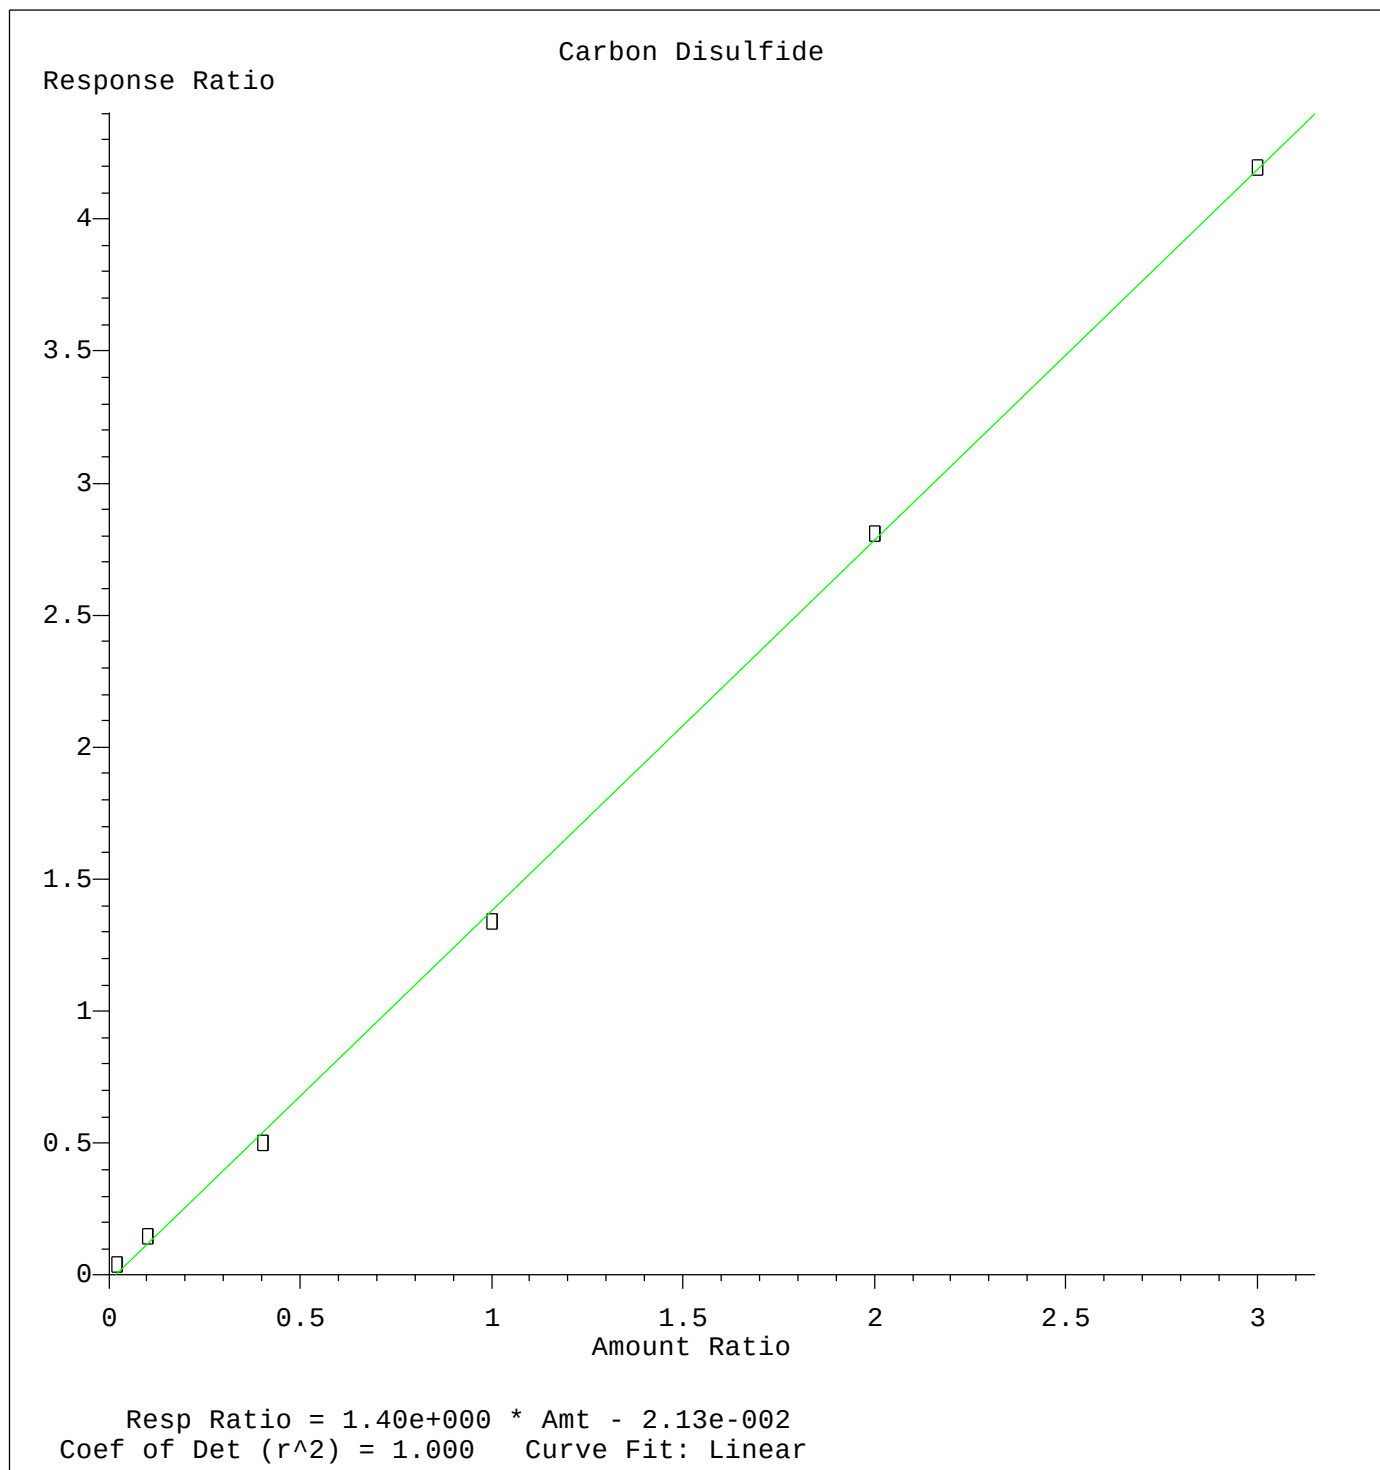

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102720W.M  
Calibration Table Last Updated: Tue Oct 27 13:55:07 2020


# Acrolein

Response Ratio

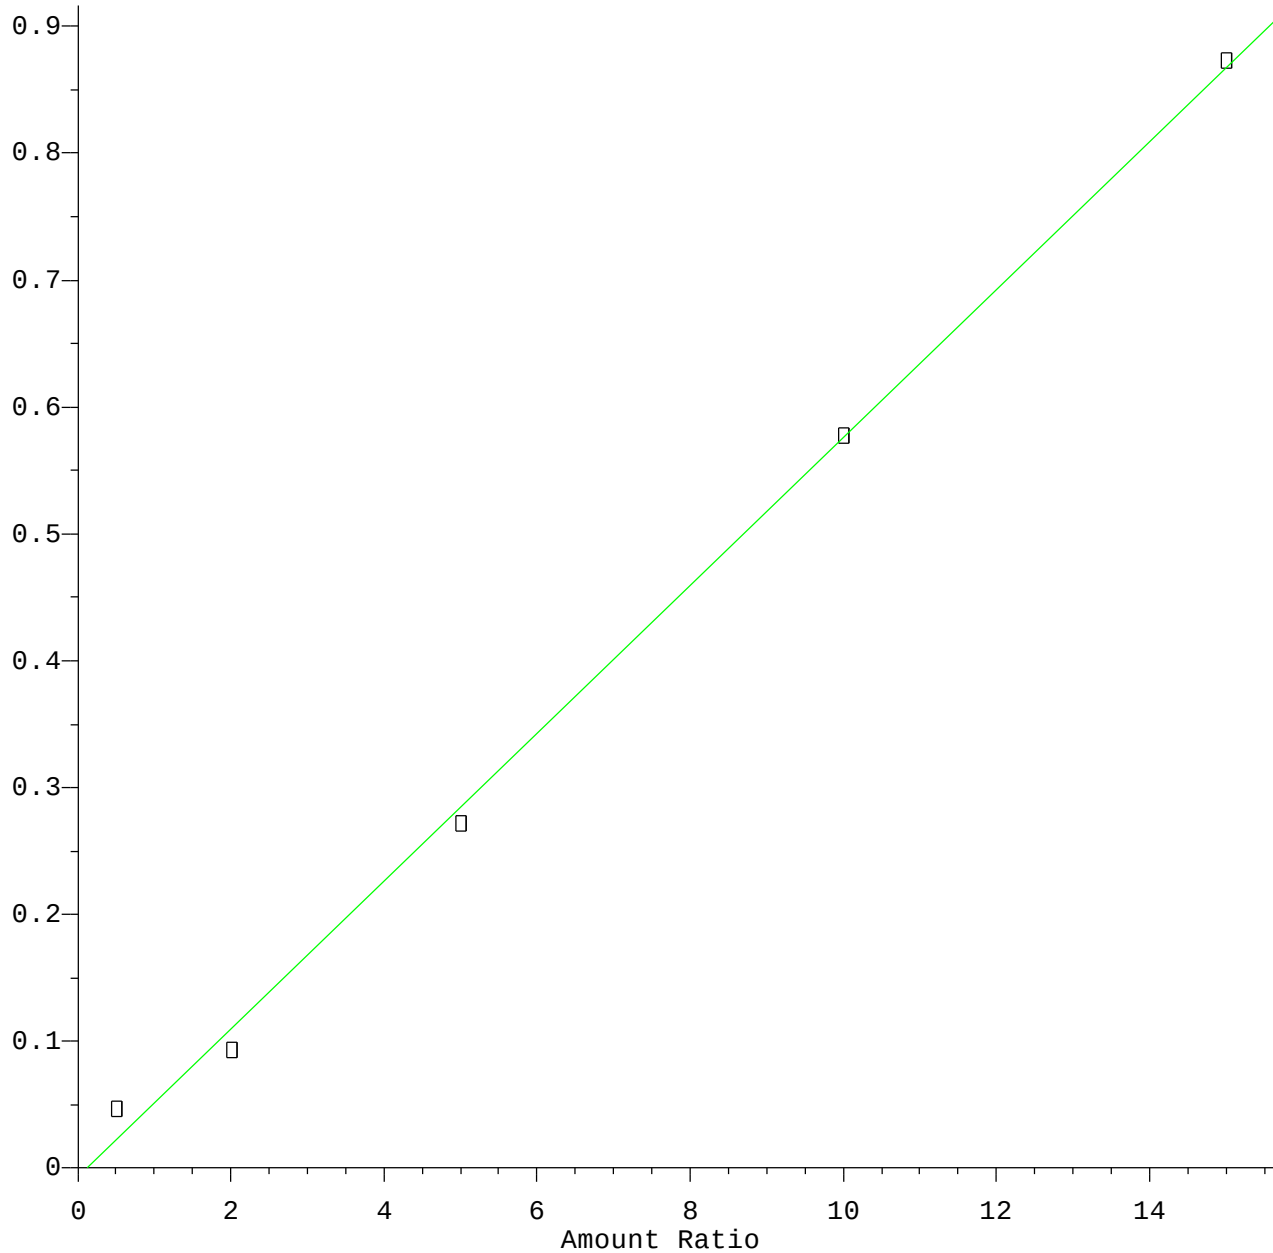

Resp Ratio =  $5.83 \times 10^{-2}$  \* Amt -  $6.58 \times 10^{-3}$   
Coef of Det ( $r^2$ ) = 0.998    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102720W.M  
Calibration Table Last Updated: Tue Oct 27 13:55:07 2020

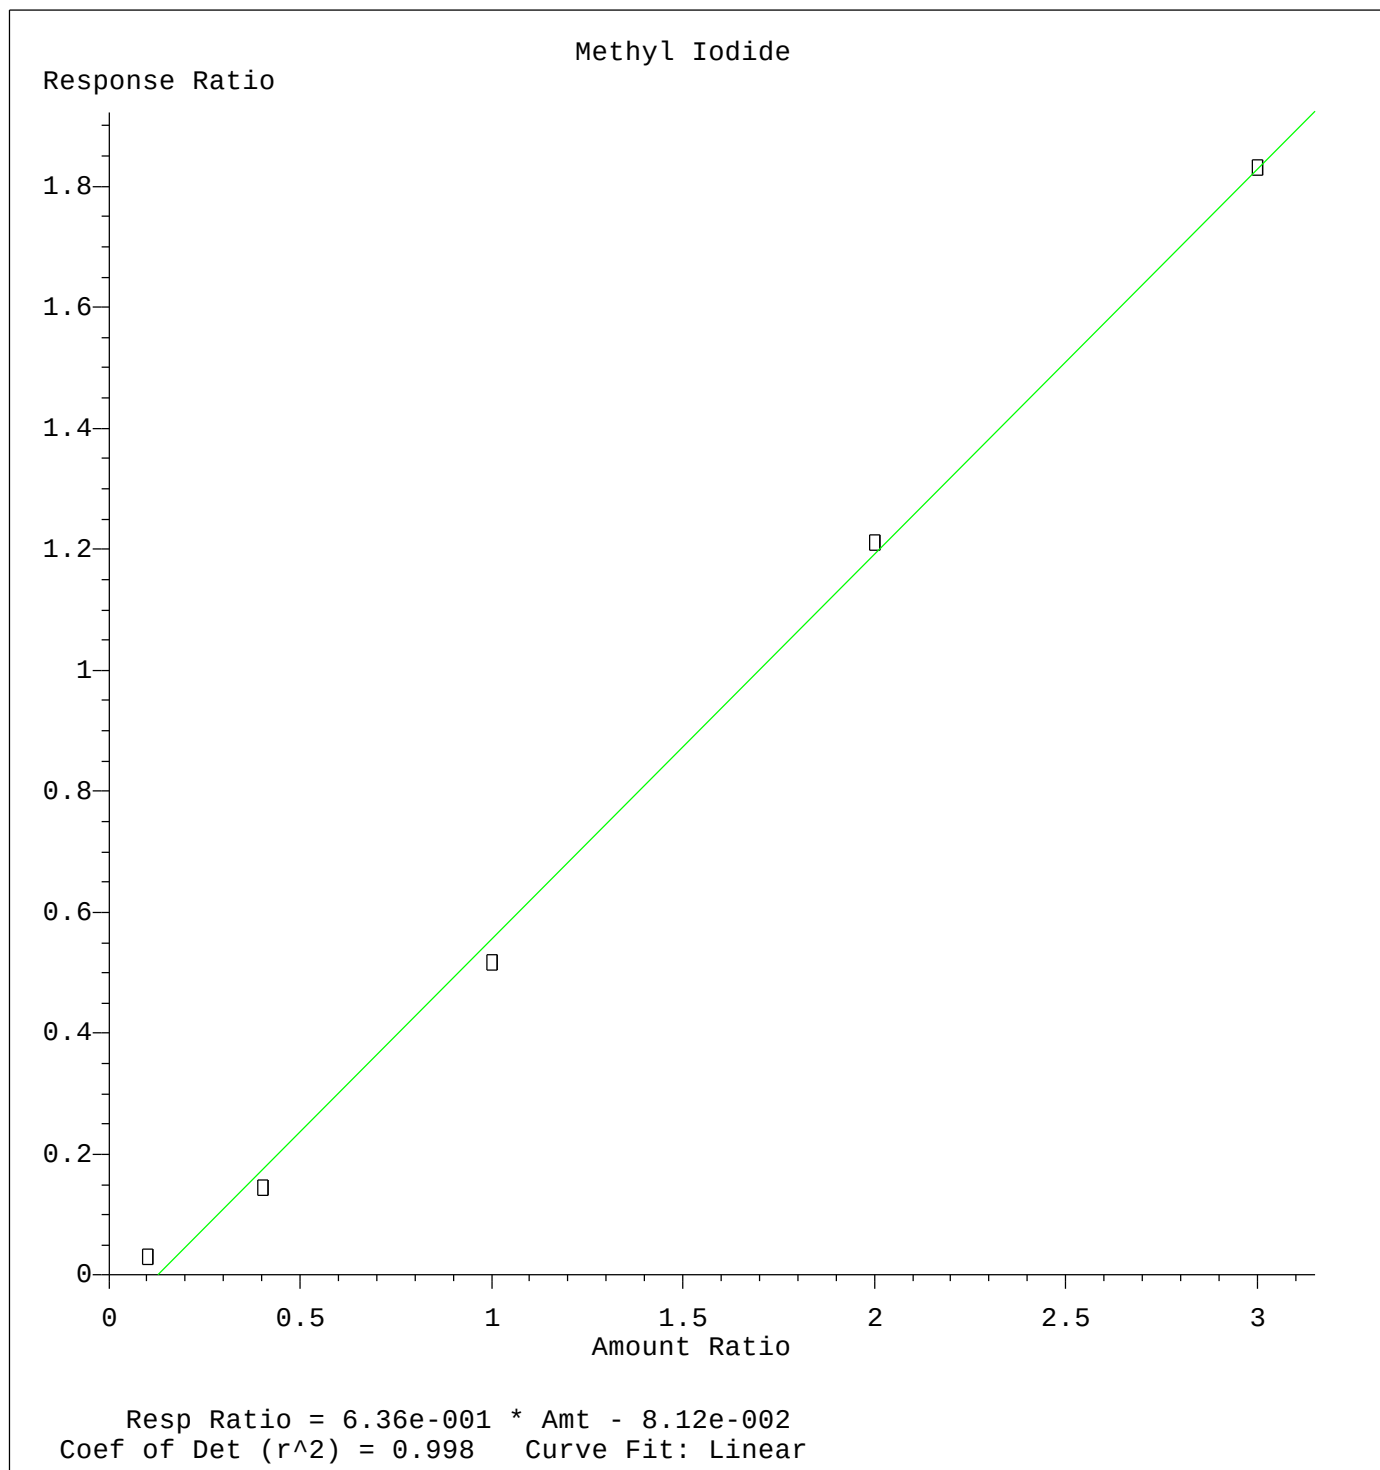

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102720W.M  
Calibration Table Last Updated: Tue Oct 27 13:55:07 2020