


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102720\
Data File : VX019129.D
Acq On : 27 Oct 2020 11:03
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Title : SW846 8260
Last Update : Tue Oct 27 13:55:07 2020

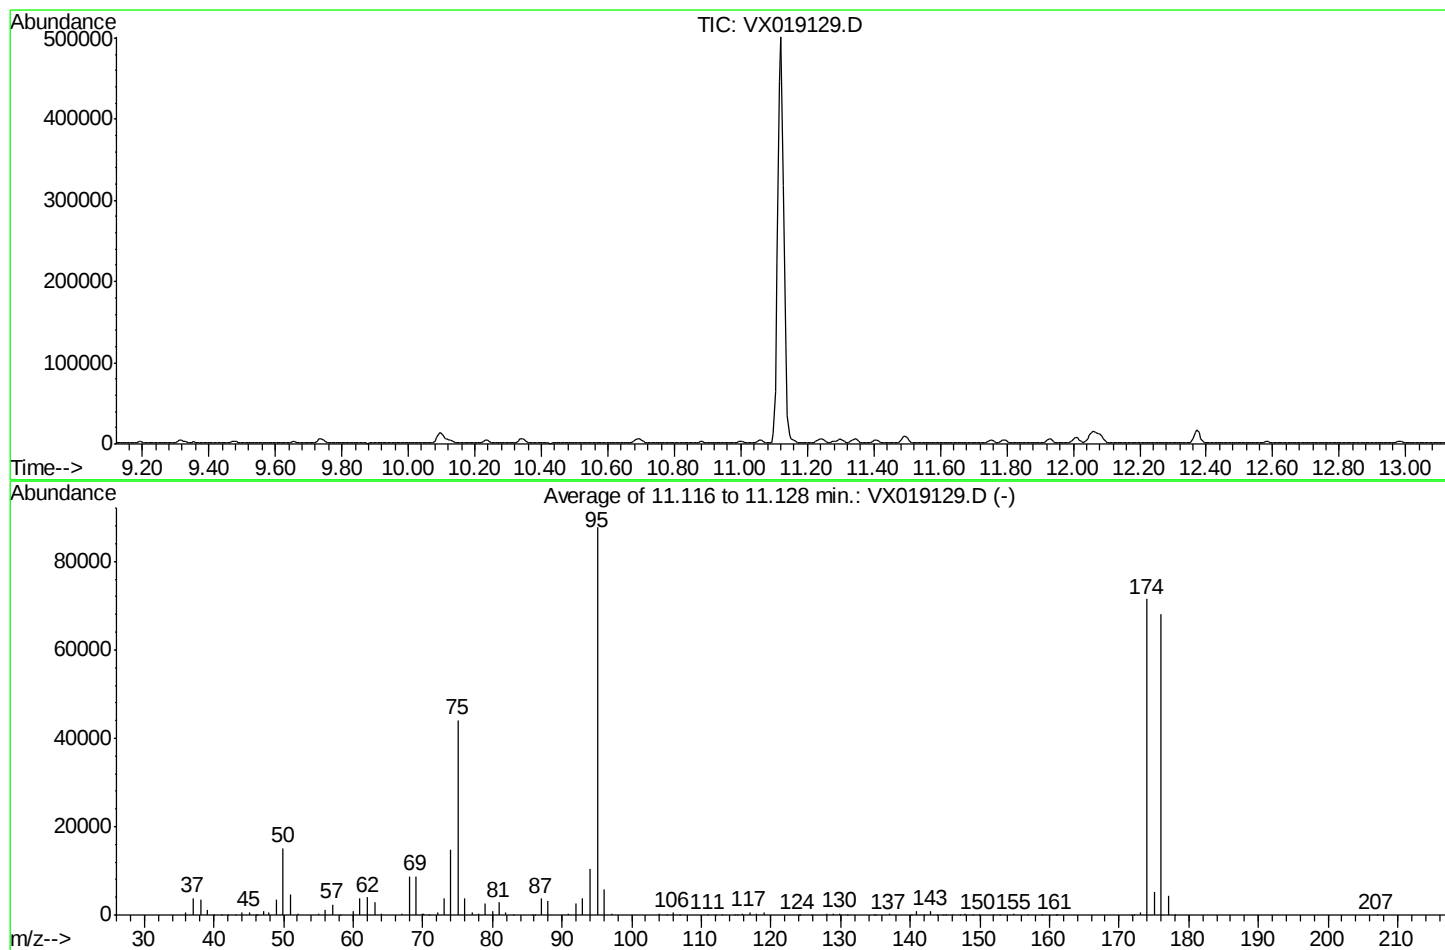

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	15076	PASS
75	95	30	60	50.3	44097	PASS
95	95	100	100	100.0	87730	PASS
96	95	5	9	6.7	5859	PASS
173	174	0.00	2	0.9	609	PASS
174	95	50	100	81.4	71421	PASS
175	174	5	9	7.3	5187	PASS
176	174	95	101	95.2	67968	PASS
177	176	5	9	6.3	4302	PASS