

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 P071-TW001-01

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

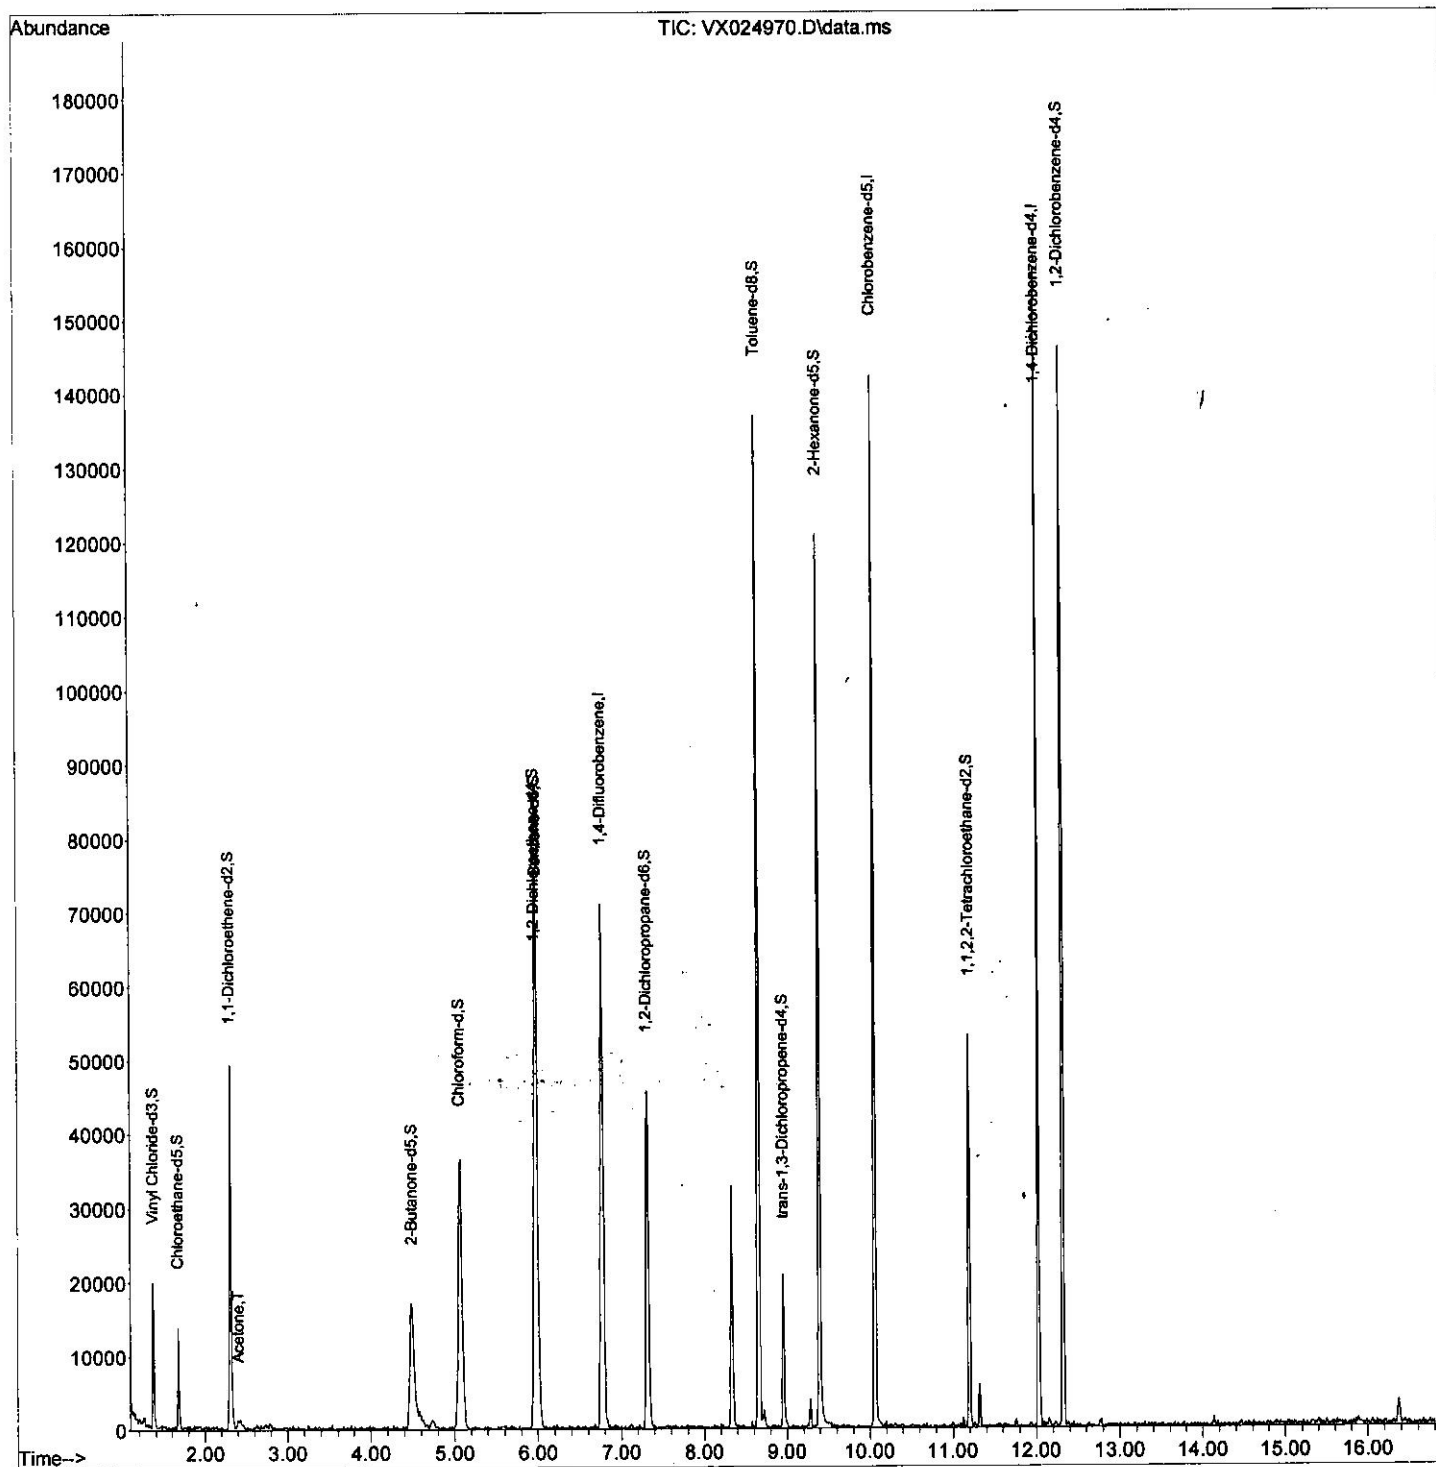

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

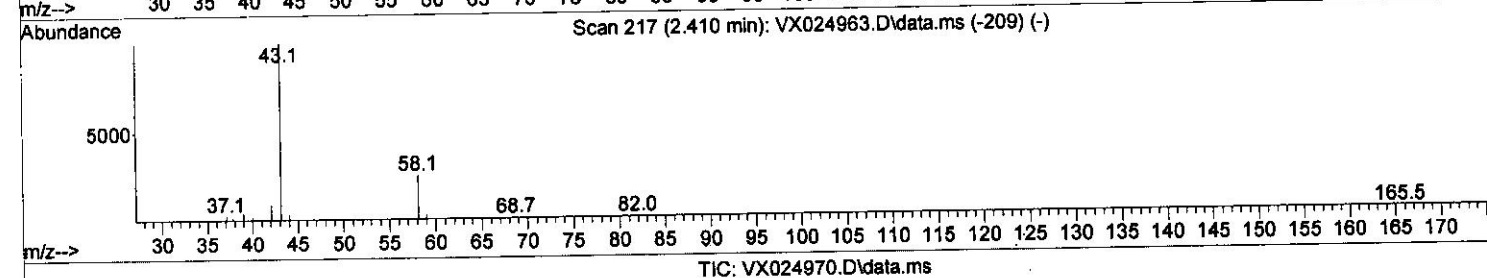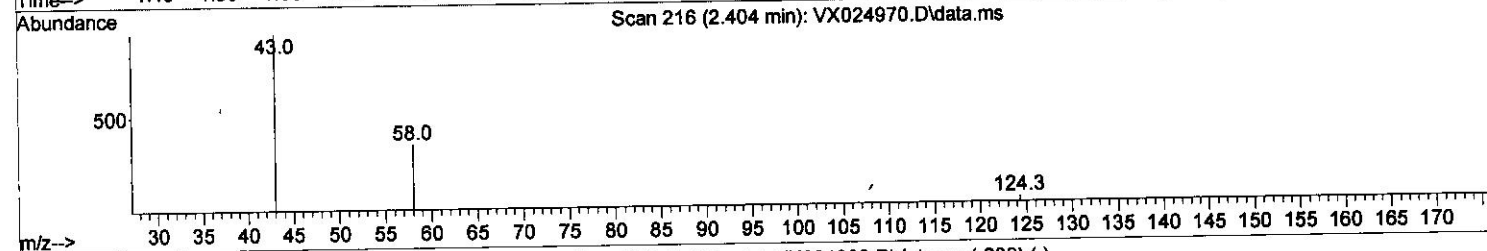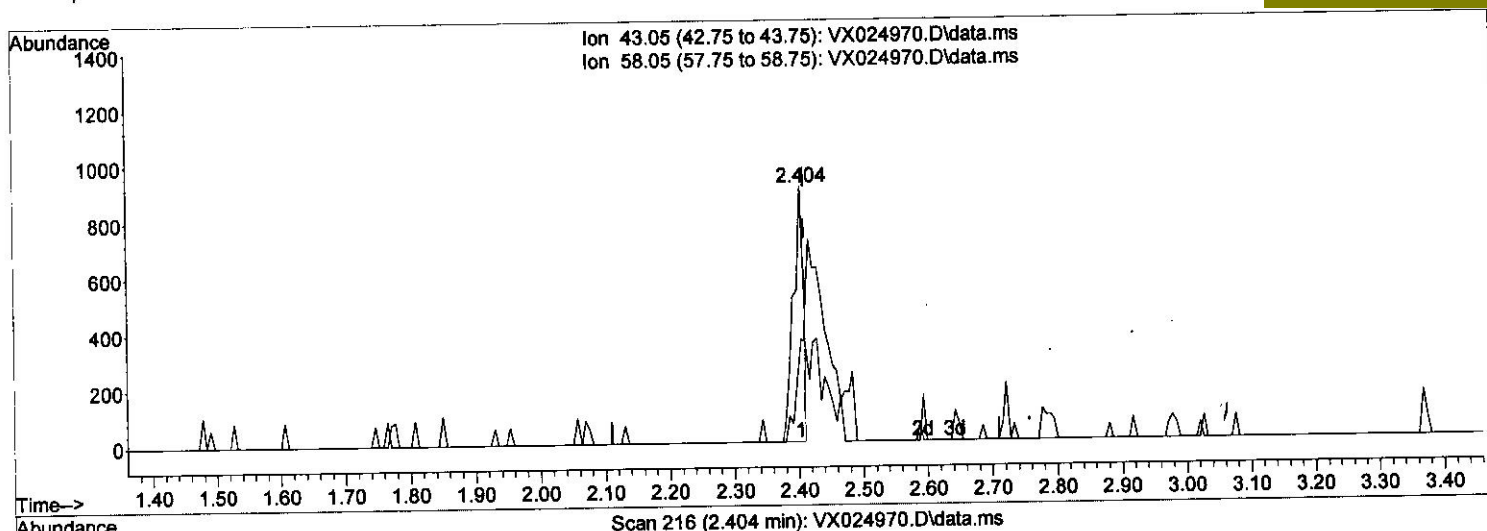

TIC: VX024970.D\data.ms

(13) Acetone (T)

2.404min (-0.006) 1.83 ug/L

response 1009

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	47.67
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

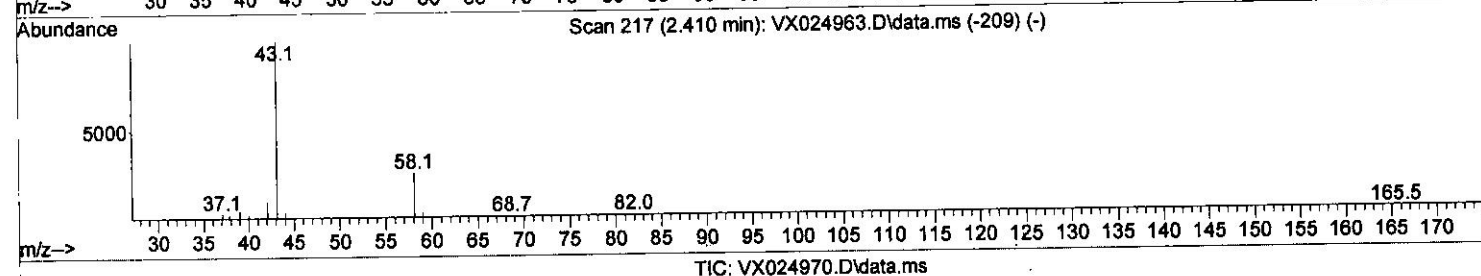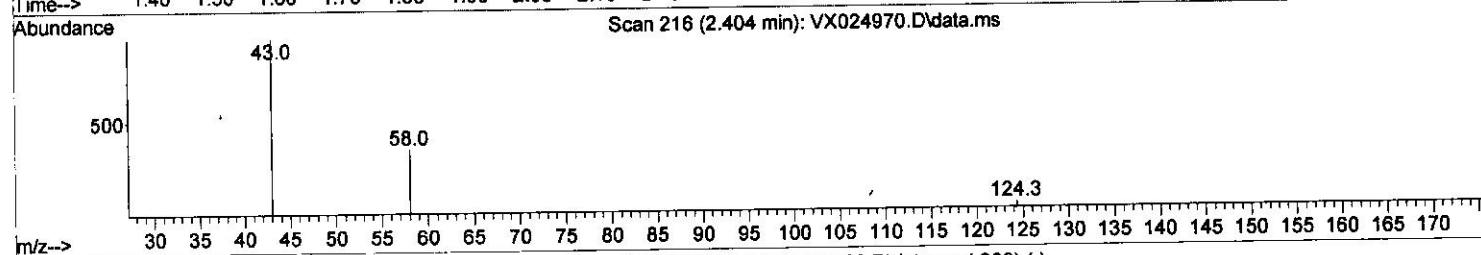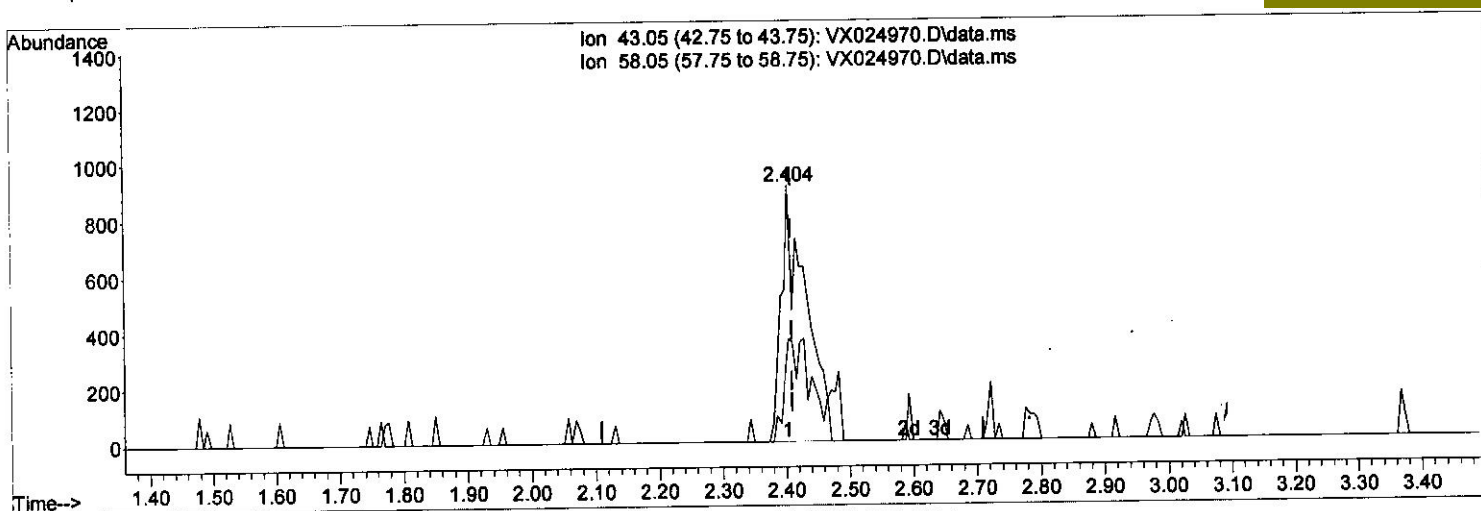

TIC: VX024970.D\data.ms

(13) Acetone (T)

2.404min (-0.006) 4.80 ug/L m

response 2653

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	18.13
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

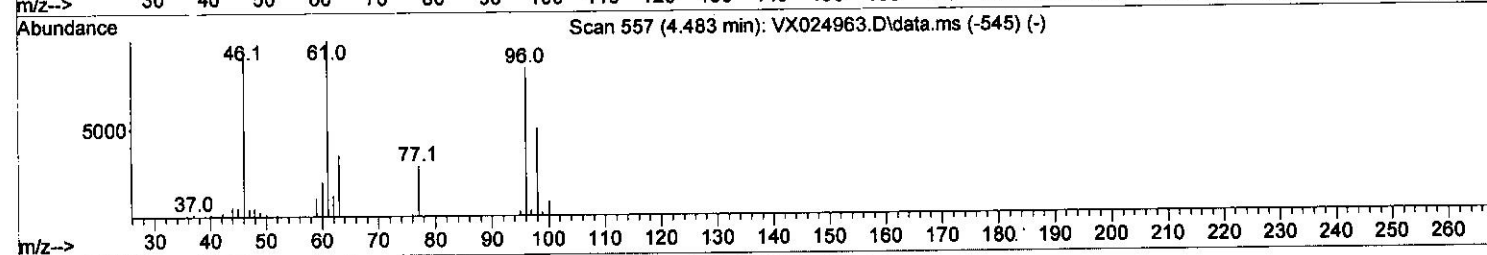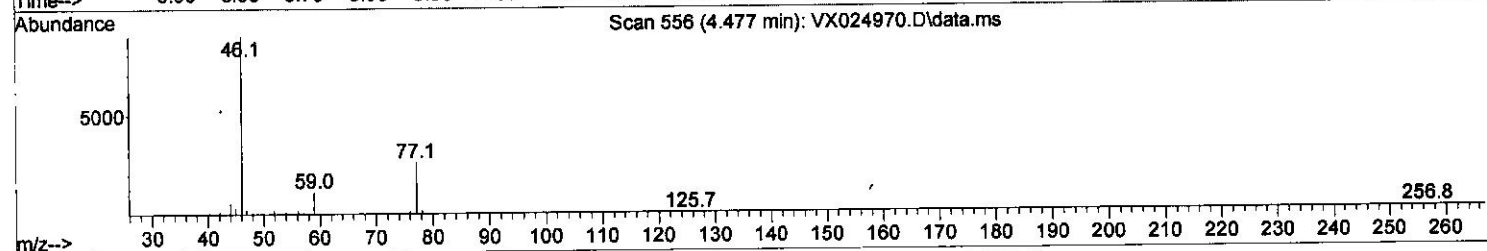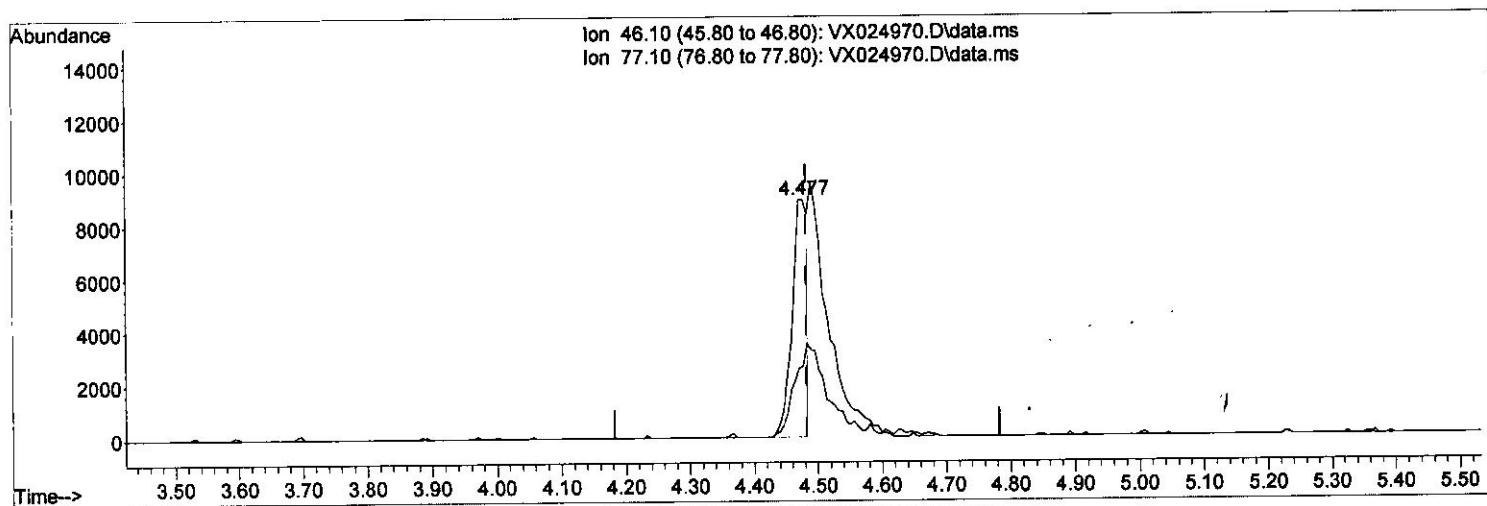

TIC: VX024970.D\data.ms

(20) 2-Butanone-d5 (S)

4.477min (-0.006) 19.87 ug/L

response 14646

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	32.30	83.15#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

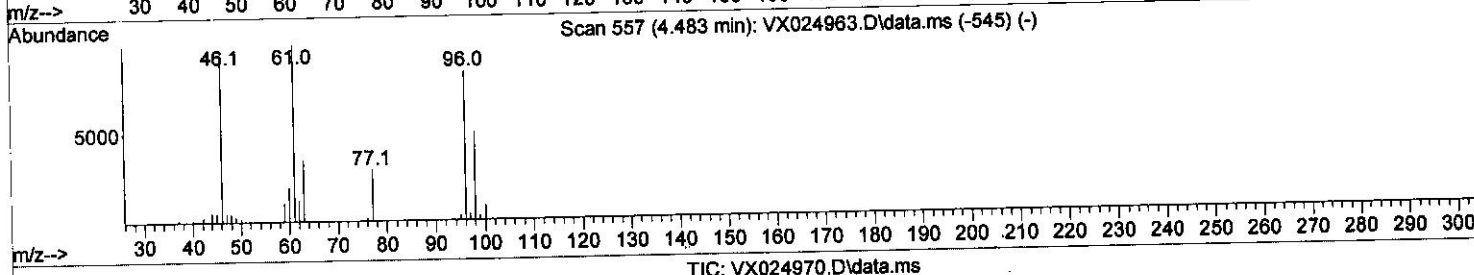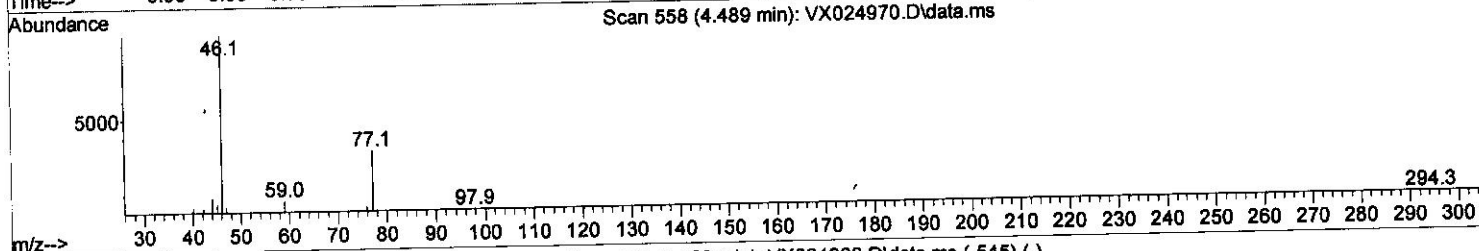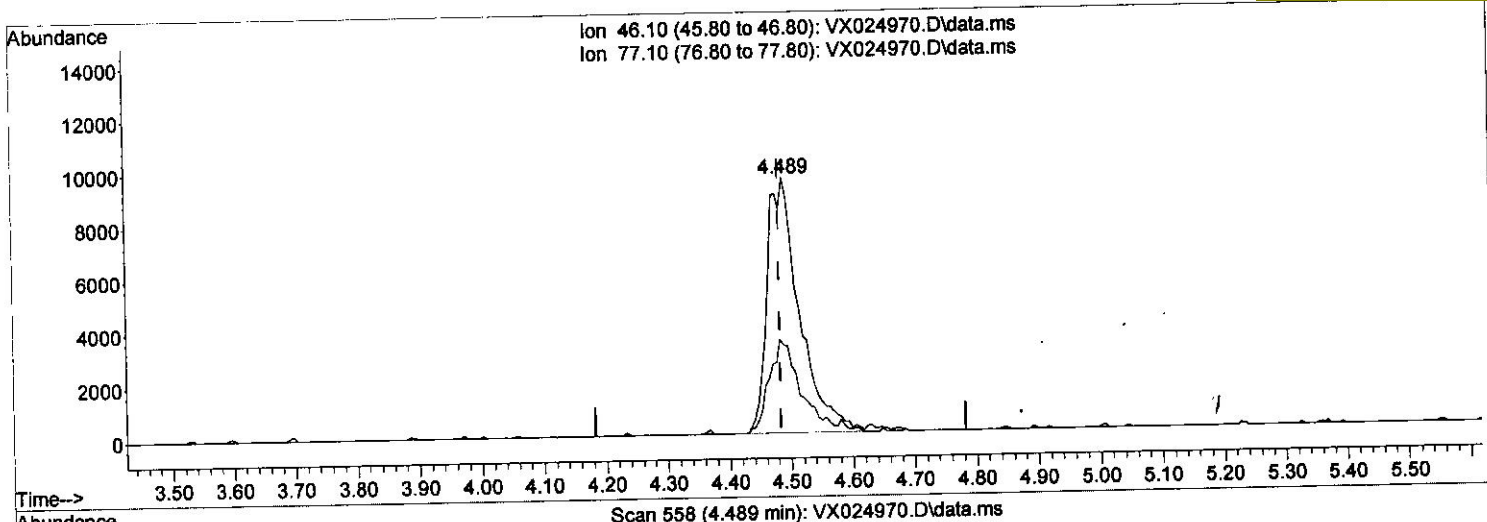

TIC: VX024970.D\data.ms

(20) 2-Butanone-d5 (S)

4.489min (+ 0.006) 47.11 ug/L m } m p
 10/29/21

response 34722

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	32.30	35.07
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\WX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 P071-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	68668	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	64046	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31758	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	10985	5.449	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery = 109.000%			
7) Chloroethane-d5	1.673	69	8557	4.711	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery = 94.200%			
11) 1,1-Dichloroethene-d2	2.307	63	27233	3.624	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery = 72.400%			
20) 2-Butanone-d5	4.489	46	34722m	47.109	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery = 94.220%			
24) Chloroform-d	5.062	84	49228	5.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery = 101.400%			
26) 1,2-Dichloroethane-d4	5.964	65	25898	4.882	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery = 97.600%			
32) Benzene-d6	5.989	84	79160	5.305	ug/L	0.01
Spiked Amount	5.000	Range 70 - 125	Recovery = 106.000%			
36) 1,2-Dichloropropane-d6	7.312	67	22174	4.657	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery = 93.200%			
41) Toluene-d8	8.653	98	80085	5.353	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery = 107.000%			
43) trans-1,3-Dichloroprop...	8.958	79	11802	5.401	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery = 108.000%			
46) 2-Hexanone-d5	9.391	63	37997	48.314	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery = 96.620%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19564	5.376	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery = 107.600%			
66) 1,2-Dichlorobenzene-d4	12.323	152	29083	5.434	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery = 108.600%			
Target Compounds						
13) Acetone	2.404	43	2653m	4.799	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed