

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024972.D
 Acq On : 27 Oct 2021 14:00
 Operator : JC/MD
 Sample : M4319-15
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-211020

Quant Time: Oct 28 03:11:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:13 PM

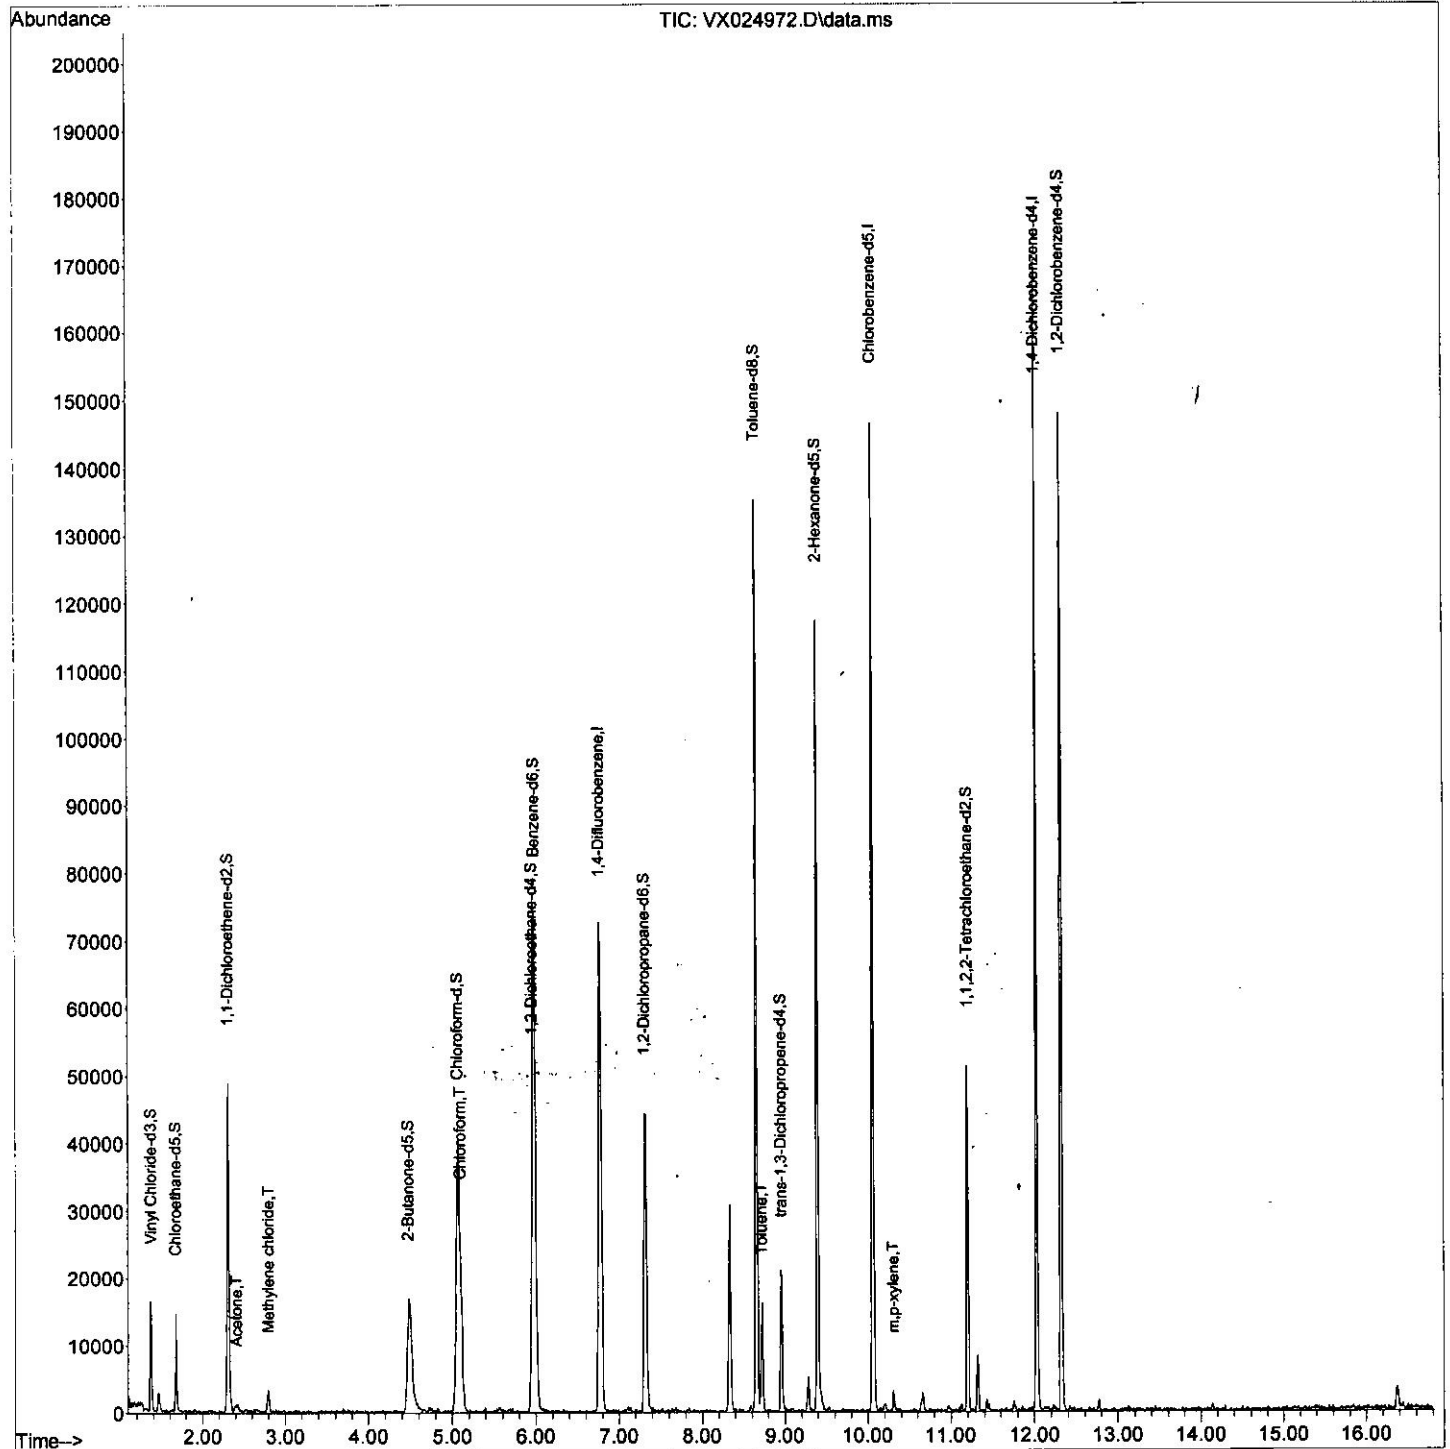

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024972.D
 Acq On : 27 Oct 2021 14:00
 Operator : JC/MD
 Sample : M4319-15
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 TB-211020

Quant Time: Oct 28 03:11:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:13 PM

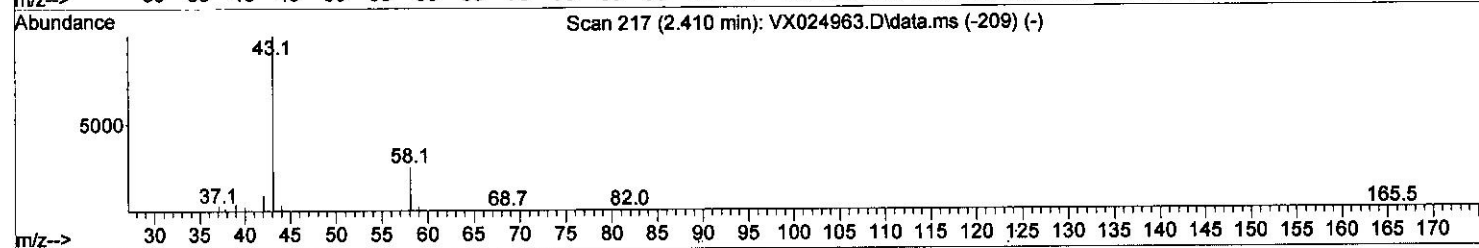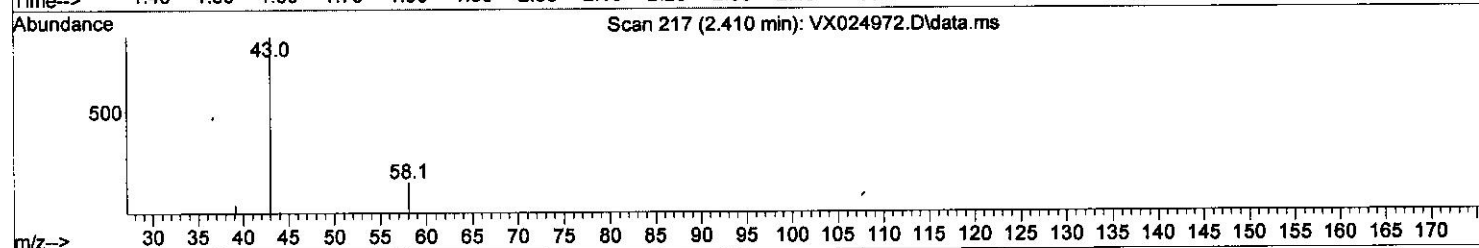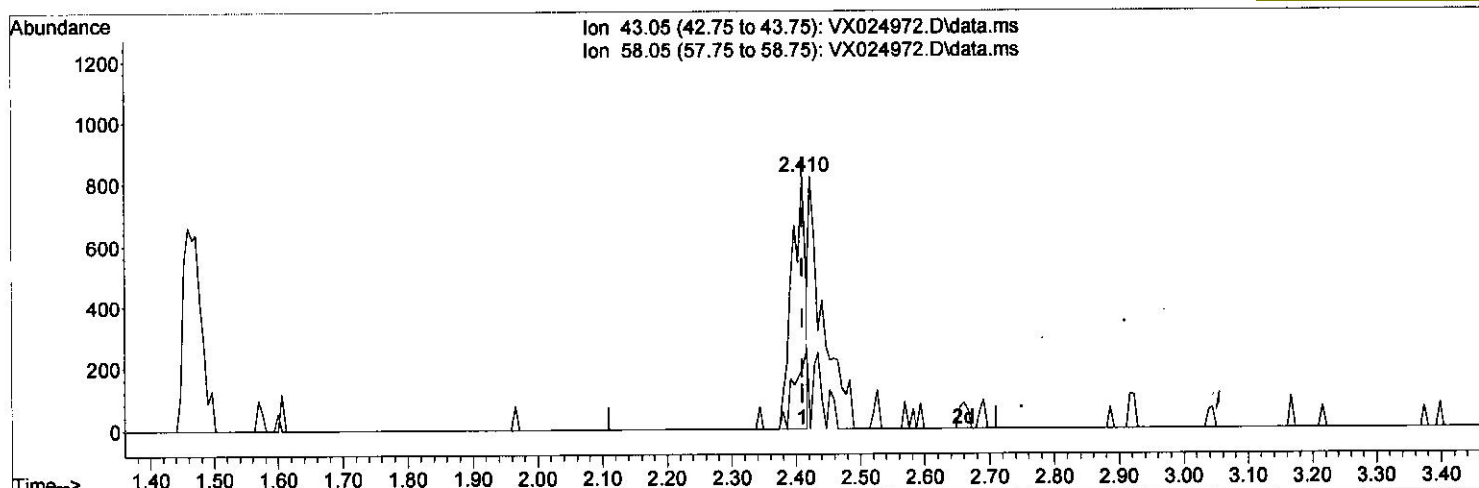

TIC: VX024972.D\data.ms

(13) Acetone (T)

2.410min (+ 0.000) 2.03 ug/L

response 1196

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	29.93
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024972.D
 Acq On : 27 Oct 2021 14:00
 Operator : JC/MD
 Sample : M4319-15
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 TB-211020

Quant Time: Oct 28 03:11:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:13 PM

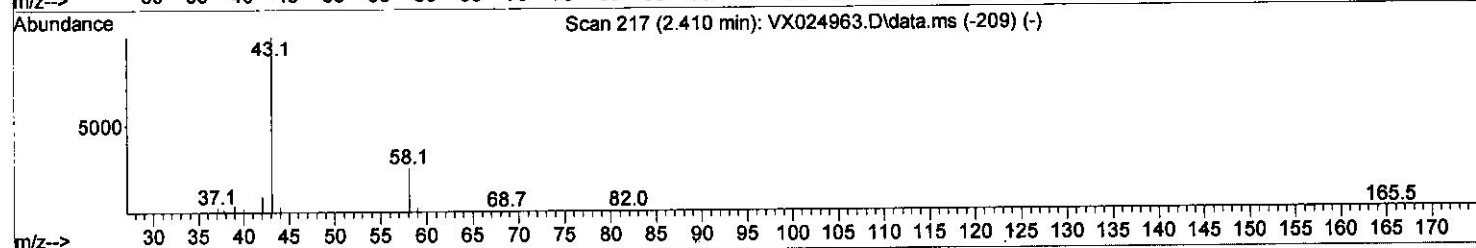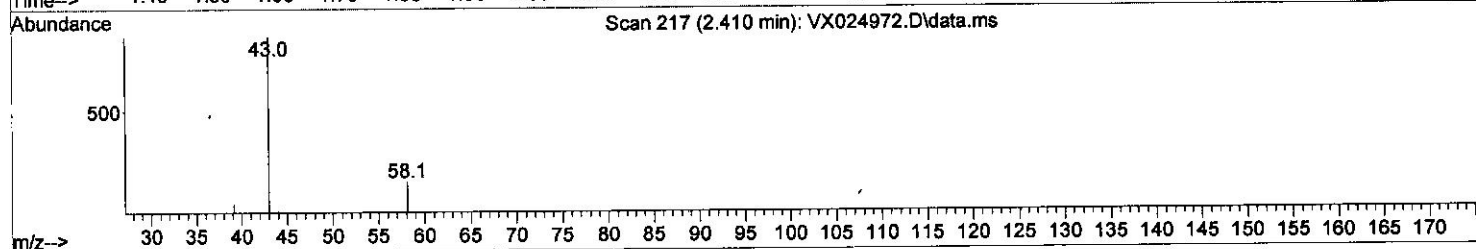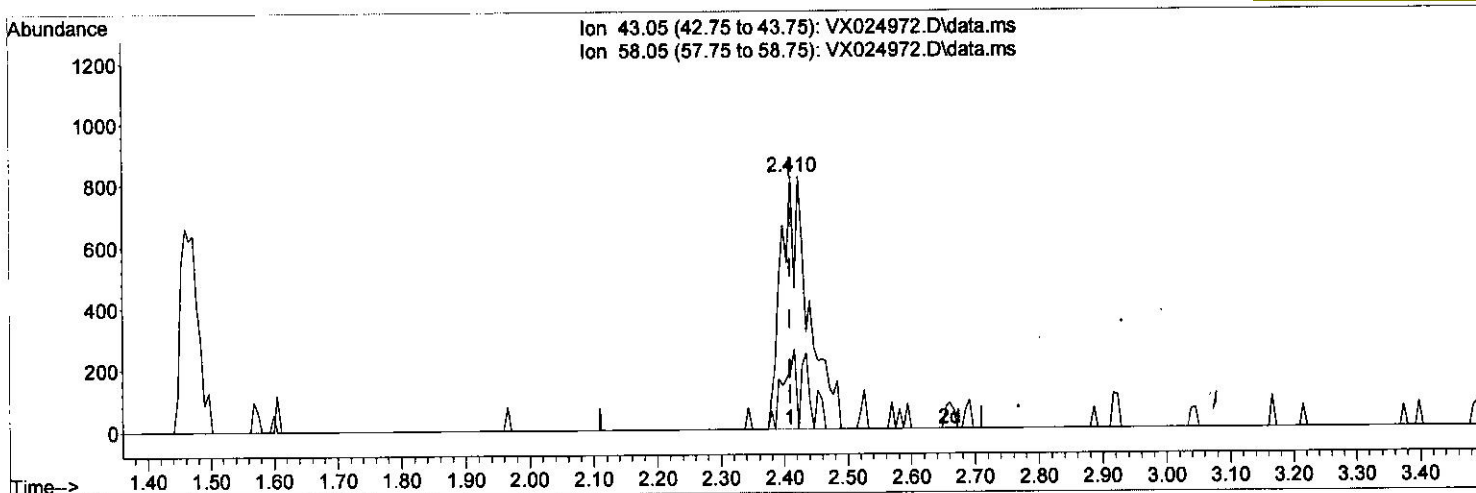

TIC: VX024972.D\data.ms

(13) Acetone (T)

2.410min (+ 0.000) 4.20 ug/L m

response 2478

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	14.45
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024972.D
 Acq On : 27 Oct 2021 14:00
 Operator : JC/MD
 Sample : M4319-15
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 TB-211020

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:13 PM

Quant Time: Oct 28 03:11:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	73218	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	68133	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32695	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	9854	4.584	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.600%	
7) Chloroethane-d5	1.672	69	8398	4.336	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.800%	
11) 1,1-Dichloroethene-d2	2.313	63	29010	3.621	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	4.477	46	34383	43.750	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.500%	
24) Chloroform-d	5.068	84	50684	4.898	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	5.958	65	25859	4.572	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
32) Benzene-d6	5.983	84	77839	4.903	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
36) 1,2-Dichloropropane-d6	7.312	67	21988	4.341	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.800%	
41) Toluene-d8	8.653	98	80464	5.055	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.200%	
43) trans-1,3-Dichloroprop...	8.958	79	12120	5.214	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	104.200%	
46) 2-Hexanone-d5	9.391	63	36741	43.914	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.820%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	17926	4.631	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	12.323	152	28571	5.185	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.800%	
Target Compounds						
13) Acetone	2.410	43	2478m	4.204	ug/L	
16) Methylene chloride	2.800	84	1804	0.346	ug/L	# 86
25) Chloroform	5.093	83	13732	1.154	ug/L	75
42) Toluene	8.720	91	10255	0.440	ug/L	99
53) m,p-xylene	10.305	106	916	0.094	ug/L	64

MP
 10/29/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed