




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
Data File : VX024974.D  
Acq On : 27 Oct 2021 14:44  
Operator : JC/MD  
Sample : MDL01  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MDL01

Manual Integrations  
APPROVED

MMDadoda  
10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Oct 28 03:09:30 2021  
Response via : Initial Calibration

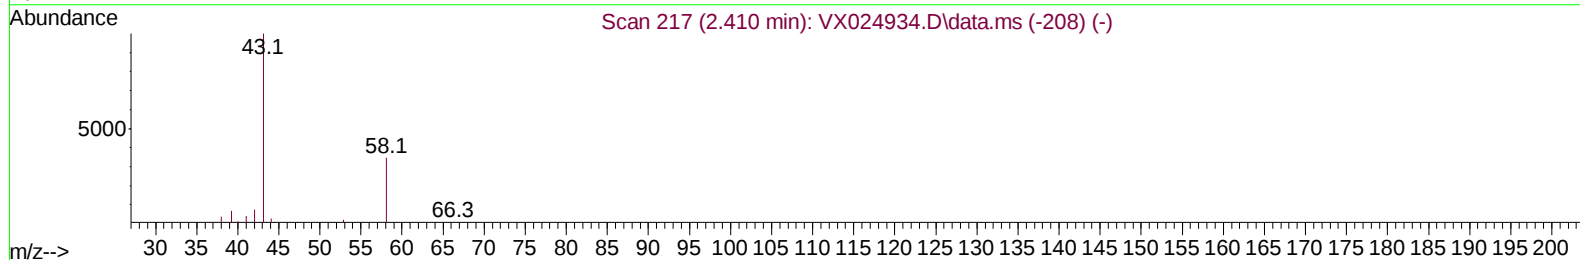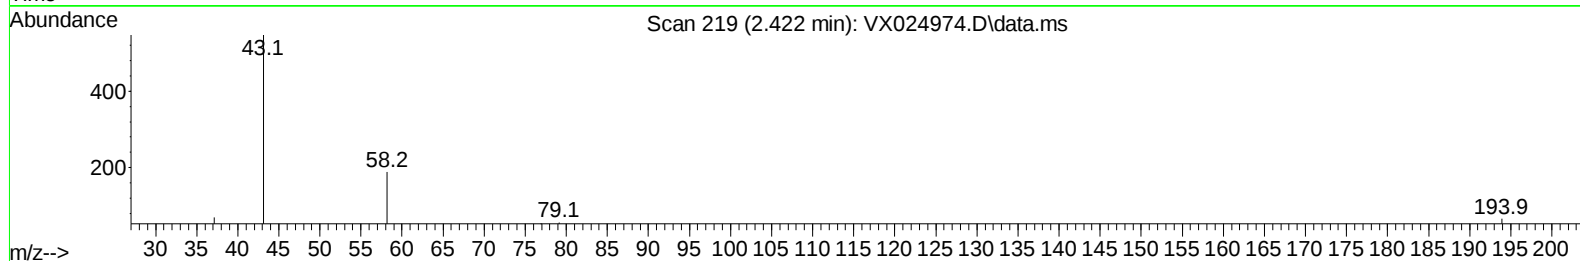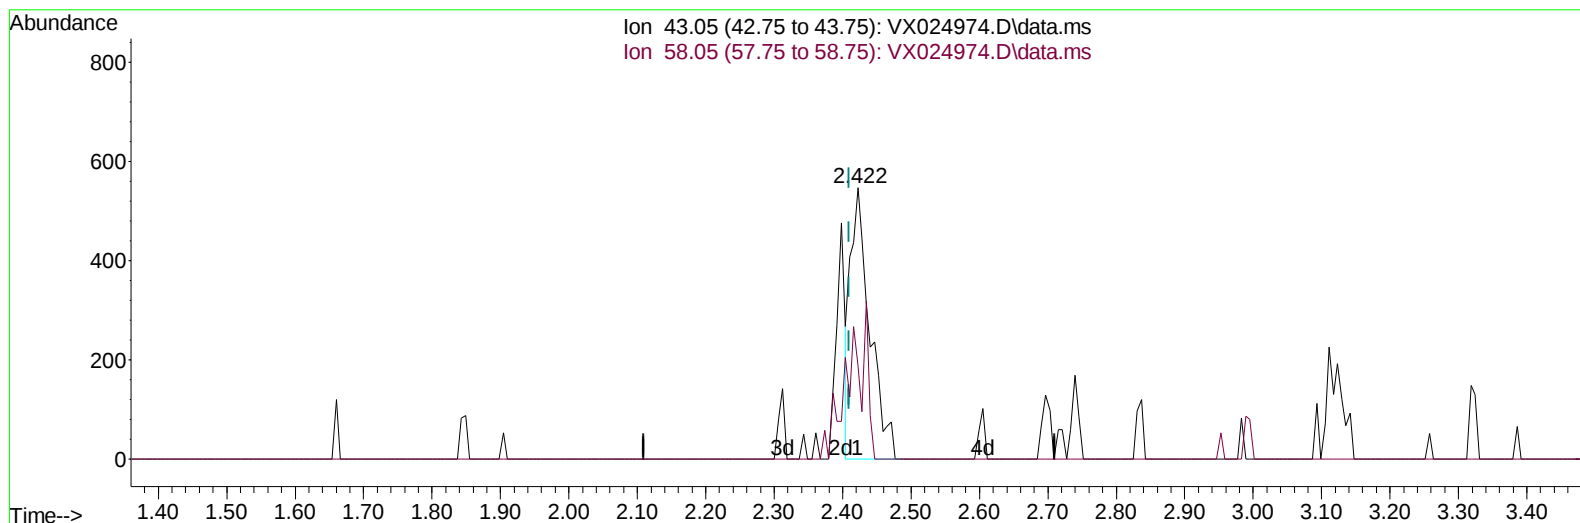

TIC: VX024974.D\data.ms

(13) Acetone (T)

2.422min (+ 0.012) 1.88 ug/L

response 1089

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 32.10  | 41.23  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

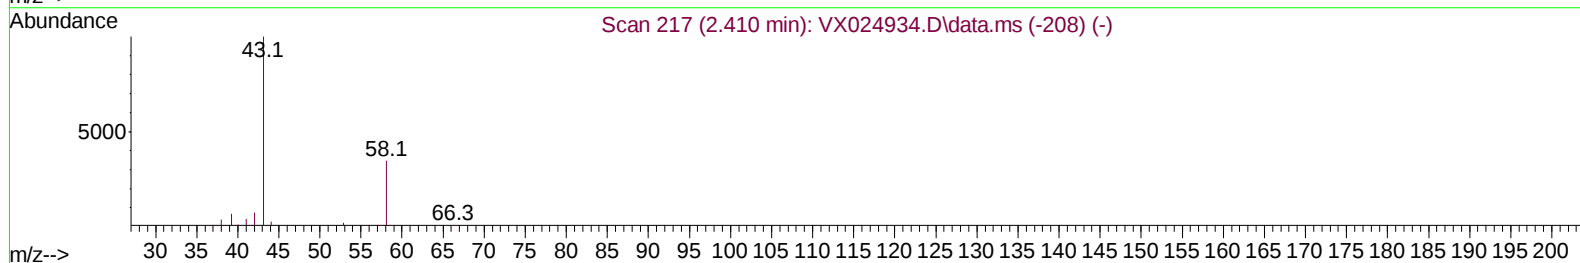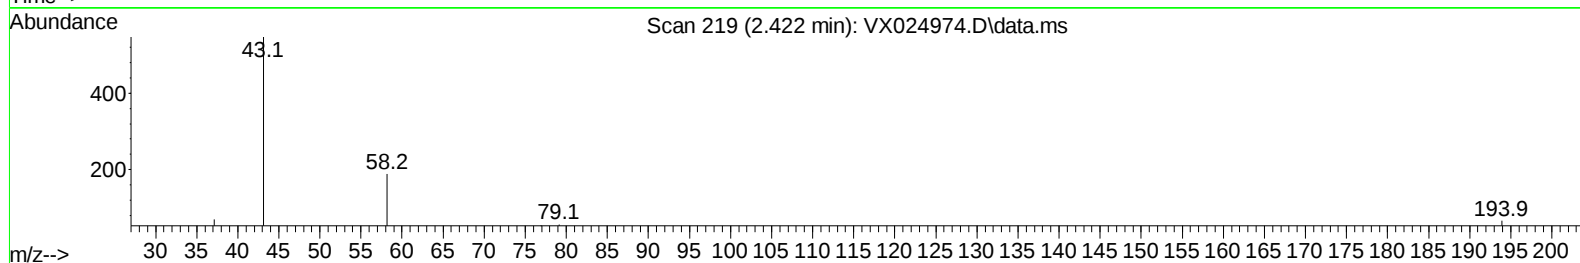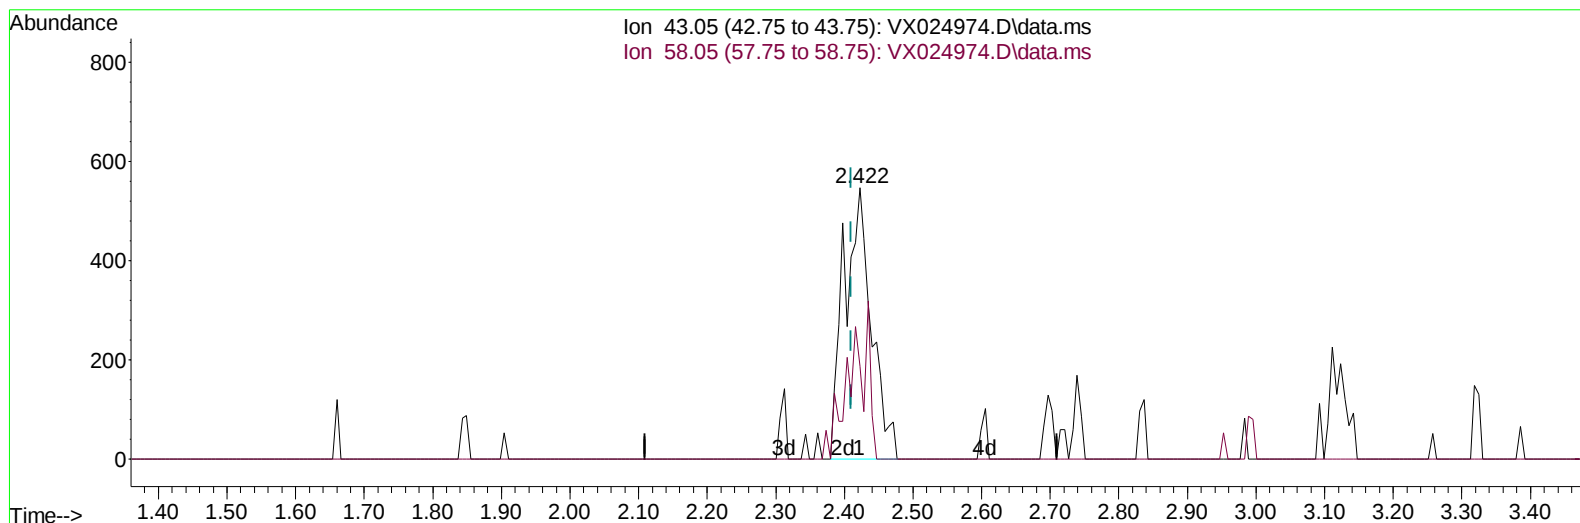

TIC: VX024974.D\data.ms

**(13) Acetone (T)**

**2.422min (+ 0.012) 2.61 ug/L m**

**response 1513**

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 32.10  | 29.68  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

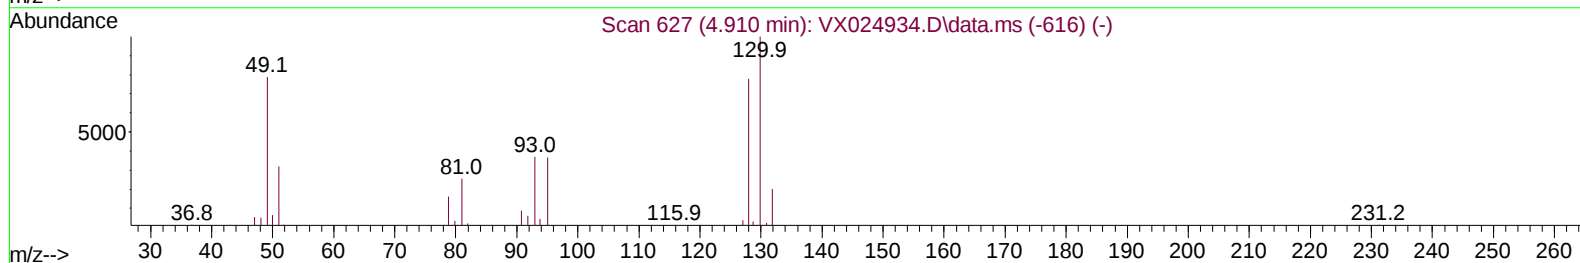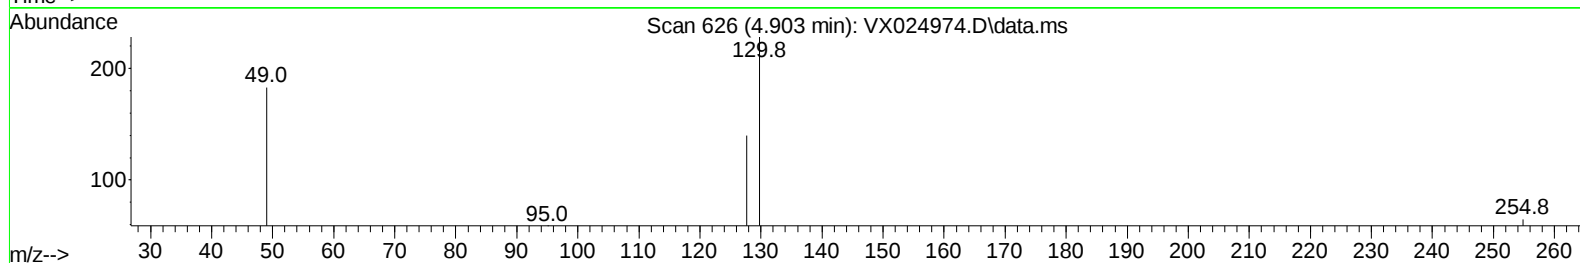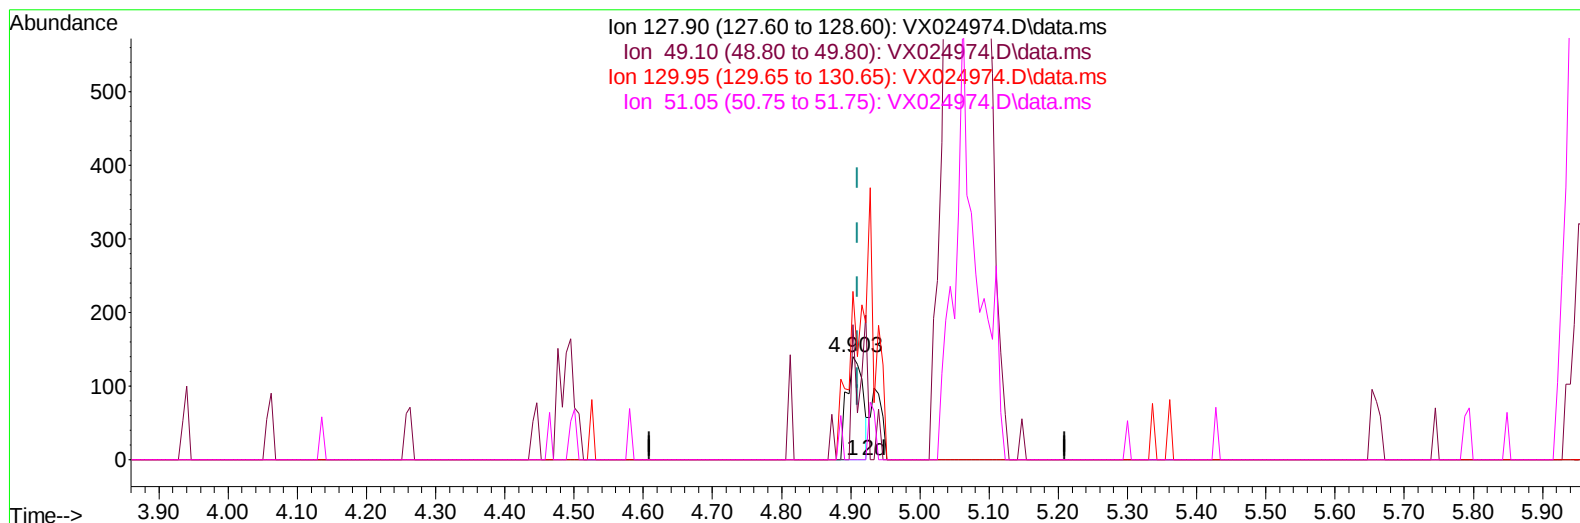

TIC: VX024974.D\data.ms

**(23) Bromochloromethane (T)**

4.903min (-0.006) 0.09 ug/L

response 225

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 127.90 | 100.00 | 100.00  |
| 49.10  | 122.50 | 130.71  |
| 129.95 | 116.30 | 162.86# |
| 51.05  | 36.00  | 0.00#   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
Data File : VX024974.D  
Acq On : 27 Oct 2021 14:44  
Operator : JC/MD  
Sample : MDL01  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MDL01

Manual Integrations  
APPROVED

MMDadoda  
10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Oct 28 03:09:30 2021  
Response via : Initial Calibration

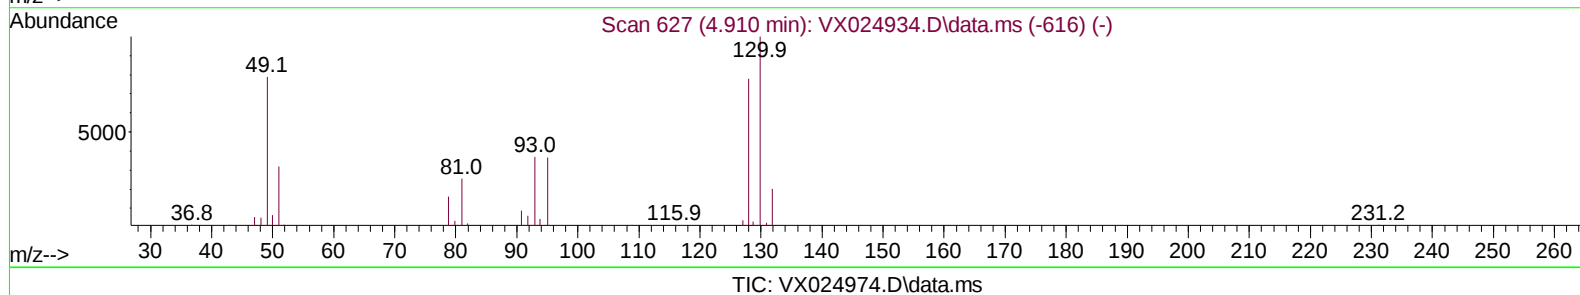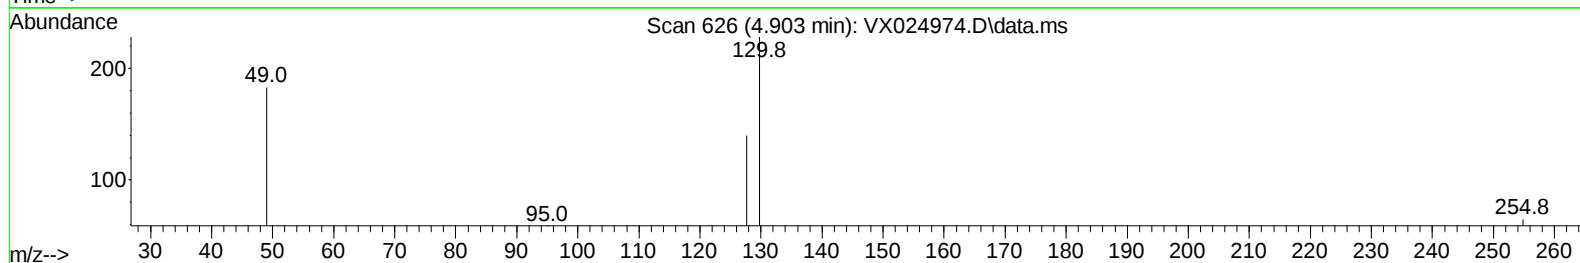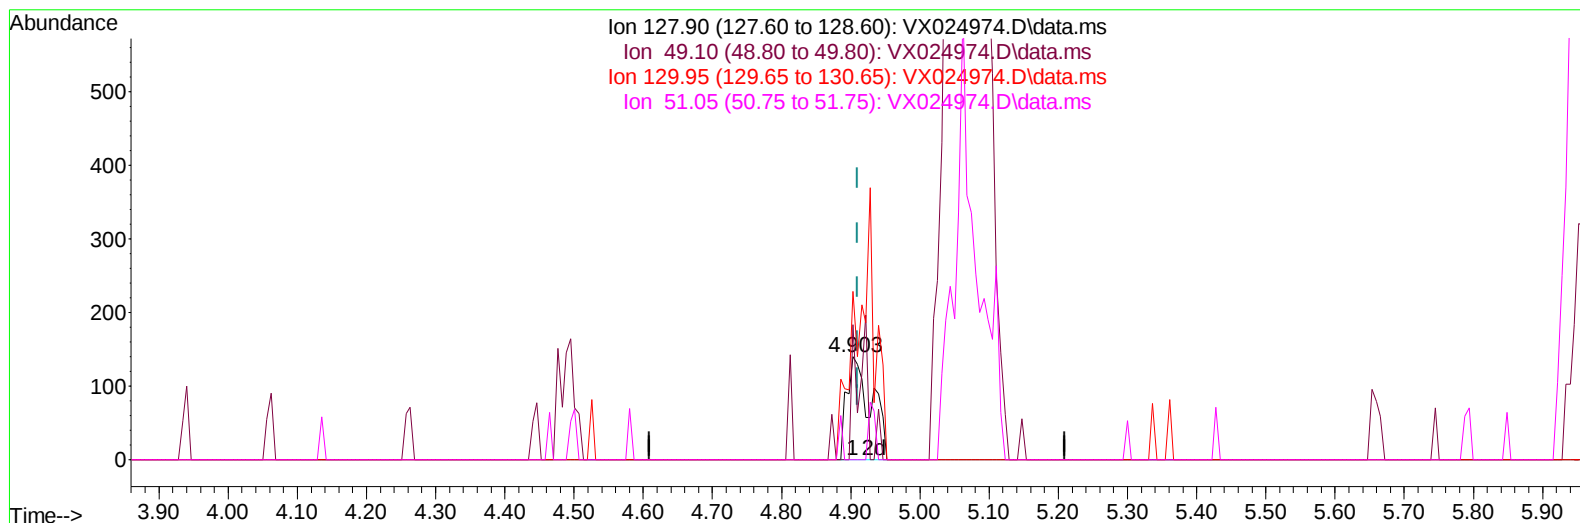

(23) Bromochloromethane (T)

4.903min (-0.006) 0.13 ug/L m

response 335

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 127.90 | 100.00 | 100.00  |
| 49.10  | 122.50 | 130.71  |
| 129.95 | 116.30 | 162.86# |
| 51.05  | 36.00  | 0.00#   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

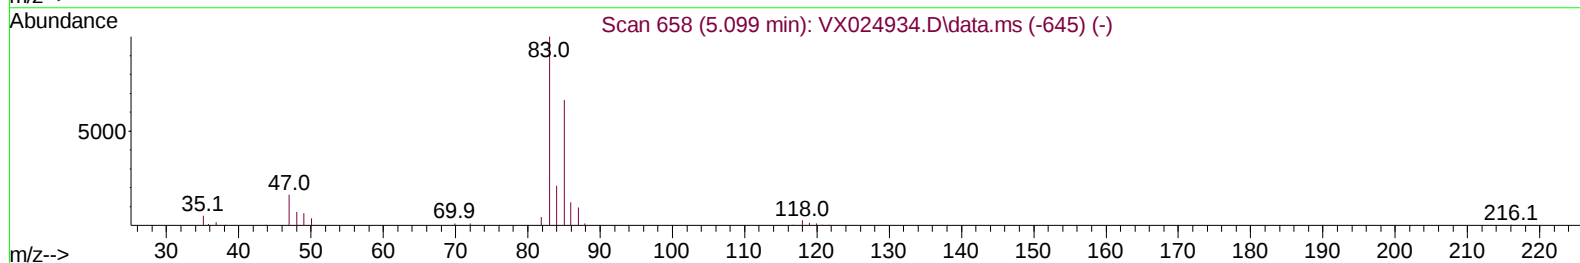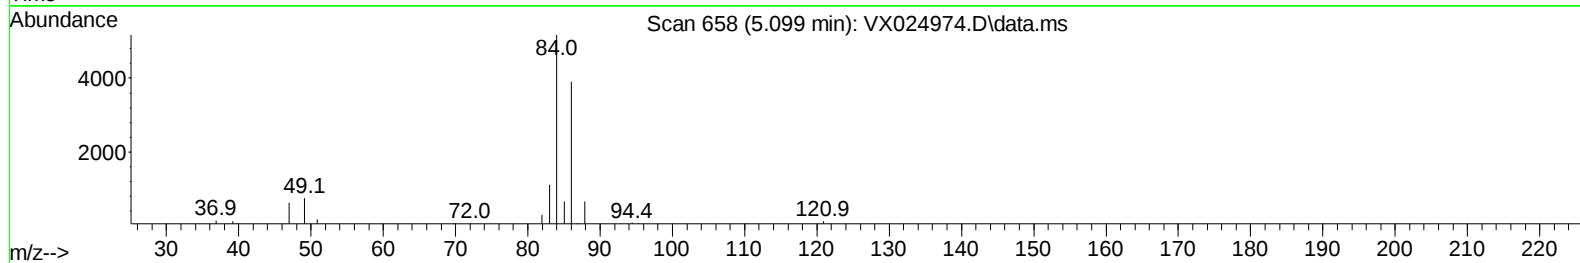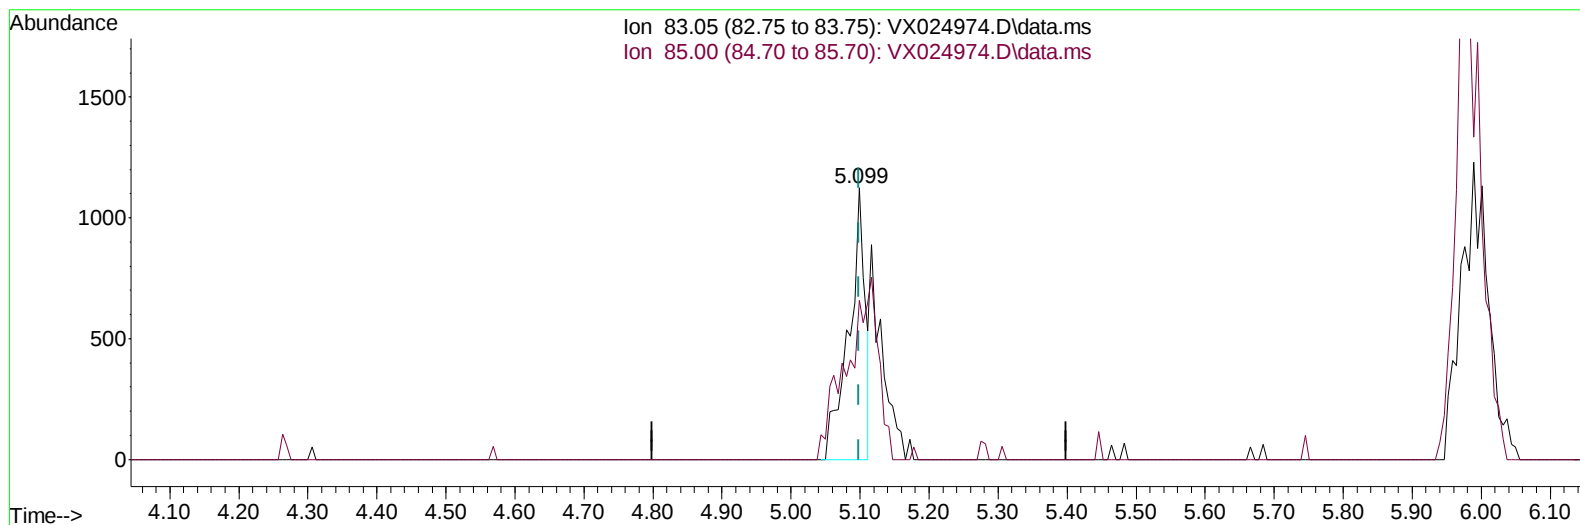

TIC: VX024974.D\data.ms

(25) Chloroform (T)

5.099min (-0.000) 0.16 ug/L

| response | 1845   |        |
|----------|--------|--------|
| Ion      | Exp%   | Act%   |
| 83.05    | 100.00 | 100.00 |
| 85.00    | 67.20  | 58.72  |
| 0.00     | 0.00   | 0.00   |
| 0.00     | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
Data File : VX024974.D  
Acq On : 27 Oct 2021 14:44  
Operator : JC/MD  
Sample : MDL01  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MDL01

Manual Integrations  
APPROVED

MMDadoda  
10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Oct 28 03:09:30 2021  
Response via : Initial Calibration

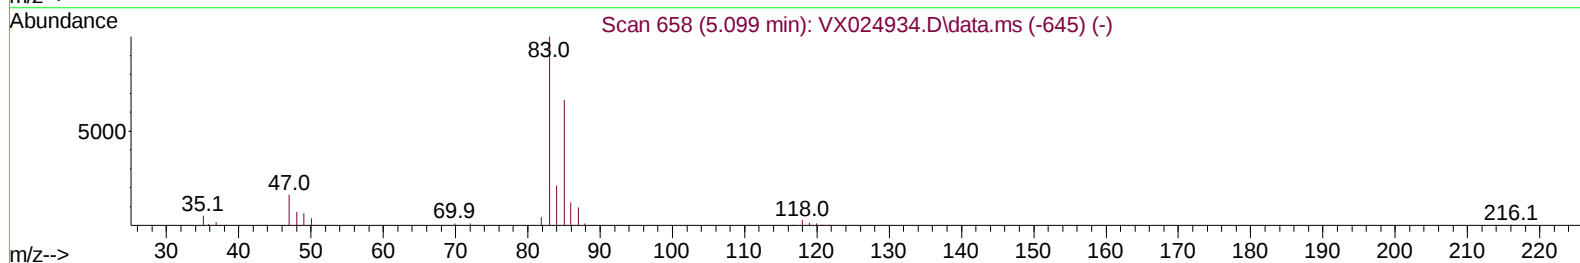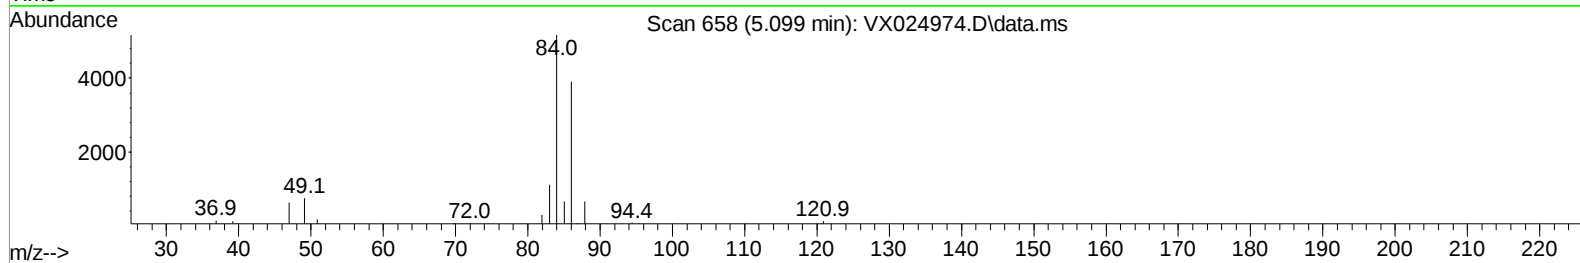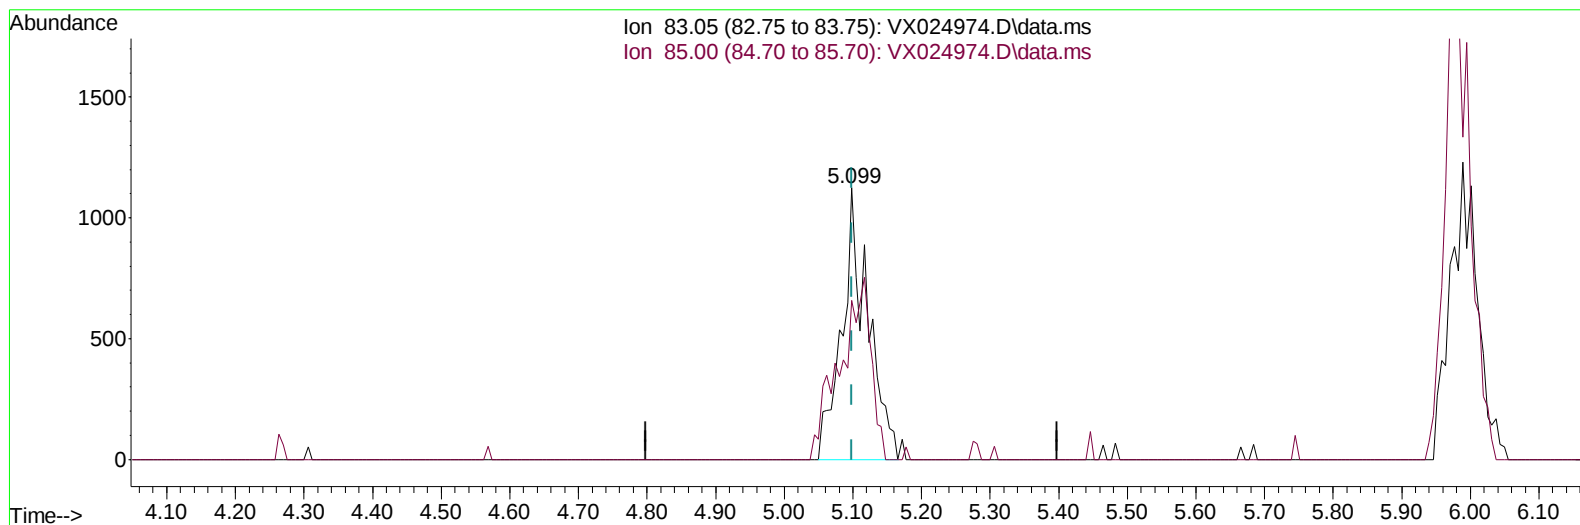

TIC: VX024974.D\data.ms

(25) Chloroform (T)

5.099min (-0.000) 0.25 ug/L m

response 2944

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 83.05 | 100.00 | 100.00 |
| 85.00 | 67.20  | 58.72  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

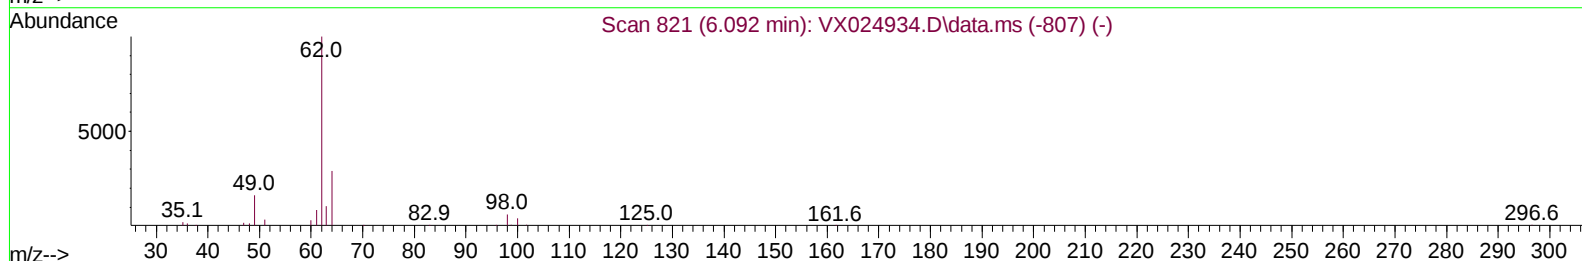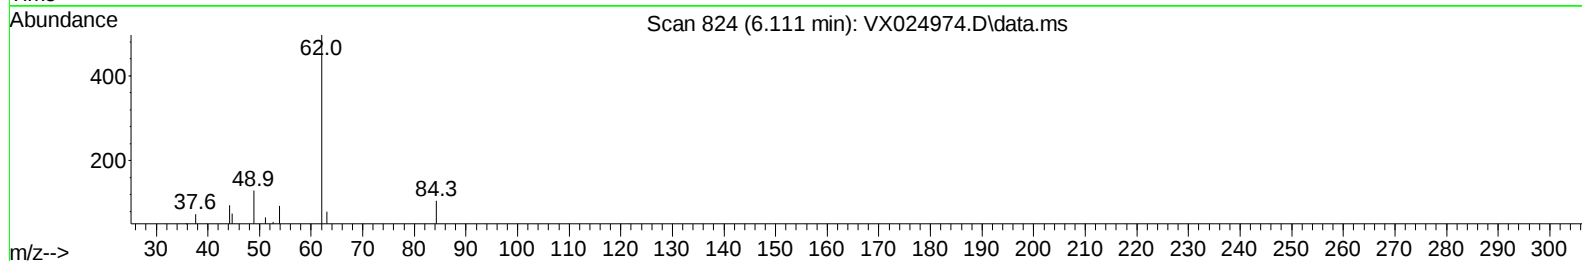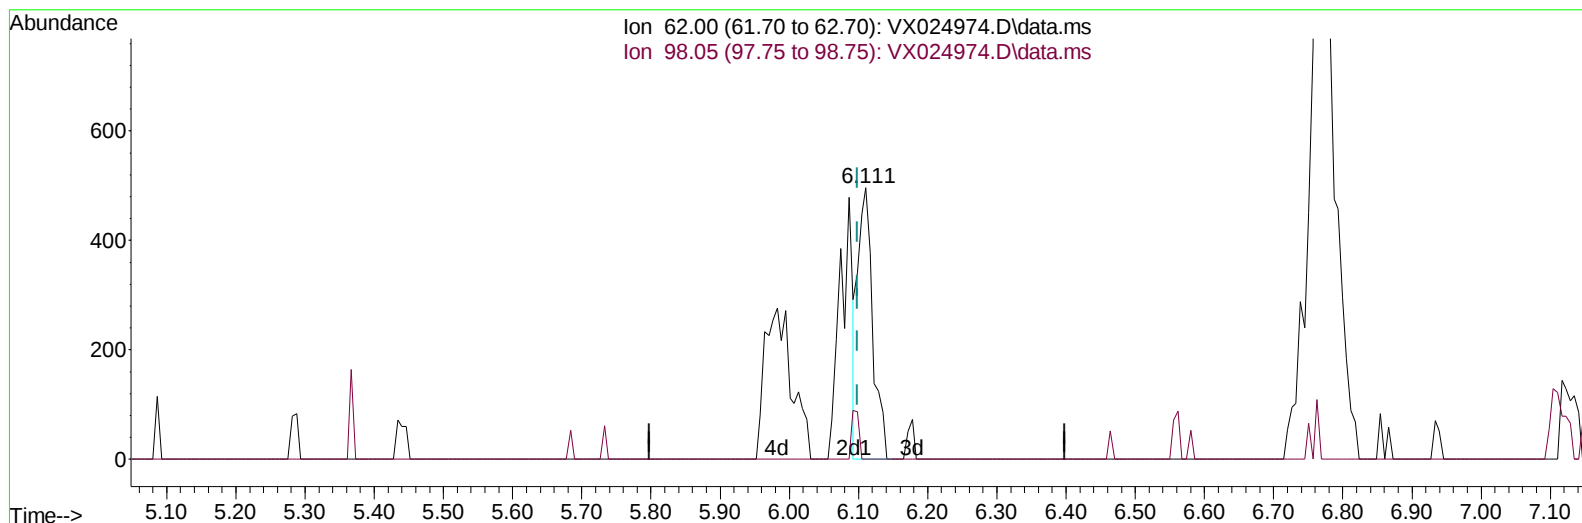

TIC: VX024974.D\data.ms

(27) 1,2-Dichloroethane (T)

6.111min (+ 0.012) 0.10 ug/L

response 736

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 62.00 | 100.00 | 100.00 |
| 98.05 | 5.10   | 0.00#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

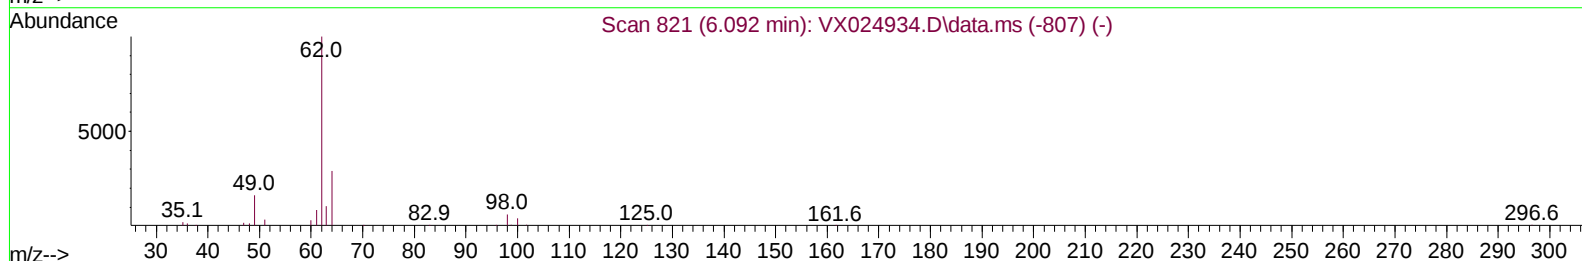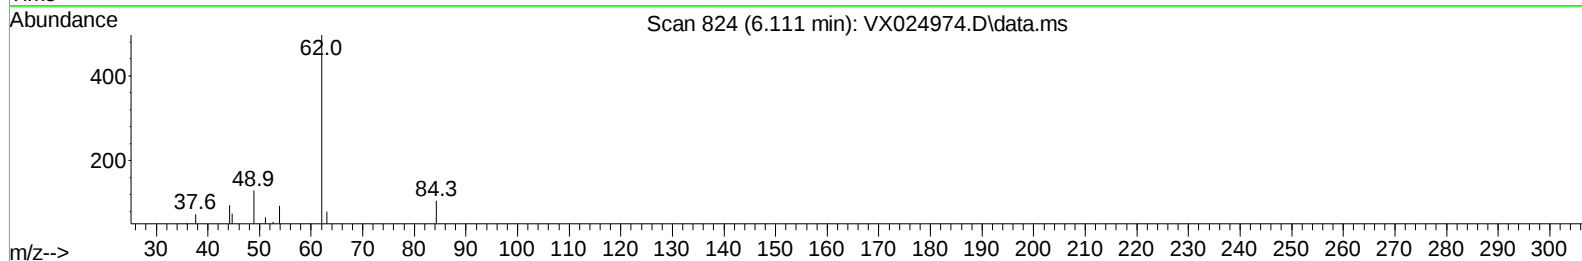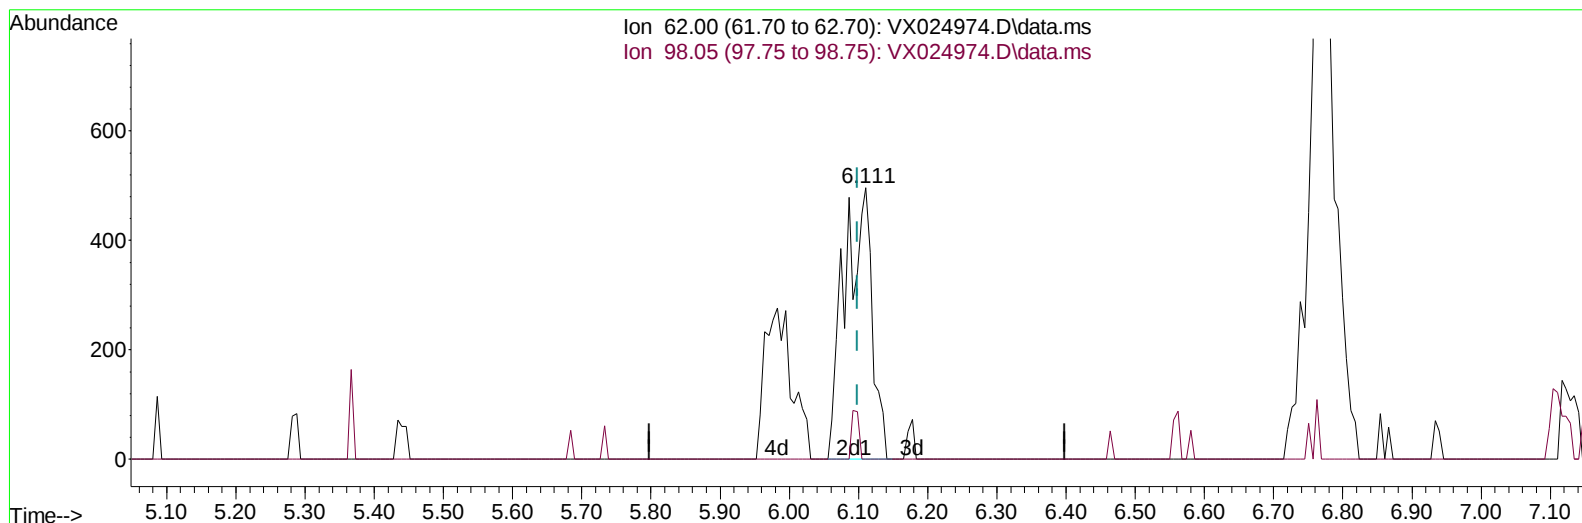

TIC: VX024974.D\data.ms

(27) 1,2-Dichloroethane (T)

6.111min (+ 0.012) 0.19 ug/L m

response 1353

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 62.00 | 100.00 | 100.00 |
| 98.05 | 5.10   | 0.00#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

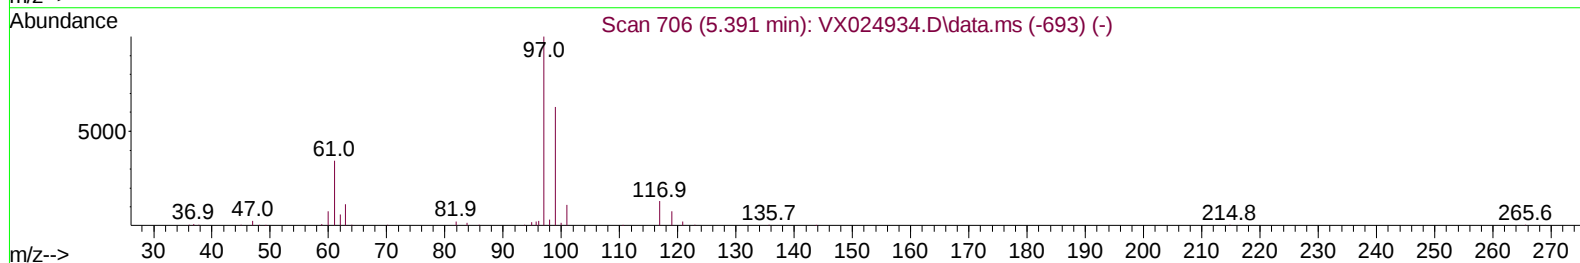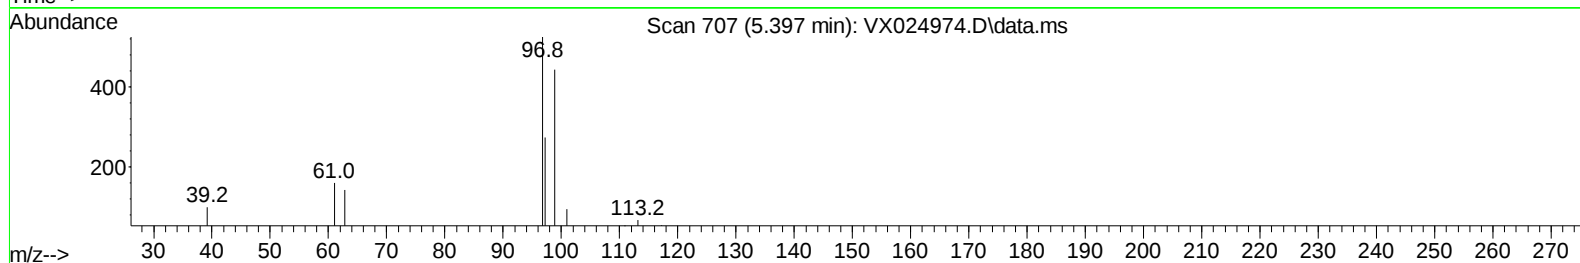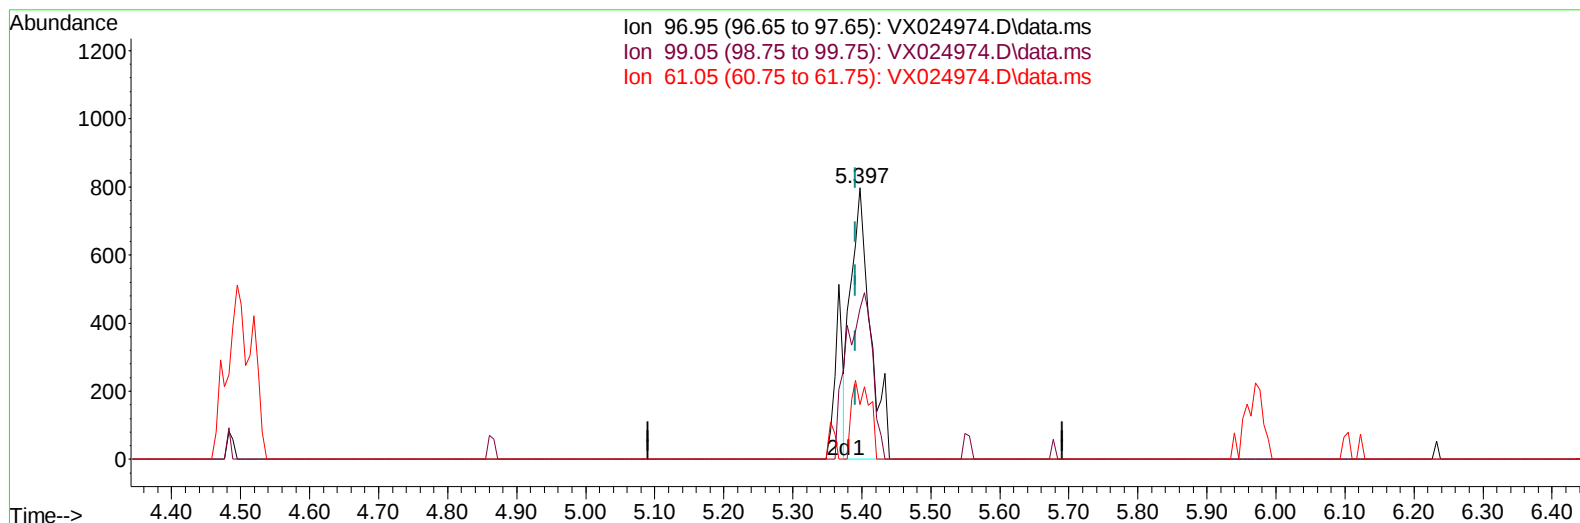

TIC: VX024974.D\data.ms

**(29) 1,1,1-Trichloroethane (T)**

**5.397min (+ 0.006) 0.14 ug/L**

**response 1573**

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 96.95 | 100.00 | 100.00 |
| 99.05 | 62.80  | 79.91# |
| 61.05 | 33.80  | 25.81# |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
Data File : VX024974.D  
Acq On : 27 Oct 2021 14:44  
Operator : JC/MD  
Sample : MDL01  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MDL01

Manual Integrations  
APPROVED

MMDadoda  
10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Oct 28 03:09:30 2021  
Response via : Initial Calibration

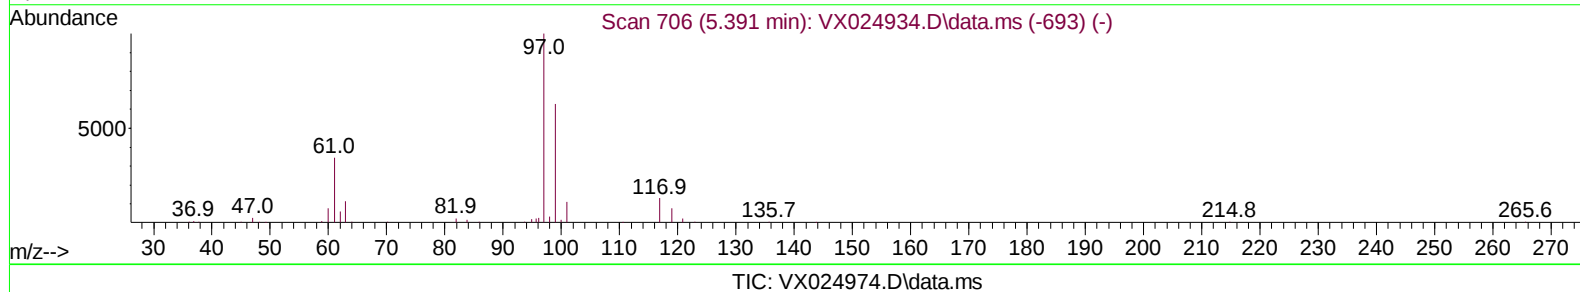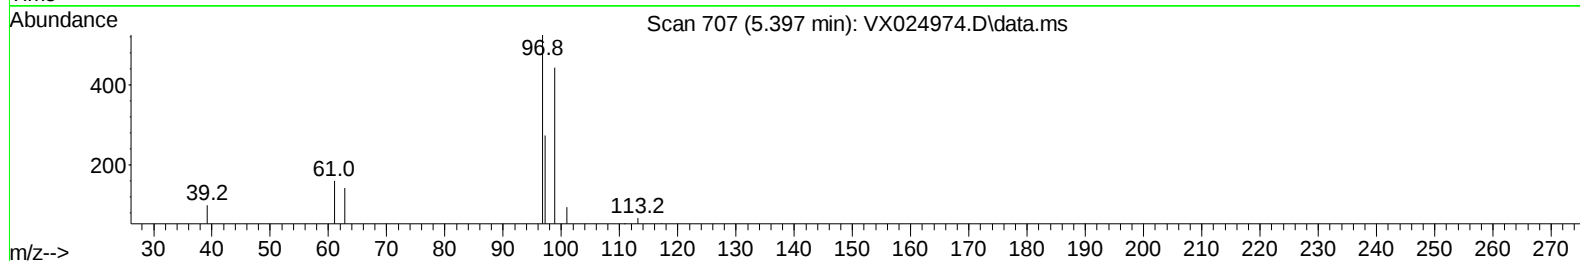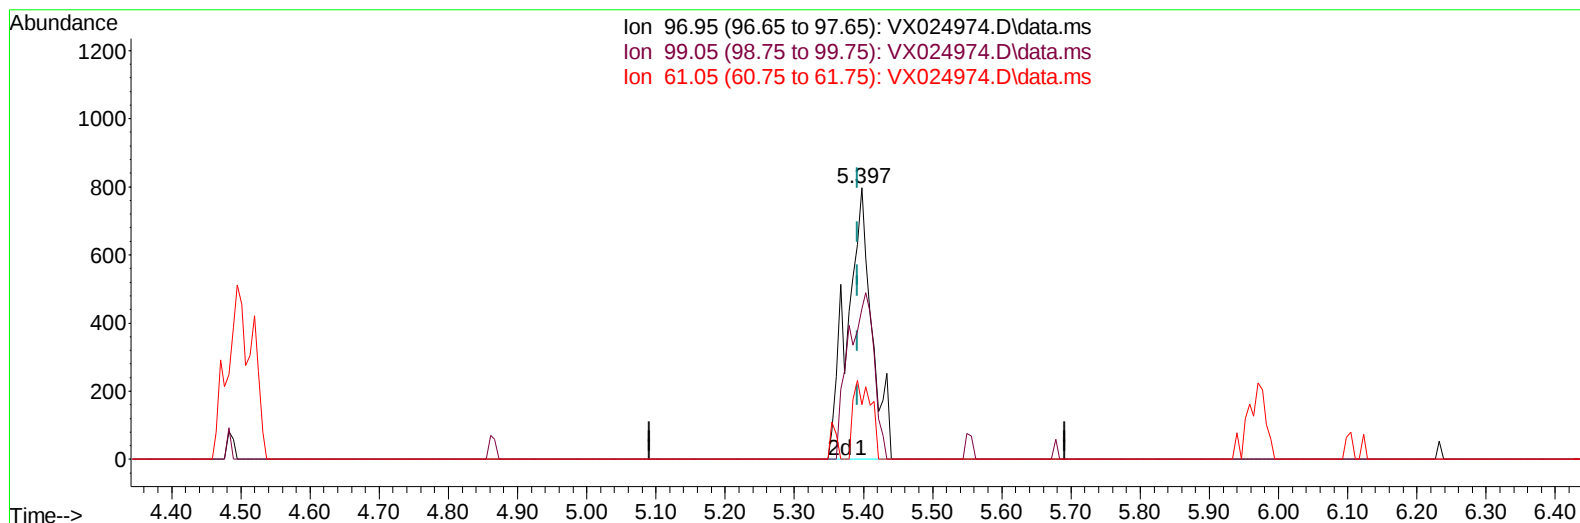

(29) 1,1,1-Trichloroethane (T)

5.397min (+ 0.006) 0.17 ug/L m

response 1973

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 96.95 | 100.00 | 100.00 |
| 99.05 | 62.80  | 63.71  |
| 61.05 | 33.80  | 20.58# |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

| Compound                      | R.T.     | QIon  | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|----------|-------|----------|--------|----------|----------|
| -----                         |          |       |          |        |          |          |
| Internal Standards            |          |       |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 6.769    | 114   | 72058    | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 10.061   | 117   | 67027    | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 12.024   | 152   | 33950    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |          |       |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.368    | 65    | 10803    | 5.107  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 40 | - 130 | Recovery | =      | 102.200% |          |
| 7) Chloroethane-d5            | 1.672    | 69    | 8281     | 4.345  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 130 | Recovery | =      | 86.800%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.306    | 63    | 27269    | 3.458  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 125 | Recovery | =      | 69.200%  |          |
| 20) 2-Butanone-d5             | 4.483    | 46    | 33531    | 43.353 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 40 | - 130 | Recovery | =      | 86.700%  |          |
| 24) Chloroform-d              | 5.068    | 84    | 48980    | 4.809  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 | Recovery | =      | 96.200%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.964    | 65    | 25776    | 4.631  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 | Recovery | =      | 92.600%  |          |
| 32) Benzene-d6                | 5.983    | 84    | 78553    | 5.030  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 | Recovery | =      | 100.600% |          |
| 36) 1,2-Dichloropropane-d6    | 7.318    | 67    | 22010    | 4.417  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 140 | Recovery | =      | 88.400%  |          |
| 41) Toluene-d8                | 8.653    | 98    | 78585    | 5.019  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 | Recovery | =      | 100.400% |          |
| 43) trans-1,3-Dichloroprop... | 8.952    | 79    | 11917    | 5.211  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 55 | - 130 | Recovery | =      | 104.200% |          |
| 46) 2-Hexanone-d5             | 9.390    | 63    | 37156    | 45.143 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 45 | - 130 | Recovery | =      | 90.280%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 11.195   | 84    | 17668    | 4.639  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 120 | Recovery | =      | 92.800%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.323   | 152   | 28028    | 4.899  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 80 | - 120 | Recovery | =      | 98.000%  |          |
| Target Compounds              |          |       |          |        |          |          |
|                               |          |       |          |        | Qvalue   |          |
| 2) Dichlorodifluoromethane    | 1.166    | 85    | 1211     | 0.146  | ug/L     | 97       |
| 3) Chloromethane              | 1.288    | 50    | 379      | 0.131  | ug/L     | 93       |
| 5) Vinyl chloride             | 1.374    | 62    | 590      | 0.167  | ug/L #   | 1        |
| 6) Bromomethane               | 1.617    | 94    | 461      | 0.167  | ug/L #   | 53       |
| 8) Chloroethane               | 1.697    | 64    | 384      | 0.181  | ug/L #   | 82       |
| 9) Trichlorofluoromethane     | 1.892    | 101   | 1503     | 0.143  | ug/L #   | 77       |
| 10) 1,1,2-Trichloro-1,2,2-... | 2.325    | 101   | 1481     | 0.269  | ug/L #   | 79       |
| 12) 1,1-Dichloroethene        | 2.319    | 96    | 938      | 0.212  | ug/L #   | 1        |
| 13) Acetone                   | 2.422    | 43    | 1513m    | 2.608  | ug/L     |          |
| 14) Carbon disulfide          | 2.520    | 76    | 1656     | 0.137  | ug/L #   | 66       |
| 16) Methylene chloride        | 2.794    | 84    | 1071     | 0.209  | ug/L #   | 66       |
| 17) Methyl tert-butyl Ether   | 3.123    | 73    | 1988     | 0.156  | ug/L     | 96       |
| 18) trans-1,2-Dichloroethene  | 3.099    | 96    | 715      | 0.139  | ug/L     | 86       |
| 19) 1,1-Dichloroethane        | 3.617    | 63    | 1418     | 0.157  | ug/L #   | 65       |
| 21) 2-Butanone                | 4.599    | 43    | 1218     | 1.427  | ug/L #   | 62       |
| 22) cis-1,2-Dichloroethene    | 4.501    | 96    | 1227     | 0.222  | ug/L #   | 63       |
| 23) Bromochloromethane        | 4.903    | 128   | 335m     | 0.134  | ug/L     |          |
| 25) Chloroform                | 5.099    | 83    | 2944m    | 0.251  | ug/L     |          |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|-------|--------|----------|
| -----                         |        |      |          |       |        |          |
| 27) 1,2-Dichloroethane        | 6.111  | 62   | 1353m    | 0.189 | ug/L   |          |
| 29) 1,1,1-Trichloroethane     | 5.397  | 97   | 1973m    | 0.170 | ug/L   |          |
| 30) Cyclohexane               | 5.483  | 56   | 1063     | 0.147 | ug/L # | 88       |
| 31) Carbon tetrachloride      | 5.684  | 117  | 1891     | 0.189 | ug/L # | 59       |
| 33) Benzene                   | 6.037  | 78   | 3174     | 0.162 | ug/L   | 100      |
| 34) Trichloroethene           | 7.135  | 95   | 1240     | 0.194 | ug/L # | 76       |
| 35) Methylcyclohexane         | 7.385  | 83   | 1282     | 0.144 | ug/L # | 83       |
| 37) 1,2-Dichloropropane       | 7.440  | 63   | 782      | 0.163 | ug/L # | 87       |
| 38) Bromodichloromethane      | 7.836  | 83   | 1418     | 0.178 | ug/L # | 56       |
| 39) cis-1,3-Dichloropropene   | 8.372  | 75   | 1078     | 0.134 | ug/L   | 92       |
| 40) 4-Methyl-2-pentanone      | 8.574  | 43   | 2869     | 1.345 | ug/L # | 81       |
| 42) Toluene                   | 8.720  | 91   | 5169     | 0.226 | ug/L   | 80       |
| 44) trans-1,3-Dichloropropene | 8.982  | 75   | 1442     | 0.197 | ug/L # | 81       |
| 45) 1,1,2-Trichloroethane     | 9.153  | 97   | 583      | 0.151 | ug/L # | 66       |
| 47) Tetrachloroethene         | 9.281  | 164  | 837      | 0.188 | ug/L # | 50       |
| 48) 2-Hexanone                | 9.439  | 43   | 2379     | 1.528 | ug/L   | 93       |
| 49) Dibromochloromethane      | 9.531  | 129  | 766      | 0.152 | ug/L   | 90       |
| 50) 1,2-Dibromoethane         | 9.610  | 107  | 788      | 0.204 | ug/L # | 55       |
| 51) Chlorobenzene             | 10.085 | 112  | 2244     | 0.154 | ug/L   | 87       |
| 52) Ethylbenzene              | 10.201 | 91   | 4232     | 0.157 | ug/L   | 100      |
| 53) m,p-xylene                | 10.305 | 106  | 1749     | 0.182 | ug/L   | 72       |
| 54) o-xylene                  | 10.646 | 106  | 1454     | 0.156 | ug/L   | 64       |
| 55) Styrene                   | 10.659 | 104  | 2332     | 0.149 | ug/L   | 95       |
| 57) 1,1,2,2-Tetrachloroethane | 11.207 | 83   | 767      | 0.173 | ug/L # | 63       |
| 59) Bromoform                 | 10.799 | 173  | 452      | 0.192 | ug/L # | 75       |
| 60) Isopropylbenzene          | 10.963 | 105  | 3641     | 0.135 | ug/L # | 88       |
| 61) 1,2,3-Trichloropropane    | 11.232 | 75   | 549      | 0.166 | ug/L # | 73       |
| 62) 1,3,5-Trimethylbenzene    | 11.451 | 105  | 3191     | 0.135 | ug/L   | 91       |
| 63) 1,2,4-Trimethylbenzene    | 11.756 | 105  | 3517     | 0.145 | ug/L   | 98       |
| 64) 1,3-Dichlorobenzene       | 11.975 | 146  | 1252     | 0.111 | ug/L # | 44       |
| 65) 1,4-Dichlorobenzene       | 12.042 | 146  | 1676     | 0.149 | ug/L # | 75       |
| 67) 1,2-Dichlorobenzene       | 12.335 | 146  | 1273     | 0.123 | ug/L # | 73       |
| 68) 1,2-Dibromo-3-chloropr... | 12.951 | 75   | 109      | 0.135 | ug/L # | 32       |
| 69) 1,3,5-Trichlorobenzene    | 13.115 | 180  | 1165     | 0.136 | ug/L   | 94       |
| 70) 1,2,4-trichlorobenzene    | 13.591 | 180  | 726      | 0.107 | ug/L # | 87       |
| 71) Naphthalene               | 13.786 | 128  | 1088     | 0.089 | ug/L # | 83       |
| 72) 1,2,3-Trichlorobenzene    | 13.969 | 180  | 625      | 0.103 | ug/L # | 78       |
| -----                         |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102721\  
 Data File : VX024974.D  
 Acq On : 27 Oct 2021 14:44  
 Operator : JC/MD  
 Sample : MDL01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampled :  
 MDL01

Manual Integrations  
 APPROVED

MMDadoda  
 10/28/2021 12:34:17 PM

Quant Time: Oct 28 03:12:19 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 28 03:09:30 2021  
 Response via : Initial Calibration

