

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024966.D
 Acq On : 27 Oct 2021 11:37
 Operator : JC/MD
 Sample : M4318-09
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Oct 28 03:10:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	82658	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	77391	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	36663	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	11530	4.751	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.672	69	9619	4.399	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%
11) 1,1-Dichloroethene-d2	2.307	63	28285	3.127	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.600%
20) 2-Butanone-d5	4.489	46	36564	41.212	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.420%
24) Chloroform-d	5.062	84	53259	4.559	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.964	65	27187	4.258	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.977	84	85495	4.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	7.312	67	25573	4.445	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%
41) Toluene-d8	8.653	98	86512	4.785	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	8.952	79	12917	4.892	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.800%
46) 2-Hexanone-d5	9.391	63	38942	40.977	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.960%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	18905	4.299	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.000%
66) 1,2-Dichlorobenzene-d4	12.323	152	29749	4.815	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds						Qvalue
16) Methylene chloride	2.794	84	3646	0.619	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024966.D
Acq On : 27 Oct 2021 11:37
Operator : JC/MD
Sample : M4318-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Oct 28 03:10:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 03:09:30 2021
Response via : Initial Calibration

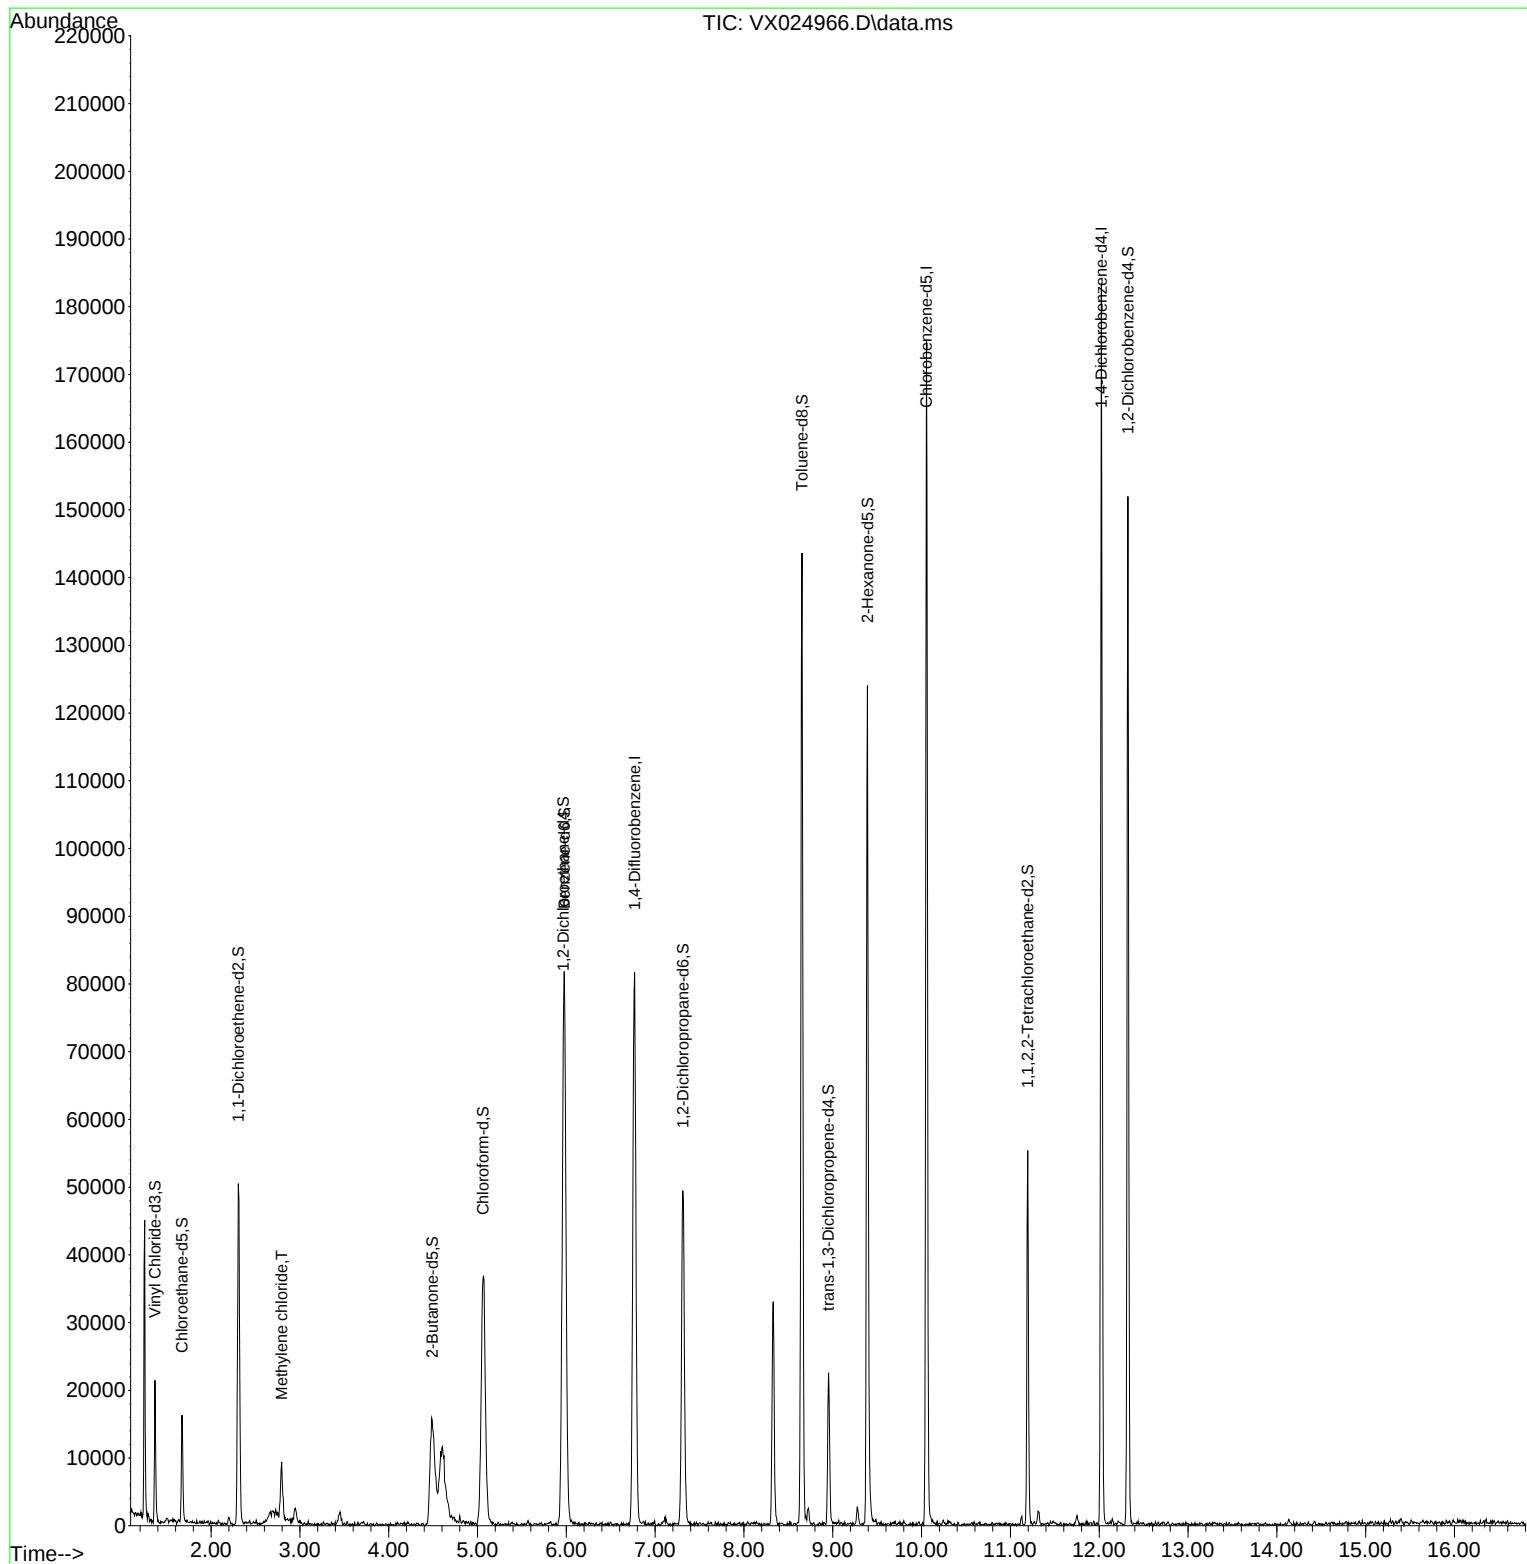

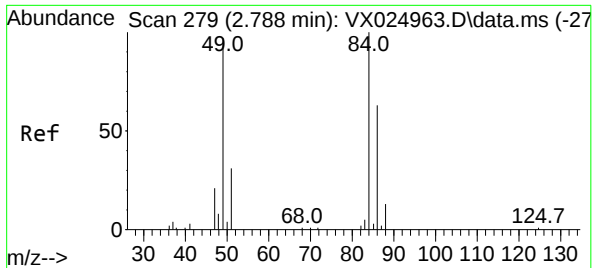

#16
Methylene chloride
Concen: 0.619 ug/L
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX024966.D
Acq: 27 Oct 2021 11:37

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	3646
Ion	Ratio	Lower	Upper
84	100		
86	70.5	49.5	91.9
49	67.6	62.7	116.5

