

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024968.D
 Acq On : 27 Oct 2021 12:24
 Operator : JC/MD
 Sample : M4304-14
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Oct 28 03:10:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	69246	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	63814	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	30639	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	10366	5.099	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.000%
7) Chloroethane-d5	1.672	69	8519	4.651	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.306	63	27023	3.566	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.400%
20) 2-Butanone-d5	4.483	46	34298	46.146	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.300%
24) Chloroform-d	5.068	84	49177	5.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.964	65	25143	4.701	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.982	84	77061	5.183	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
36) 1,2-Dichloropropane-d6	7.318	67	22213	4.683	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.600%
41) Toluene-d8	8.653	98	76833	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%
43) trans-1,3-Dichloroprop...	8.951	79	12206	5.606	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	112.200%
46) 2-Hexanone-d5	9.390	63	35002	44.667	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.340%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	18331	5.056	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	12.323	152	28252	5.472	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						
16) Methylene chloride	2.800	84	2059	0.417	ug/L	Qvalue # 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024968.D
Acq On : 27 Oct 2021 12:24
Operator : JC/MD
Sample : M4304-14
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Oct 28 03:10:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 03:09:30 2021
Response via : Initial Calibration

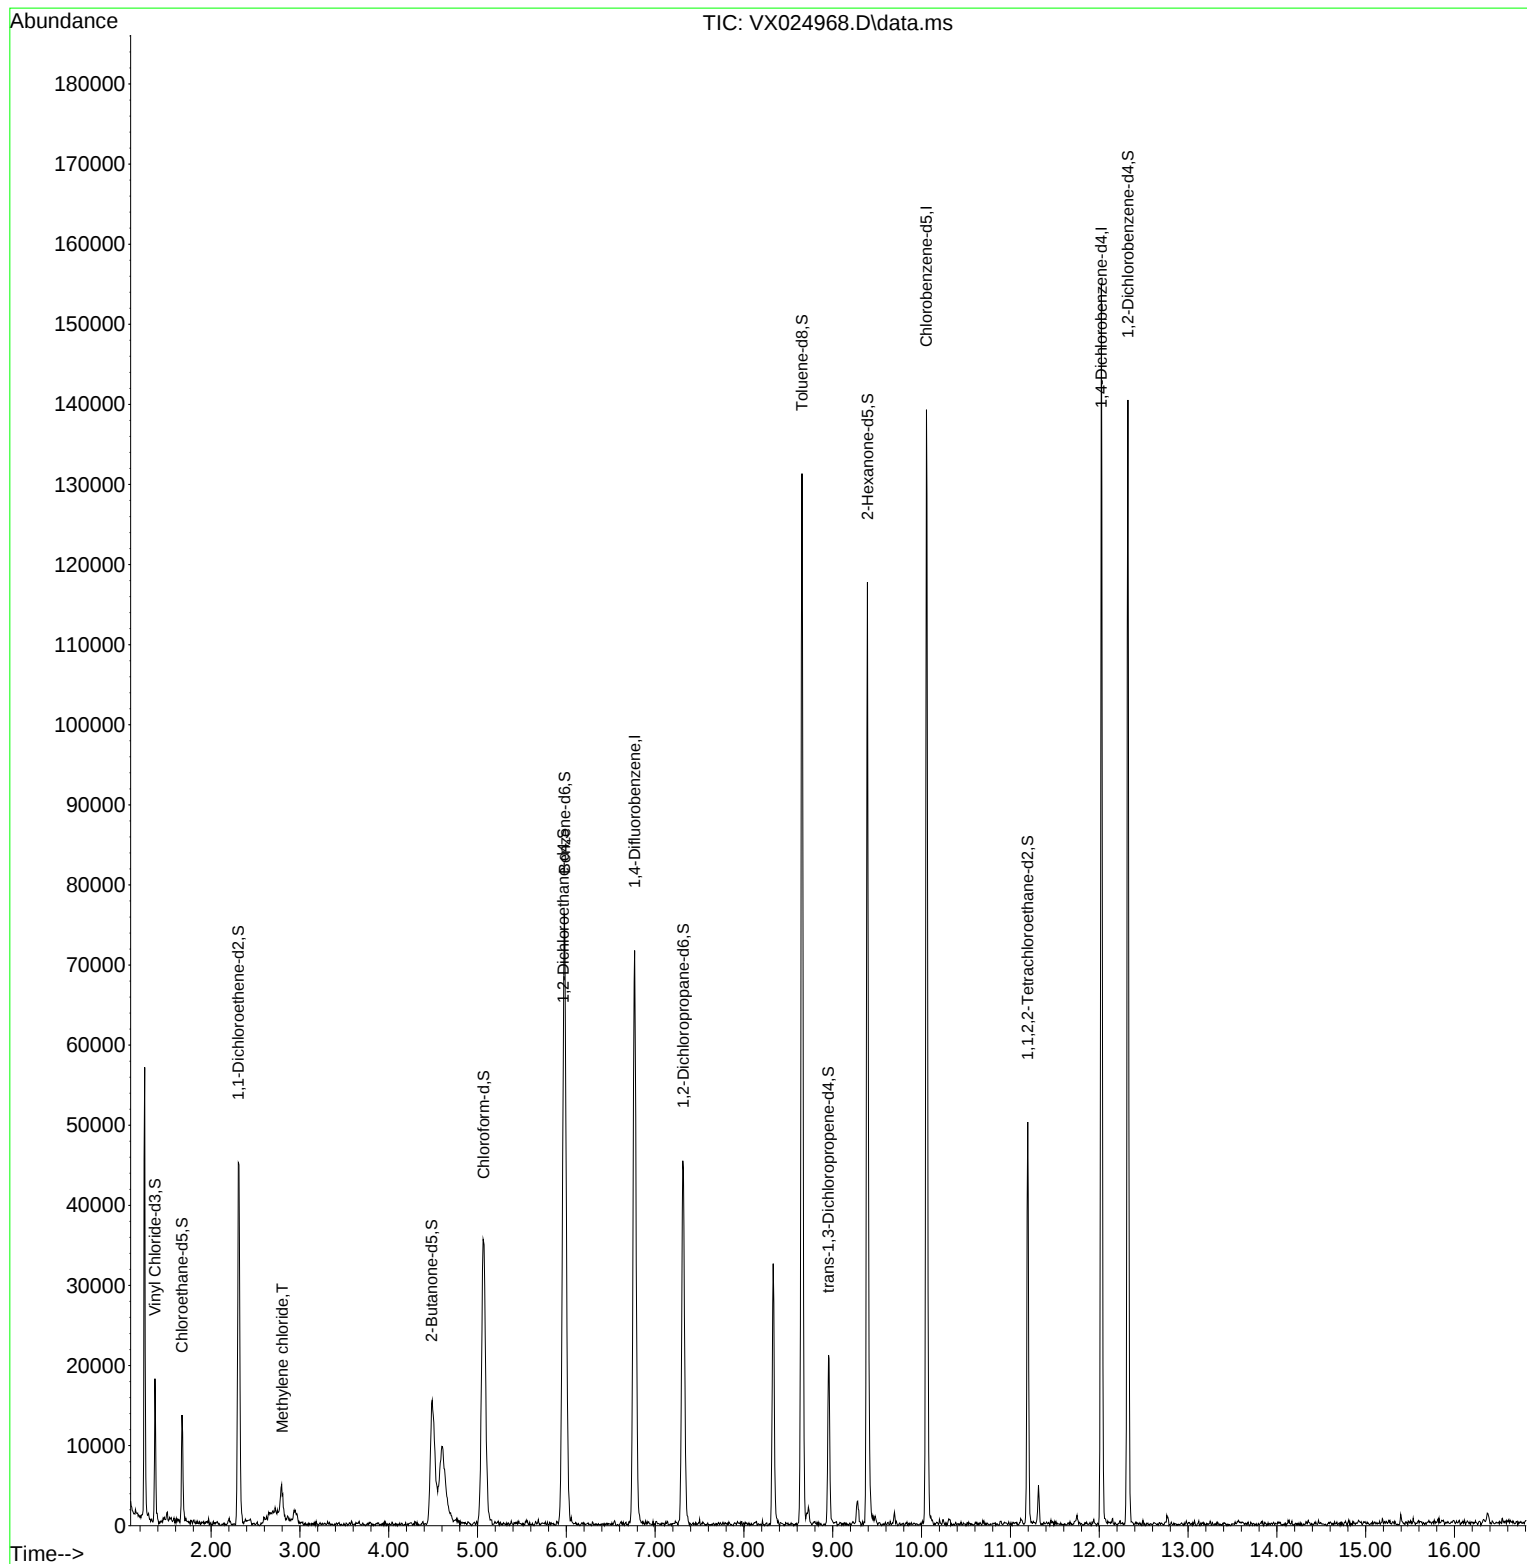

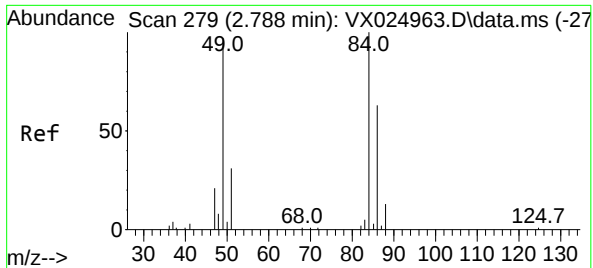

#16
Methylene chloride
Concen: 0.417 ug/L
RT: 2.800 min Scan# 281
Delta R.T. 0.012 min
Lab File: VX024968.D
Acq: 27 Oct 2021 12:24

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 2059
Ion Ratio Lower Upper
84 100
86 36.0 49.5 91.9#
49 59.3 62.7 116.5#

