

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-01

Manual Integrations
 APPROVED

MMDadoda
 10/28/2021 12:34:09 PM

Quant Time: Oct 28 03:11:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	68668	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	64046	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31758	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	10985	5.449	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	109.000%	
7) Chloroethane-d5	1.673	69	8557	4.711	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.200%	
11) 1,1-Dichloroethene-d2	2.307	63	27233	3.624	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	4.489	46	34722m	47.109	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.220%	
24) Chloroform-d	5.062	84	49228	5.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	5.964	65	25898	4.882	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.600%	
32) Benzene-d6	5.989	84	79160	5.305	ug/L	0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.000%	
36) 1,2-Dichloropropane-d6	7.312	67	22174	4.657	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.200%	
41) Toluene-d8	8.653	98	80085	5.353	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.000%	
43) trans-1,3-Dichloroprop...	8.958	79	11802	5.401	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	108.000%	
46) 2-Hexanone-d5	9.391	63	37997	48.314	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.620%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19564	5.376	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4	12.323	152	29083	5.434	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.600%	
Target Compounds					Qvalue	
13) Acetone	2.404	43	2653m	4.799	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024970.D
Acq On : 27 Oct 2021 13:12
Operator : JC/MD
Sample : M4319-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
P071-TW001-01

Manual Integrations
APPROVED

MMDadoda
10/28/2021 12:34:09 PM


Quant Time: Oct 28 03:11:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 03:09:30 2021
Response via : Initial Calibration

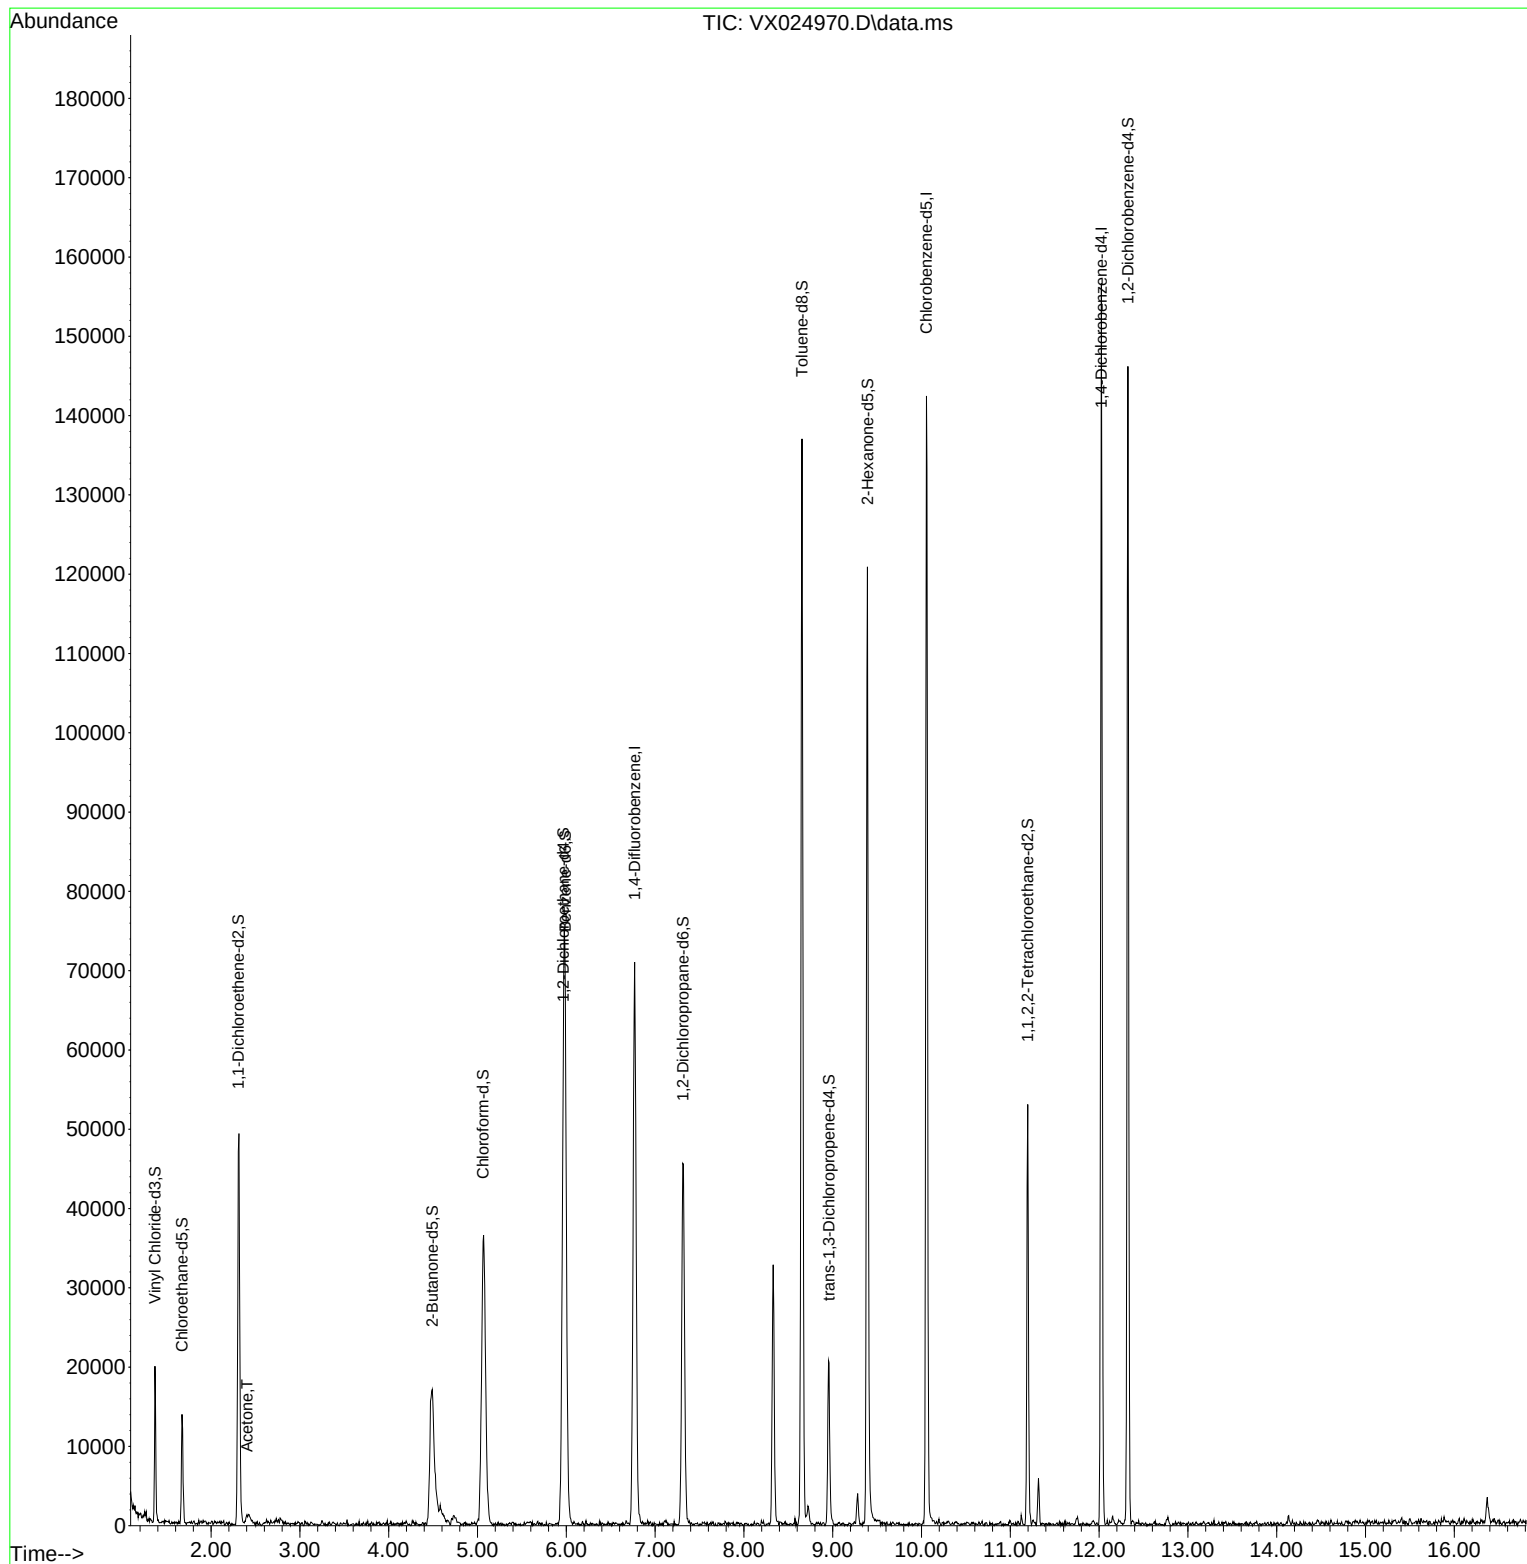

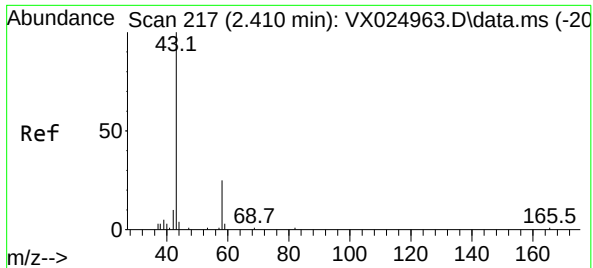

#13
Acetone
Concen: 4.799 ug/L m
RT: 2.404 min Scan# 216
Delta R.T. -0.006 min
Lab File: VX024970.D
Acq: 27 Oct 2021 13:12

Instrument :
MSVOA_X
ClientSampleId :
P071-TW001-01

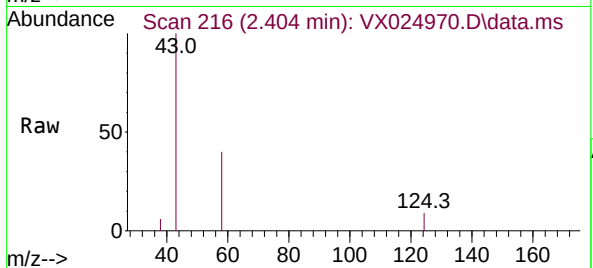

Tgt Ion: 43 Resp: 2653
Ion Ratio Lower Upper
43 100
58 18.1 0.0 64.2

Manual Integrations
APPROVED

MMDadoda
10/28/2021 12:34:09 PM

