

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024971.D
 Acq On : 27 Oct 2021 13:36
 Operator : JC/MD
 Sample : M4319-14
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-02

Quant Time: Oct 28 03:11:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 03:09:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	71818	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	68832	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32155	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	10768	5.107	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.200%
7) Chloroethane-d5	1.672	69	8751	4.607	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.306	63	28813	3.666	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	4.489	46	34044	44.164	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.320%
24) Chloroform-d	5.068	84	50169	4.943	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.964	65	26325	4.745	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	5.983	84	79823	4.977	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
36) 1,2-Dichloropropane-d6	7.312	67	23521	4.597	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.000%
41) Toluene-d8	8.653	98	80874	5.029	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
43) trans-1,3-Dichloroprop...	8.952	79	11265	4.797	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.000%
46) 2-Hexanone-d5	9.391	63	37103	43.897	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.800%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	18983	4.854	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	12.323	152	29165	5.382	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.600%
Target Compounds						Qvalue
13) Acetone	2.416	43	2333	4.035	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024971.D
Acq On : 27 Oct 2021 13:36
Operator : JC/MD
Sample : M4319-14
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P071-TW001-02


Quant Time: Oct 28 03:11:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 03:09:30 2021
Response via : Initial Calibration

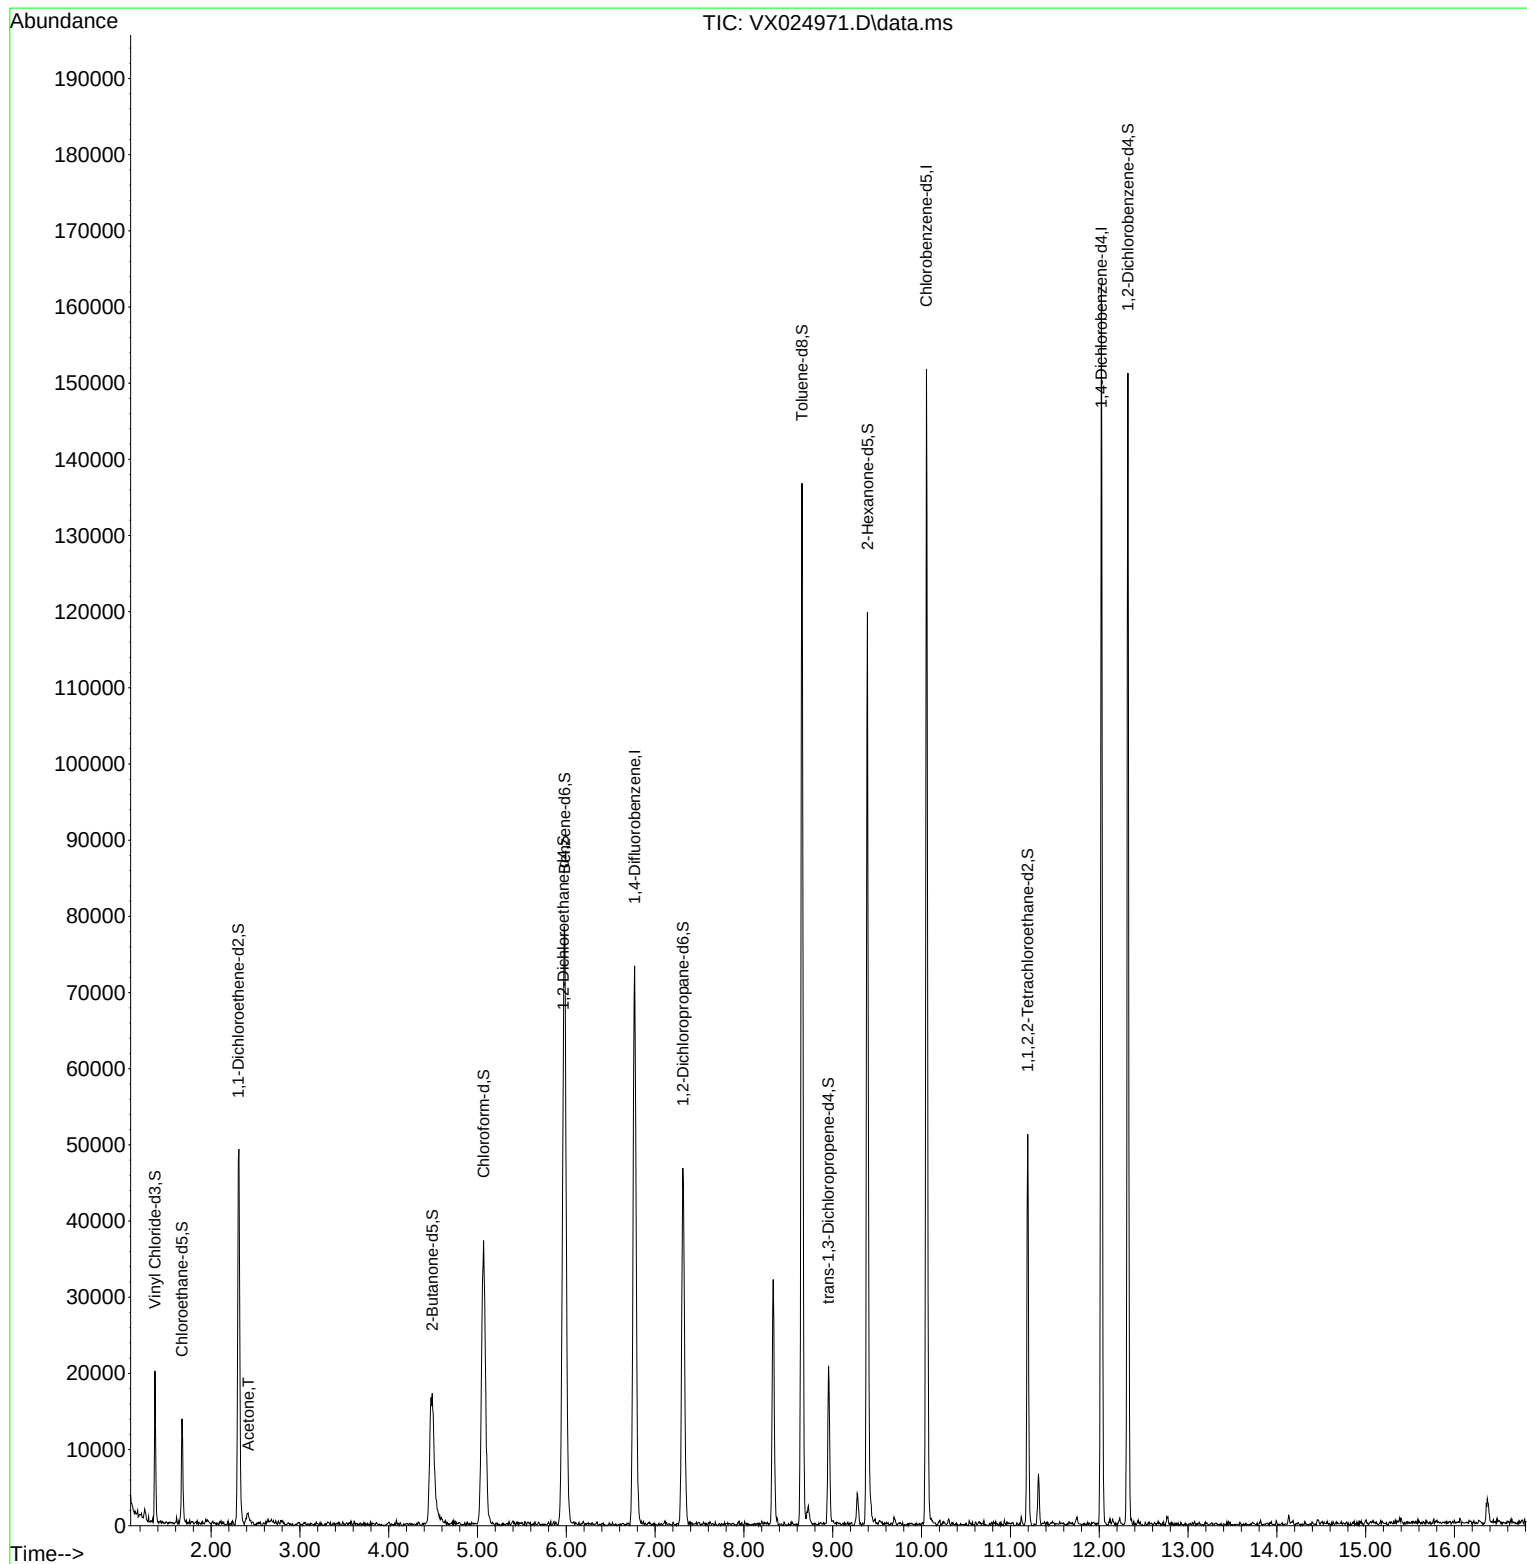

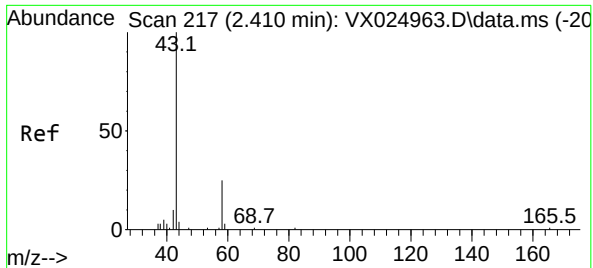

#13
 Acetone
 Concen: 4.035 ug/L
 RT: 2.416 min Scan# 218
 Delta R.T. 0.006 min
 Lab File: VX024971.D
 Acq: 27 Oct 2021 13:36

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-02

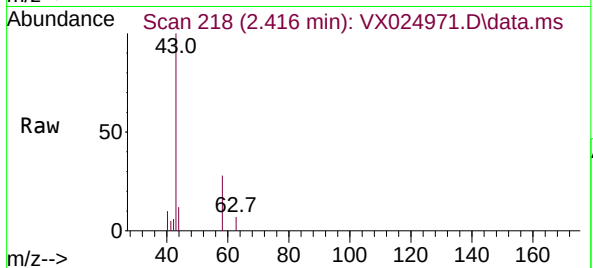

Tgt Ion: 43 Resp: 2333
 Ion Ratio Lower Upper
 43 100
 58 37.1 0.0 64.2

