

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024965.D
 Acq On : 27 Oct 2021 11:07
 Operator : JC/MD
 Sample : VX1027WBL02
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	55	rVB	21870	21922	8.88%	1.013%
2	1.672	92	96	102	rVB	14754	17301	7.01%	0.799%
3	2.306	191	200	209	rBV	51333	83180	33.69%	3.842%
4	2.794	274	280	287	rVB2	4280	8790	3.56%	0.406%
5	3.459	384	389	393	rVB4	1617	2751	1.11%	0.127%
6	4.477	546	556	574	rBV	18478	67796	27.46%	3.131%
7	5.062	640	652	667	rBV2	40728	126317	51.16%	5.834%
8	5.976	790	802	817	rBV4	83946	246927	100.00%	11.405%
9	6.763	923	931	943	rBV	84421	206686	83.70%	9.547%
10	7.311	1013	1021	1028	rBV2	48605	110129	44.60%	5.087%
11	8.330	1179	1188	1196	rBV	34040	58074	23.52%	2.682%
12	8.653	1234	1241	1249	rBV	145517	228323	92.47%	10.546%
13	8.726	1249	1253	1256	rVB2	2456	3133	1.27%	0.145%
14	8.951	1285	1290	1299	rBV3	22898	36277	14.69%	1.676%
15	9.390	1354	1362	1372	rBV	127757	190879	77.30%	8.816%
16	10.055	1466	1471	1481	rBV	174189	240476	97.39%	11.107%
17	11.195	1653	1658	1667	rVB	56880	71012	28.76%	3.280%
18	12.024	1789	1794	1803	rVB	189053	243820	98.74%	11.262%
19	12.323	1837	1843	1850	rVB	159960	201248	81.50%	9.295%




Sum of corrected areas: 2165041

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024965.D
Acq On : 27 Oct 2021 11:07
Operator : JC/MD
Sample : VX1027WBL02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

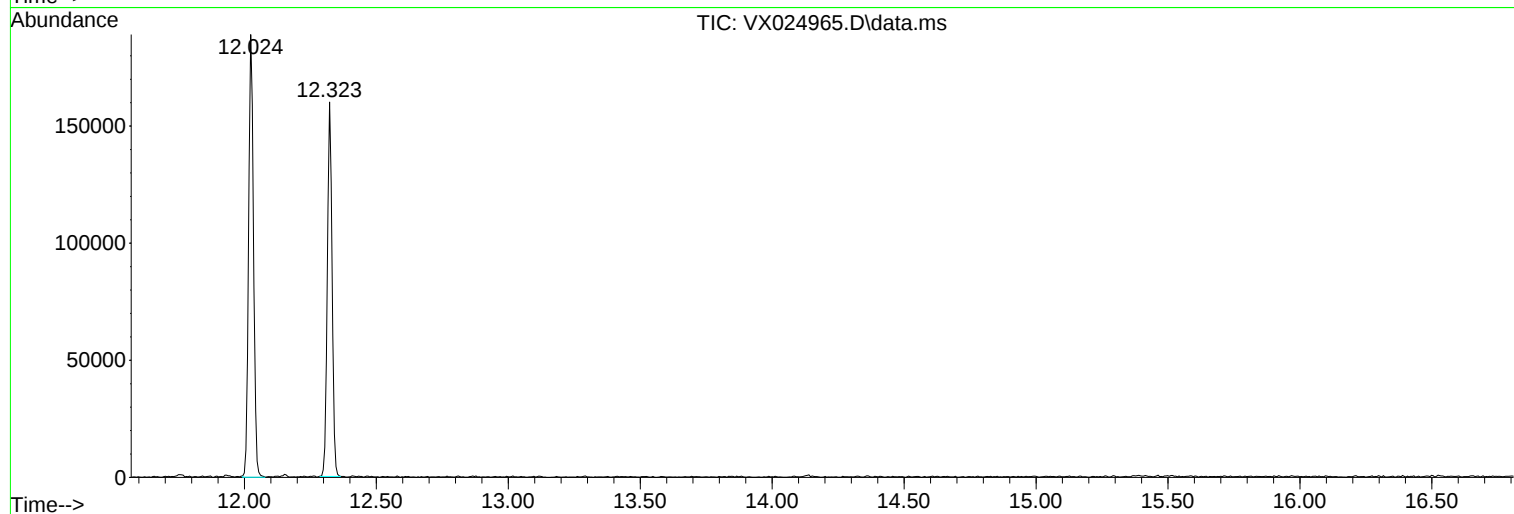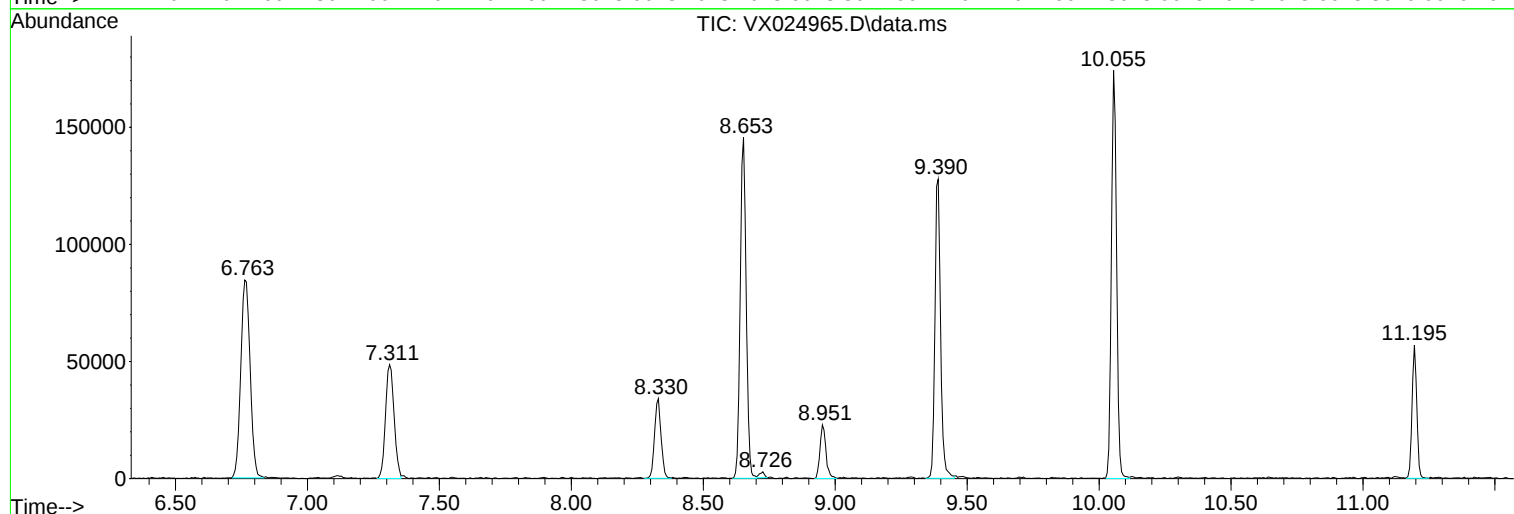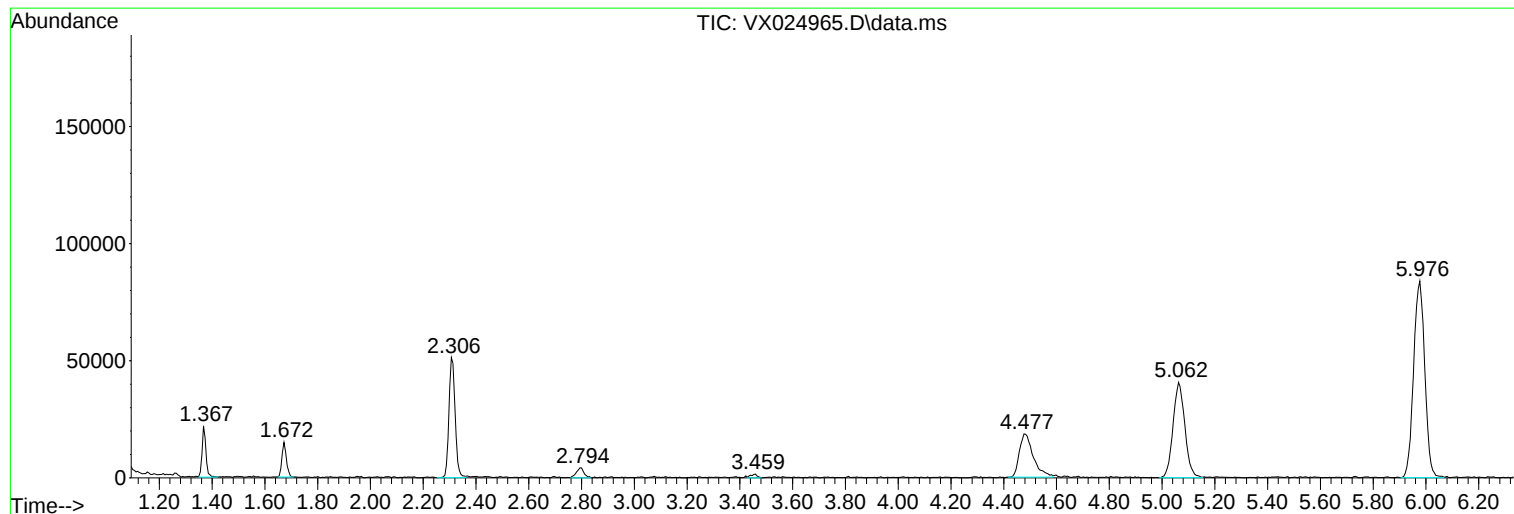

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024965.D
Acq On : 27 Oct 2021 11:07
Operator : JC/MD
Sample : VX1027WBL02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024965.D
Acq On : 27 Oct 2021 11:07
Operator : JC/MD
Sample : VX1027WBL02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
