

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024966.D
 Acq On : 27 Oct 2021 11:37
 Operator : JC/MD
 Sample : M4318-09
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rVB	44227	40236	16.72%	1.850%
2	1.368	43	46	55	rVB	21112	20757	8.62%	0.955%
3	1.672	92	96	104	rBV	15796	18845	7.83%	0.867%
4	2.307	193	200	210	rBV	50335	80561	33.47%	3.705%
5	2.666	251	259	261	rBV3	1411	2767	1.15%	0.127%
6	2.794	275	280	287	rVB2	8621	14960	6.22%	0.688%
7	2.947	301	305	311	rVB4	2111	3974	1.65%	0.183%
8	3.453	380	388	393	rVB5	1898	4140	1.72%	0.190%
9	4.483	548	557	568	rBV	15685	60672	25.21%	2.790%
10	4.605	568	577	579	rBV2	6897	17792	7.39%	0.818%
11	5.068	640	653	669	rBV3	36738	122943	51.08%	5.654%
12	5.977	789	802	814	rBV3	81789	240677	100.00%	11.068%
13	6.769	922	932	945	rBV	81599	200653	83.37%	9.227%
14	7.312	1013	1021	1031	rBV3	49259	110694	45.99%	5.090%
15	8.330	1181	1188	1198	rVB	33028	57726	23.98%	2.655%
16	8.653	1235	1241	1247	rBV	143230	219055	91.02%	10.074%
17	8.726	1250	1253	1257	rVB4	2339	3321	1.38%	0.153%
18	8.952	1285	1290	1298	rBV	22401	34582	14.37%	1.590%
19	9.275	1338	1343	1349	rBV3	2625	4103	1.70%	0.189%
20	9.391	1356	1362	1373	rBV	123630	179708	74.67%	8.264%
21	10.055	1465	1471	1481	rBV	175061	235150	97.70%	10.814%
22	11.195	1652	1658	1667	rVB	55365	70056	29.11%	3.222%
23	11.311	1673	1677	1683	rVB3	2085	3632	1.51%	0.167%
24	11.750	1743	1749	1753	rBV4	1492	2636	1.10%	0.121%
25	12.024	1788	1794	1804	rBV	183370	231180	96.05%	10.631%
26	12.323	1837	1843	1851	rVB	151867	193718	80.49%	8.908%




Sum of corrected areas: 2174538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024966.D
Acq On : 27 Oct 2021 11:37
Operator : JC/MD
Sample : M4318-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

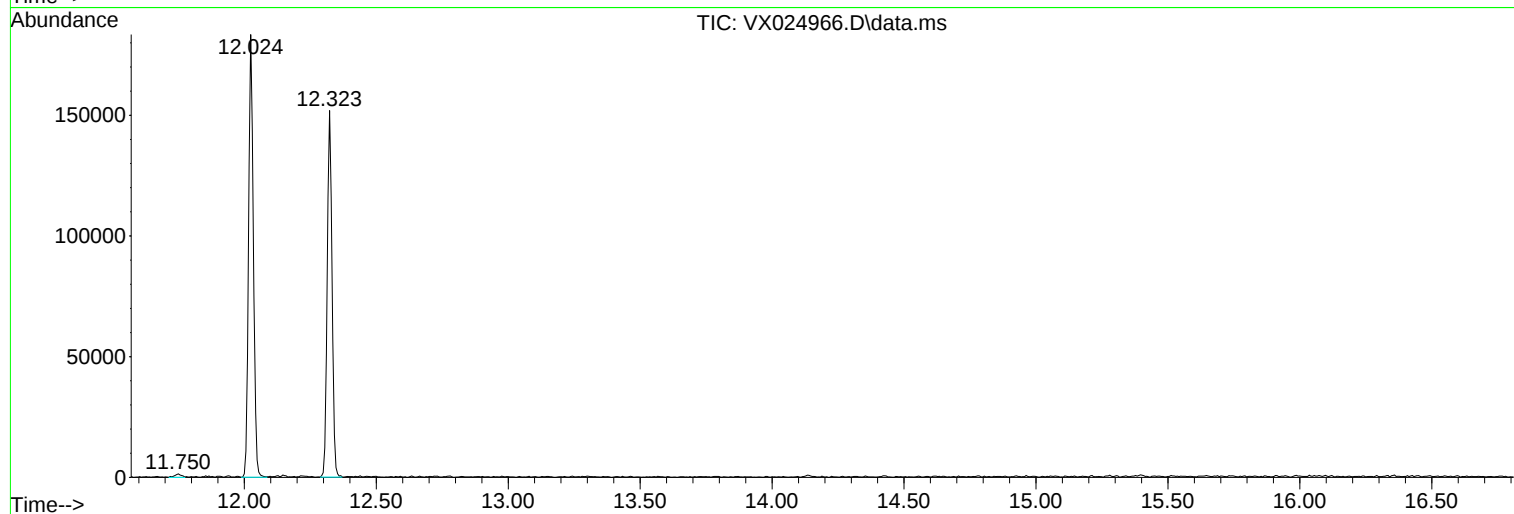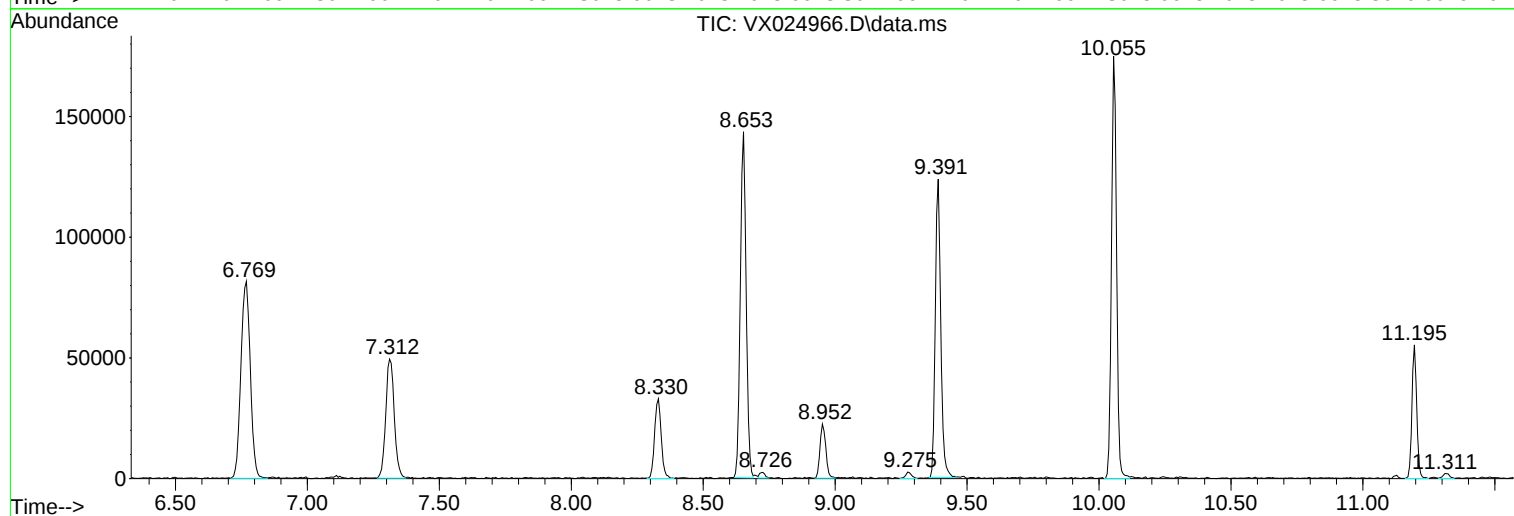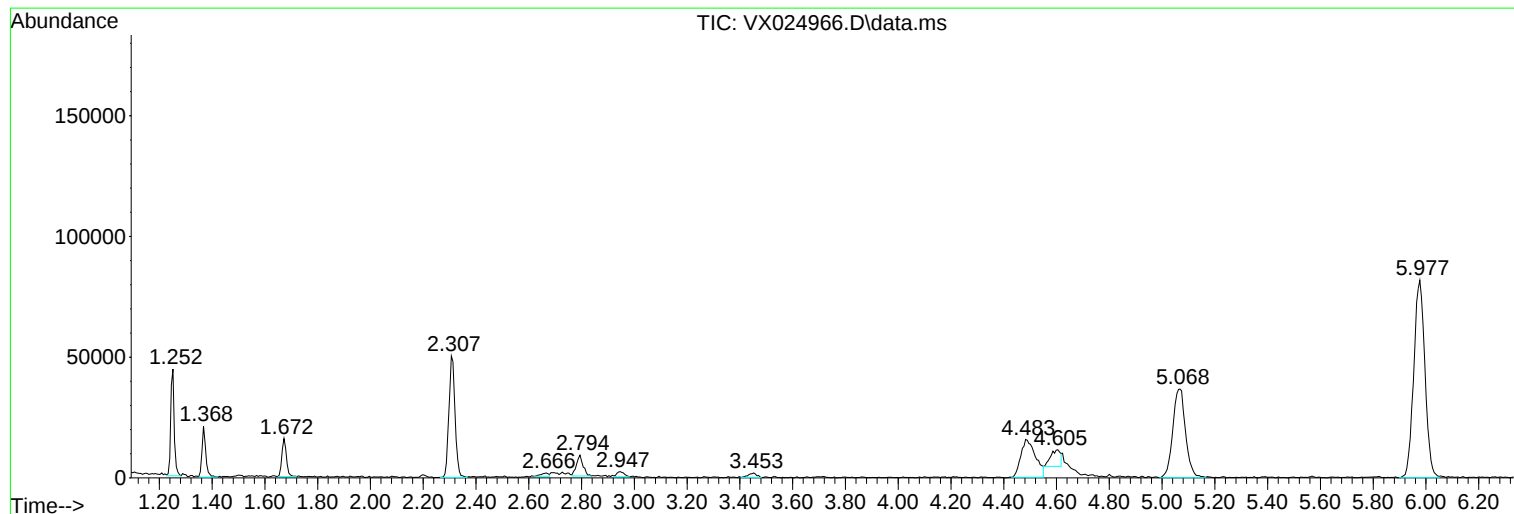

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024966.D
Acq On : 27 Oct 2021 11:37
Operator : JC/MD
Sample : M4318-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.252	1.00 ug/L	40236	1,4-Difluorobenzene	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-	([2-(Butane-1-sulfonyl)ethyl]s...	226	C8H18O3S2	1000388-83-2	9	
2	1,4,7-Oxadithionane	164	C6H12O2S2	040474-73-5	9		
3	o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4		
4	Thiirane	60	C2H4S	000420-12-2	4		
5	Carbonyl sulfide	60	COS	000463-58-1	4		

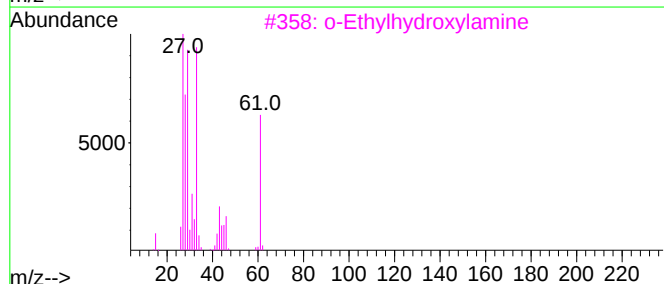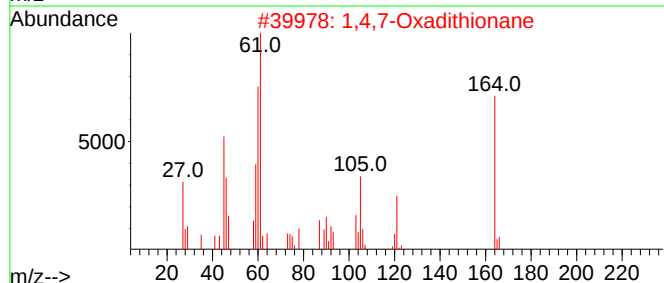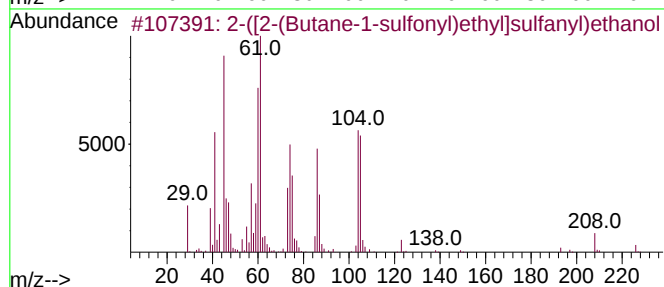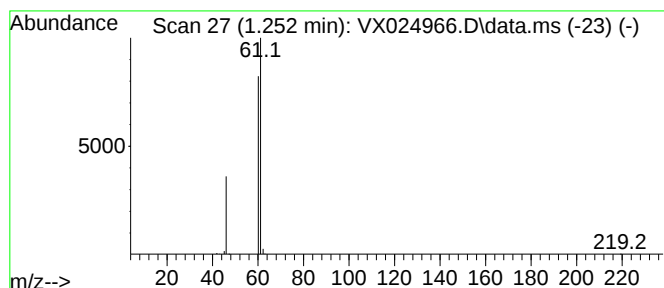

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024966.D
Acq On : 27 Oct 2021 11:37
Operator : JC/MD
Sample : M4318-09
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.252	1.0	ug/L	40236	1	6.769	200653	5.0