

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024970.D
 Acq On : 27 Oct 2021 13:12
 Operator : JC/MD
 Sample : M4319-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P071-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	19772	19853	8.87%	1.022%
2	1.673	92	96	104	rVB	13887	17719	7.92%	0.913%
3	2.313	195	201	211	rBV	49319	77230	34.52%	3.977%
4	4.489	547	558	570	rBV3	17114	63461	28.37%	3.268%
5	4.581	571	573	585	rVB5	2201	5038	2.25%	0.259%
6	5.068	644	653	671	rVB2	36655	116174	51.93%	5.983%
7	5.977	791	802	817	rBV4	75372	223706	100.00%	11.521%
8	6.769	923	932	945	rBV2	70948	168759	75.44%	8.691%
9	7.312	1013	1021	1032	rBV2	45586	101940	45.57%	5.250%
10	8.330	1181	1188	1196	rBV	32822	54498	24.36%	2.807%
11	8.653	1232	1241	1248	rBV	137012	209077	93.46%	10.767%
12	8.720	1248	1252	1258	rVB4	2323	4293	1.92%	0.221%
13	8.952	1284	1290	1300	rBV	20821	34028	15.21%	1.752%
14	9.281	1340	1344	1351	rVB2	3942	5469	2.44%	0.282%
15	9.391	1356	1362	1375	rBV	120614	176241	78.78%	9.076%
16	10.055	1466	1471	1482	rBV	142110	199145	89.02%	10.256%
17	11.195	1652	1658	1665	rBV	53072	67757	30.29%	3.489%
18	11.317	1674	1678	1682	rBV2	5944	7717	3.45%	0.397%
19	12.024	1789	1794	1801	rVB	156569	196814	87.98%	10.136%
20	12.323	1838	1843	1849	rVB	145980	187117	83.64%	9.637%
21	16.371	2502	2507	2513	rVB3	3266	5712	2.55%	0.294%




Sum of corrected areas: 1941748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024970.D
Acq On : 27 Oct 2021 13:12
Operator : JC/MD
Sample : M4319-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P071-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

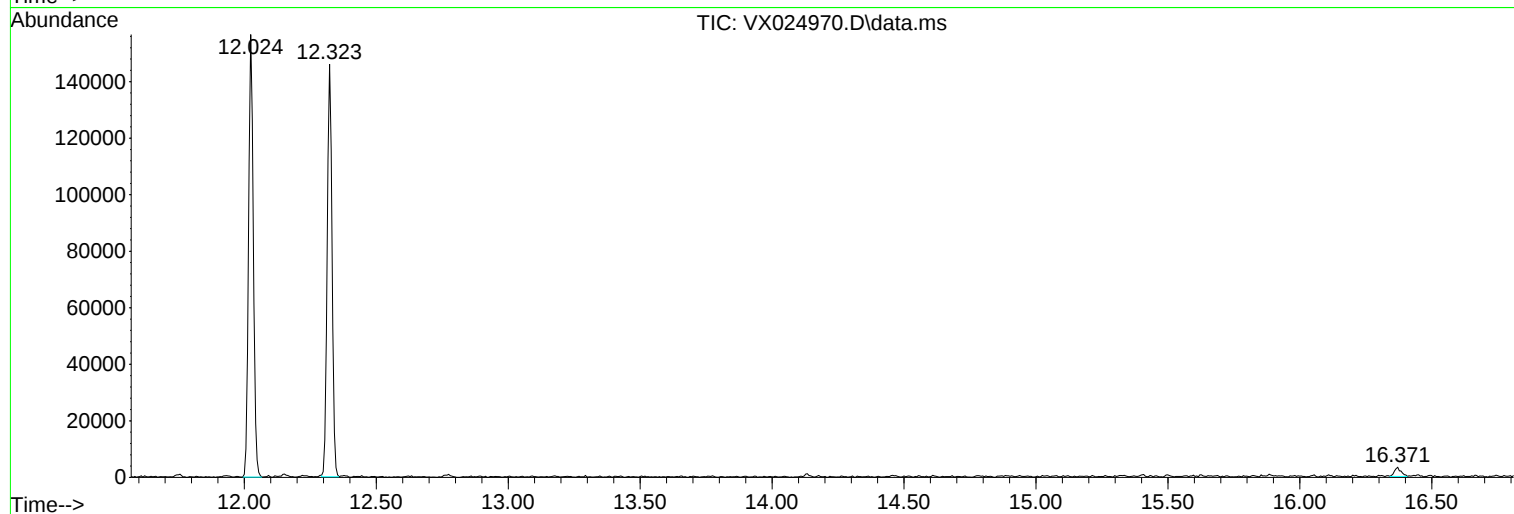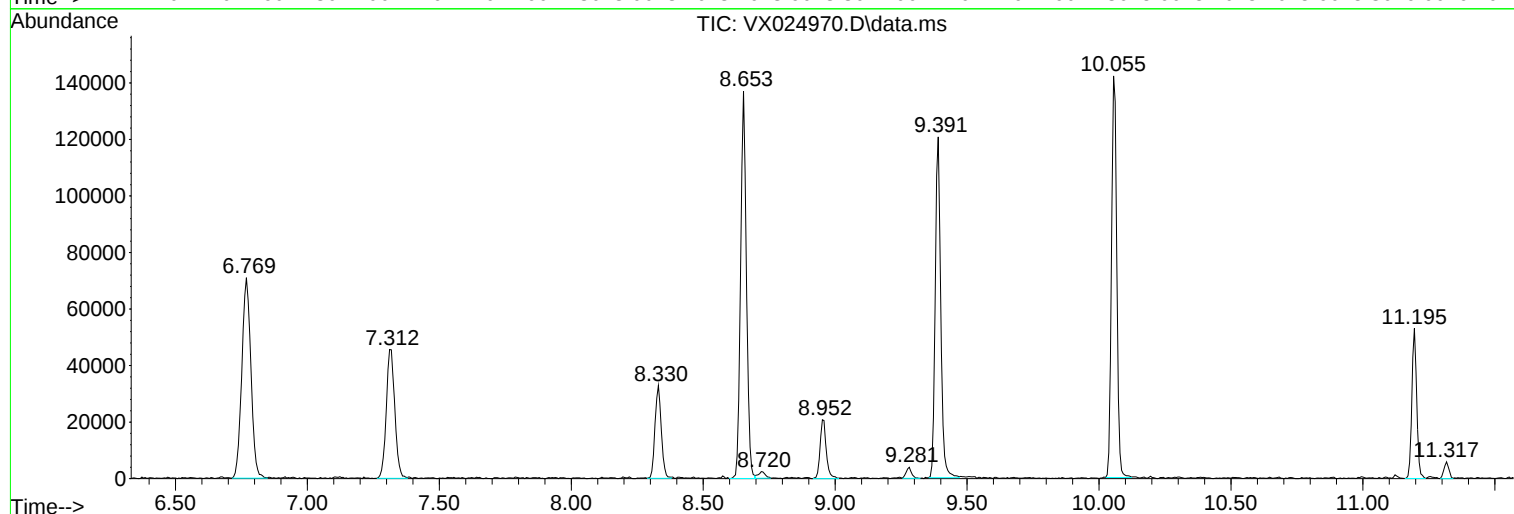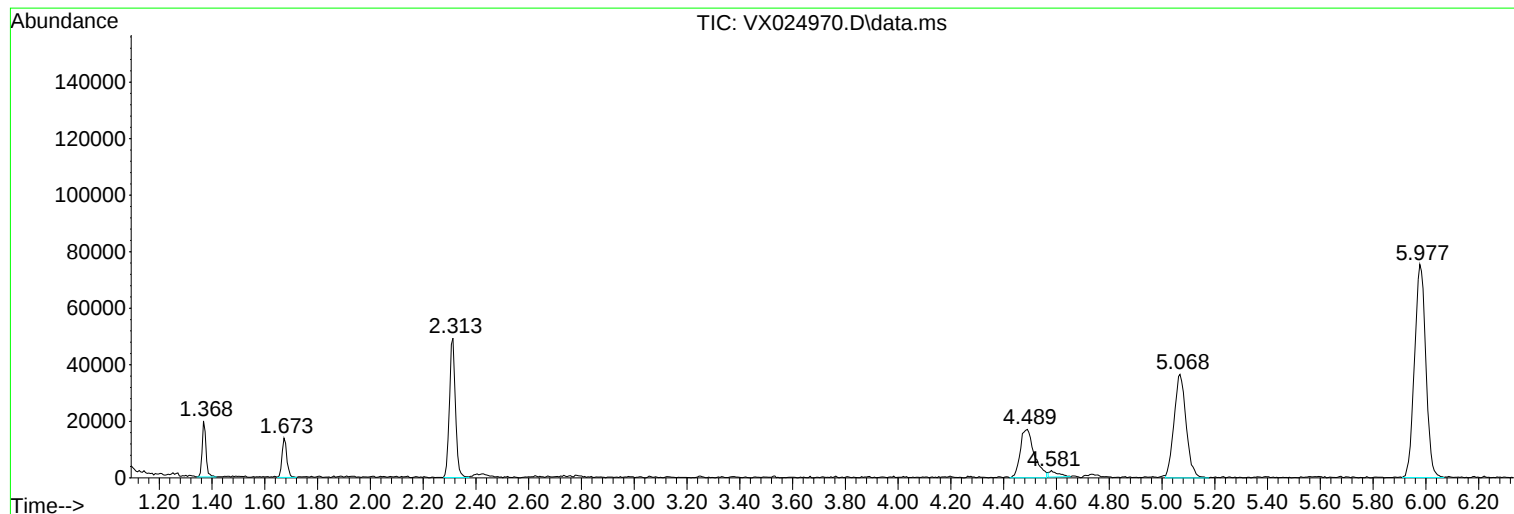

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024970.D
Acq On : 27 Oct 2021 13:12
Operator : JC/MD
Sample : M4319-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P071-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024970.D
Acq On : 27 Oct 2021 13:12
Operator : JC/MD
Sample : M4319-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P071-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
