

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024973.D
 Acq On : 27 Oct 2021 14:22
 Operator : JC/MD
 Sample : M4319-16
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	32	rBV	53236	48553	22.20%	2.473%
2	1.367	42	46	54	rVB	18071	19791	9.05%	1.008%
3	1.672	92	96	102	rBV	13113	15829	7.24%	0.806%
4	2.196	177	182	188	rBV3	1755	3098	1.42%	0.158%
5	2.312	193	201	209	rBV	48532	74868	34.23%	3.813%
6	2.794	275	280	287	rVB5	4445	9013	4.12%	0.459%
7	2.946	297	305	307	rBV4	1442	2580	1.18%	0.131%
8	4.495	550	559	570	rBV2	15452	56457	25.82%	2.876%
9	4.586	570	574	575	rBV	3315	3418	1.56%	0.174%
10	5.074	641	654	667	rBV2	36780	109469	50.06%	5.576%
11	5.976	792	802	817	rBV3	75008	218690	100.00%	11.139%
12	6.769	923	932	942	rBV	70201	172325	78.80%	8.778%
13	7.317	1014	1022	1033	rVB2	42968	98317	44.96%	5.008%
14	8.329	1182	1188	1197	rBV	29291	52359	23.94%	2.667%
15	8.653	1234	1241	1249	rBV	129823	200783	91.81%	10.227%
16	8.726	1249	1253	1258	rVB5	2757	4256	1.95%	0.217%
17	8.957	1285	1291	1299	rVB2	20409	32575	14.90%	1.659%
18	9.274	1339	1343	1349	rVB3	4250	6318	2.89%	0.322%
19	9.390	1356	1362	1376	rBV	117472	171607	78.47%	8.741%
20	10.055	1466	1471	1480	rBV	144786	200019	91.46%	10.188%
21	11.195	1651	1658	1664	rBV	50624	65356	29.89%	3.329%
22	11.317	1674	1678	1683	rVB3	6248	8269	3.78%	0.421%
23	12.024	1789	1794	1802	rBV	158689	199452	91.20%	10.159%
24	12.323	1837	1843	1849	rVB	144443	180655	82.61%	9.202%
25	12.768	1912	1916	1921	rVB	2058	2823	1.29%	0.144%
26	16.371	2503	2507	2513	rBV3	3846	6367	2.91%	0.324%




Sum of corrected areas: 1963247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024973.D
Acq On : 27 Oct 2021 14:22
Operator : JC/MD
Sample : M4319-16
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

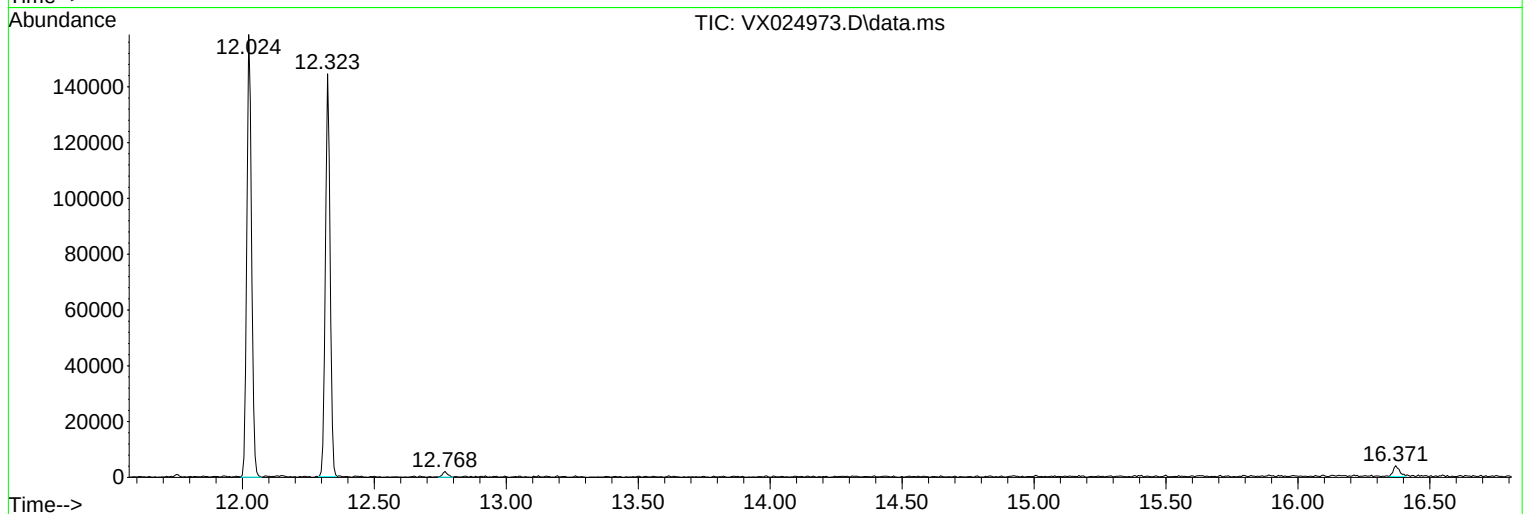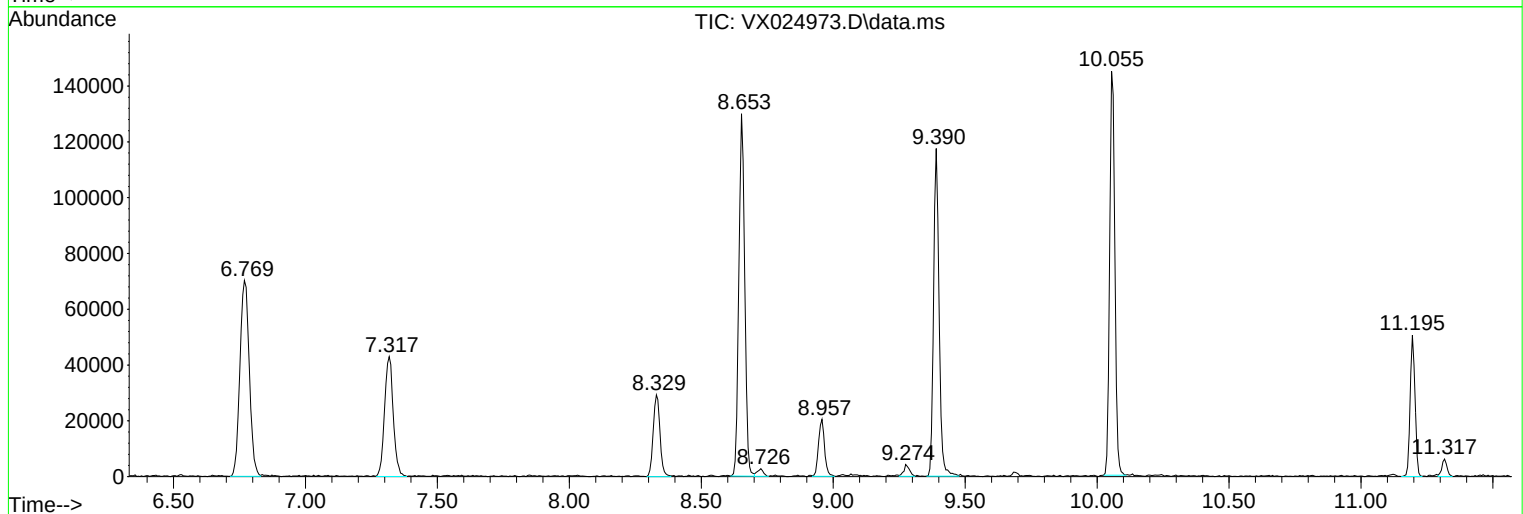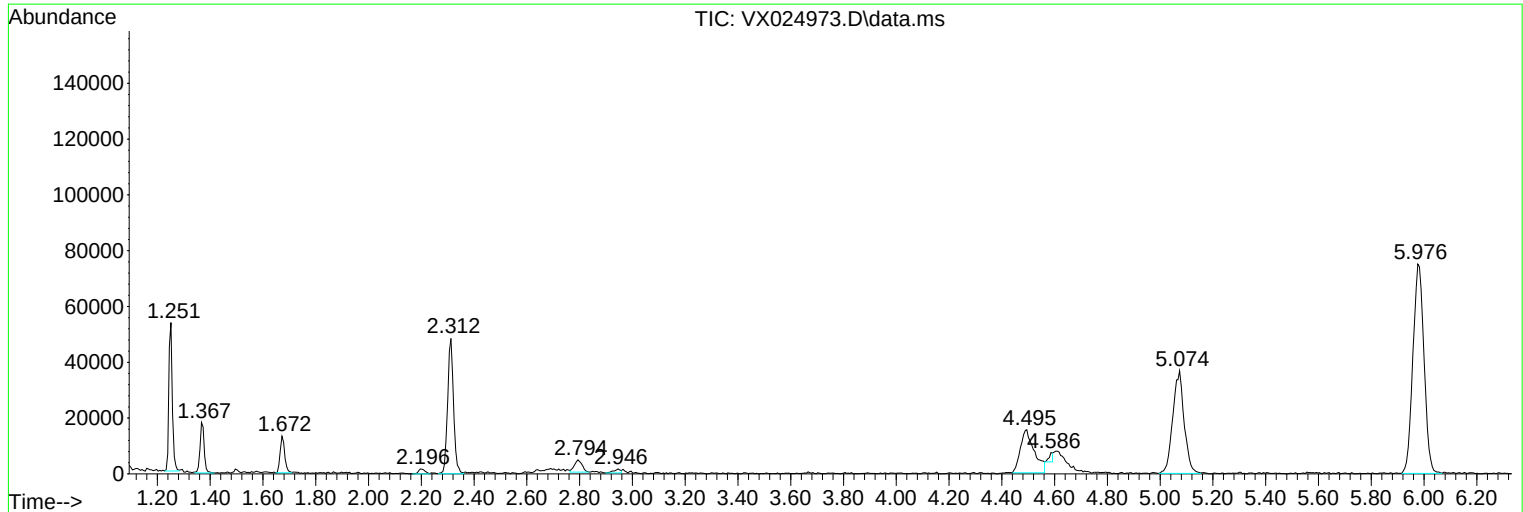

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024973.D
Acq On : 27 Oct 2021 14:22
Operator : JC/MD
Sample : M4319-16
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.251	1.41 ug/L	48553	1,4-Difluorobenzene	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,4,7-Oxadithionane		164	C6H12OS2		040474-73-5	9
2	Trifluoroguanidine		113	CH2F3N3		037950-72-4	9
3	2-([2-(Butane-1-sulfonyl)ethyl]s...		226	C8H18O3S2		1000388-83-2	9
4	Methyl nitrite		61	CH3NO2		000624-91-9	5
5	o-Ethylhydroxylamine		61	C2H7NO		000624-86-2	4

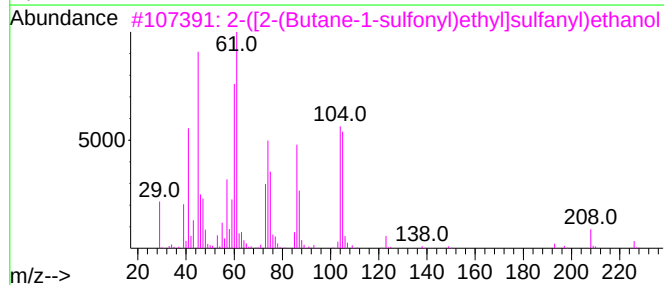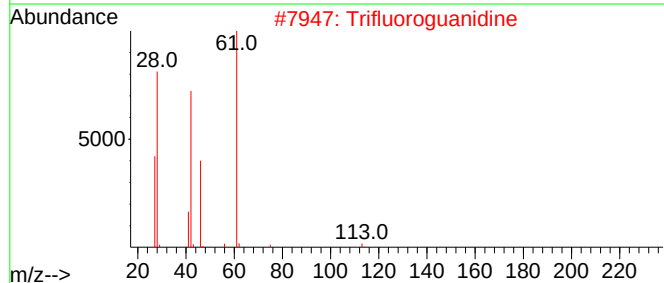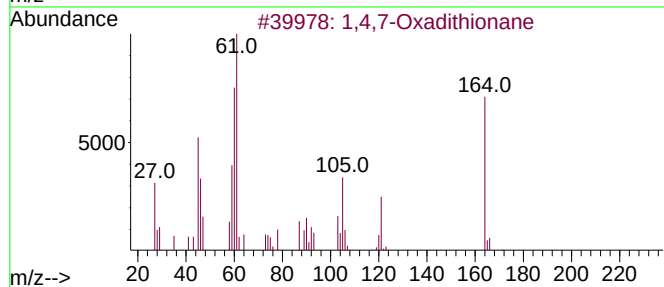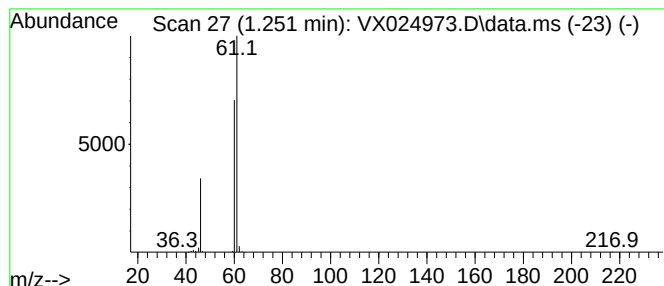

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
Data File : VX024973.D
Acq On : 27 Oct 2021 14:22
Operator : JC/MD
Sample : M4319-16
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.251	1.4	ug/L	48553	1	6.769	172325	5.0