
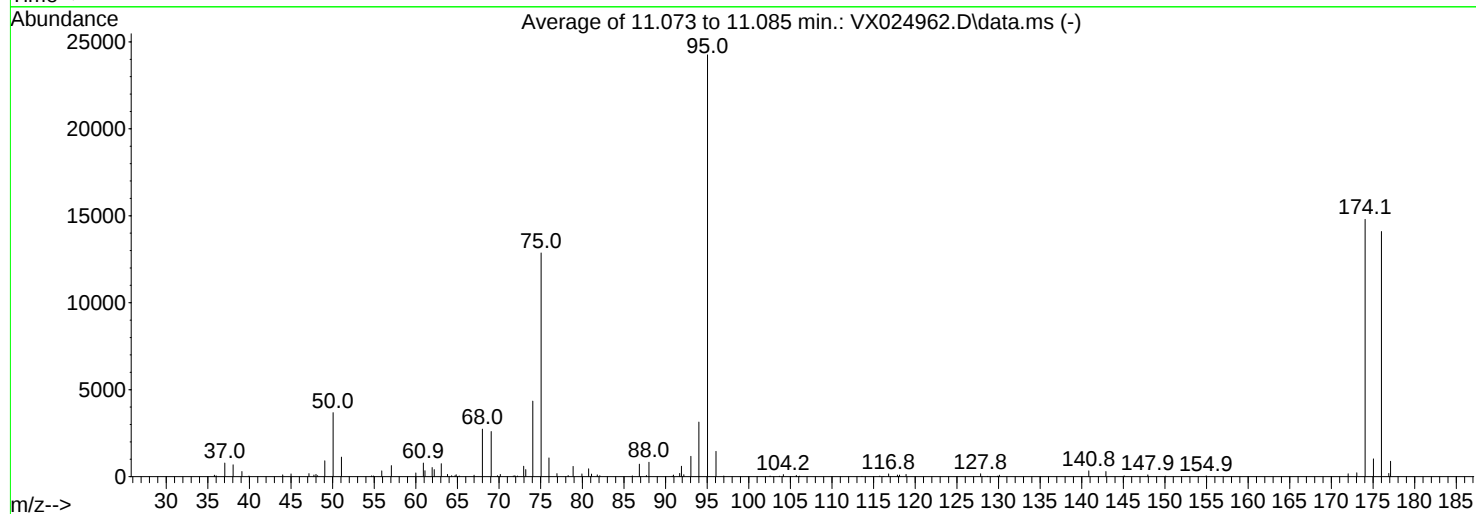


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102721\
 Data File : VX024962.D
 Acq On : 27 Oct 2021 09:24
 Operator : JC/MD
 Sample : BFB611
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB611

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Oct 28 03:09:30 2021

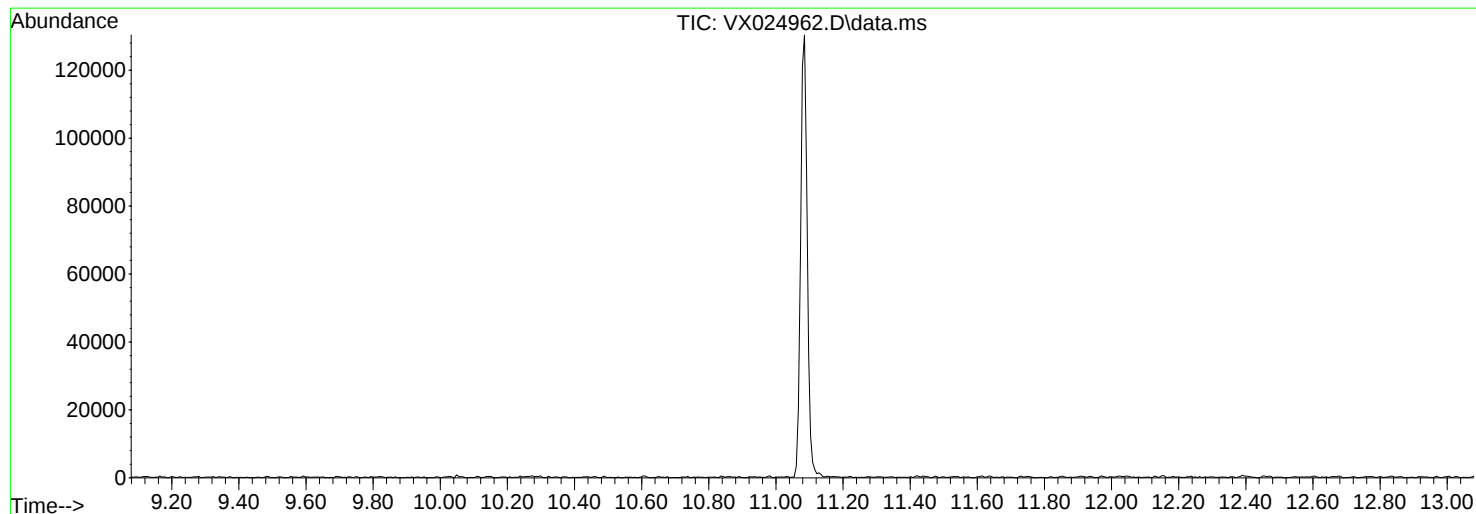

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	3682	PASS
75	95	30	80	53.0	12861	PASS
95	95	100	100	100.0	24255	PASS
96	95	5	9	6.0	1458	PASS
173	174	0.00	2	1.5	224	PASS
174	95	50	120	61.0	14796	PASS
175	174	5	9	6.9	1023	PASS
176	174	95	105	95.3	14098	PASS
177	176	5	10	6.3	882	PASS

m/z	Abundance
42.50	53.0
80.10	92.0
111.10	90.0
116.20	50.0
263.60	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
35.80	78.0
37.10	619.0
38.00	448.0
39.10	210.0
39.90	61.0
44.00	52.0
45.00	113.0
47.20	281.0
47.70	105.0
48.10	156.0
49.00	777.0
50.00	3096.0
51.00	818.0
55.90	164.0
57.00	435.0
60.10	99.0
60.90	854.0
62.00	741.0
63.00	656.0
63.80	111.0
64.30	69.0
64.70	181.0
68.00	1798.0
69.10	1482.0
69.80	152.0
73.00	838.0
74.00	2983.0
75.00	8442.0
76.00	541.0
76.90	111.0
79.00	446.0
80.00	248.0
80.80	334.0
81.90	61.0
86.00	131.0
86.80	464.0
87.70	191.0
88.10	277.0
90.80	71.0
91.70	558.0
92.20	330.0
93.10	702.0
94.00	2482.0
95.00	14877.0
96.00	1083.0
97.00	62.0
115.70	54.0
116.90	162.0
117.80	97.0
119.00	64.0
127.80	108.0
129.90	87.0
140.80	150.0
142.90	162.0
173.10	69.0
174.10	7999.0
175.00	546.0
176.00	7391.0
176.90	543.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.00	149.0
37.10	890.0
38.10	814.0
39.10	300.0
40.00	55.0
44.00	165.0
45.00	89.0
47.10	114.0
47.90	233.0
49.00	852.0
50.00	4136.0
51.00	1420.0
54.70	131.0
55.90	370.0
57.10	699.0
60.00	407.0
60.90	1495.0
61.90	824.0
63.10	687.0
63.70	113.0
64.30	94.0
64.90	176.0
67.00	172.0
68.00	2893.0
69.00	2853.0
70.10	198.0
71.70	115.0
72.20	101.0
73.20	1224.0
74.00	5247.0
75.10	15179.0
76.10	1346.0
76.90	198.0
78.30	208.0
79.00	583.0
79.90	156.0
80.70	591.0
81.80	130.0
86.90	863.0
88.00	849.0
91.00	156.0
91.90	923.0
93.10	1304.0
94.00	3165.0
95.00	29624.0
96.00	1667.0
97.00	60.0
102.50	57.0
103.70	71.0
104.20	122.0
106.10	89.0
115.80	70.0
116.20	68.0
116.80	144.0
117.90	169.0
118.80	176.0
127.90	179.0
128.70	61.0
130.10	129.0
140.90	373.0
142.90	371.0
148.00	135.0
150.10	84.0
154.90	60.0
172.00	196.0
173.10	234.0
174.00	15317.0
175.00	906.0
176.00	16416.0
177.10	1395.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
35.80	183.0
37.00	839.0
38.10	789.0
39.10	368.0
44.00	102.0
45.00	271.0
47.10	133.0
47.80	163.0
48.20	173.0
49.10	1112.0
50.10	3813.0
51.10	1140.0
54.90	114.0
55.90	468.0
57.00	767.0
60.00	128.0
61.10	1036.0
62.20	1202.0
63.10	886.0
63.90	153.0
64.80	169.0
65.20	124.0
67.00	90.0
68.00	3505.0
69.00	3458.0
70.20	185.0
71.90	164.0
72.90	962.0
74.10	4794.0
75.10	14962.0
75.90	1339.0
77.00	217.0
78.80	736.0
80.00	335.0
80.80	441.0
81.10	446.0
81.70	115.0
82.10	157.0
86.90	833.0
88.00	1346.0
90.90	122.0
91.90	869.0
93.00	1490.0
94.00	3764.0
95.10	28264.0
96.10	1624.0
102.60	67.0
104.10	236.0
105.70	229.0
113.60	65.0
116.20	118.0
116.70	175.0
118.10	276.0
119.00	150.0
127.80	221.0
130.10	131.0
140.90	464.0
142.90	361.0
145.10	136.0
147.90	170.0
155.00	79.0
172.00	313.0
173.00	369.0
174.00	21072.0
175.10	1616.0
176.00	18488.0
177.10	1250.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611