

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
 Data File : VX032438.D
 Acq On : 27 Oct 2022 19:00
 Operator : JC/MD
 Sample : N5315-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 221026039-02-VOA

Quant Time: Oct 28 07:14:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	119966	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	195984	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	172221	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	79333	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	80319	48.185	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.360%		
35) Dibromofluoromethane	5.385	113	62795	44.919	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.840%		
50) Toluene-d8	8.653	98	232180	47.763	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.520%		
62) 4-Bromofluorobenzene	11.079	95	87672	46.171	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	92.340%		
Target Compounds						Qvalue
6) Chloroethane	1.691	64	290	0.336	ug/l #	70
8) Diethyl Ether	2.130	74	6702	8.476	ug/l	97
11) Tert butyl alcohol	2.959	59	22388	92.278	ug/l	99
13) Acrolein	2.483	56	274	1.131	ug/l #	14
15) Acrylonitrile	2.965	53	317	0.481	ug/l #	1
16) Acetone	2.380	43	3685	6.082	ug/l #	87
19) Methyl tert-butyl Ether	3.111	73	1593	0.377	ug/l #	85
25) 2-Butanone	4.568	43	2526	2.691	ug/l #	76
26) 2,2-Dichloropropane	4.556	77	2221	1.171	ug/l #	53
29) Tetrahydrofuran	5.007	42	45679	76.320	ug/l	98
31) Cyclohexane	5.556	56	2729	1.350	ug/l #	9
36) 1,1-Dichloropropene	5.550	75	10078	5.177	ug/l #	48
38) Carbon Tetrachloride	5.550	117	12879	5.965	ug/l #	15
40) Benzene	6.037	78	3254	0.591	ug/l	96
41) Methacrylonitrile	5.007	41	27446	26.588	ug/l #	45
49) 1,4-Dioxane	7.677	88	2757	90.030	ug/l	98
51) 4-Methyl-2-Pentanone	8.555	43	1058	0.540	ug/l #	47
59) 2-Hexanone	9.561	43	374	0.257	ug/l	96
65) Chlorobenzene	10.079	112	29834	7.733	ug/l	96
68) m/p-Xylenes	10.305	106	2600	0.971	ug/l	90
69) o-Xylene	10.646	106	2665	1.023	ug/l	94
73) Isopropylbenzene	10.963	105	2441	0.388	ug/l	100
74) N-amyl acetate	10.884	43	769	0.324	ug/l #	54
76) 1,2,3-Trichloropropane	11.079	75	47031	26.647	ug/l #	37
79) 2-Chlorotoluene	11.366	91	2797	0.645	ug/l	90
81) trans-1,4-Dichloro-2-b...	11.079	75	47031	84.791	ug/l #	6
82) 4-Chlorotoluene	11.366	91	2797	0.551	ug/l	97
87) 1,3-Dichlorobenzene	12.043	146	18452	6.347	ug/l	96
88) 1,4-Dichlorobenzene	12.043	146	18452	6.118	ug/l	97
90) Hexachloroethane	12.616	117	227	0.254	ug/l #	12
91) 1,2-Dichlorobenzene	12.335	146	1080	0.377	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032438.D
Acq On : 27 Oct 2022 19:00
Operator : JC/MD
Sample : N5315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Quant Time: Oct 28 07:14:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration




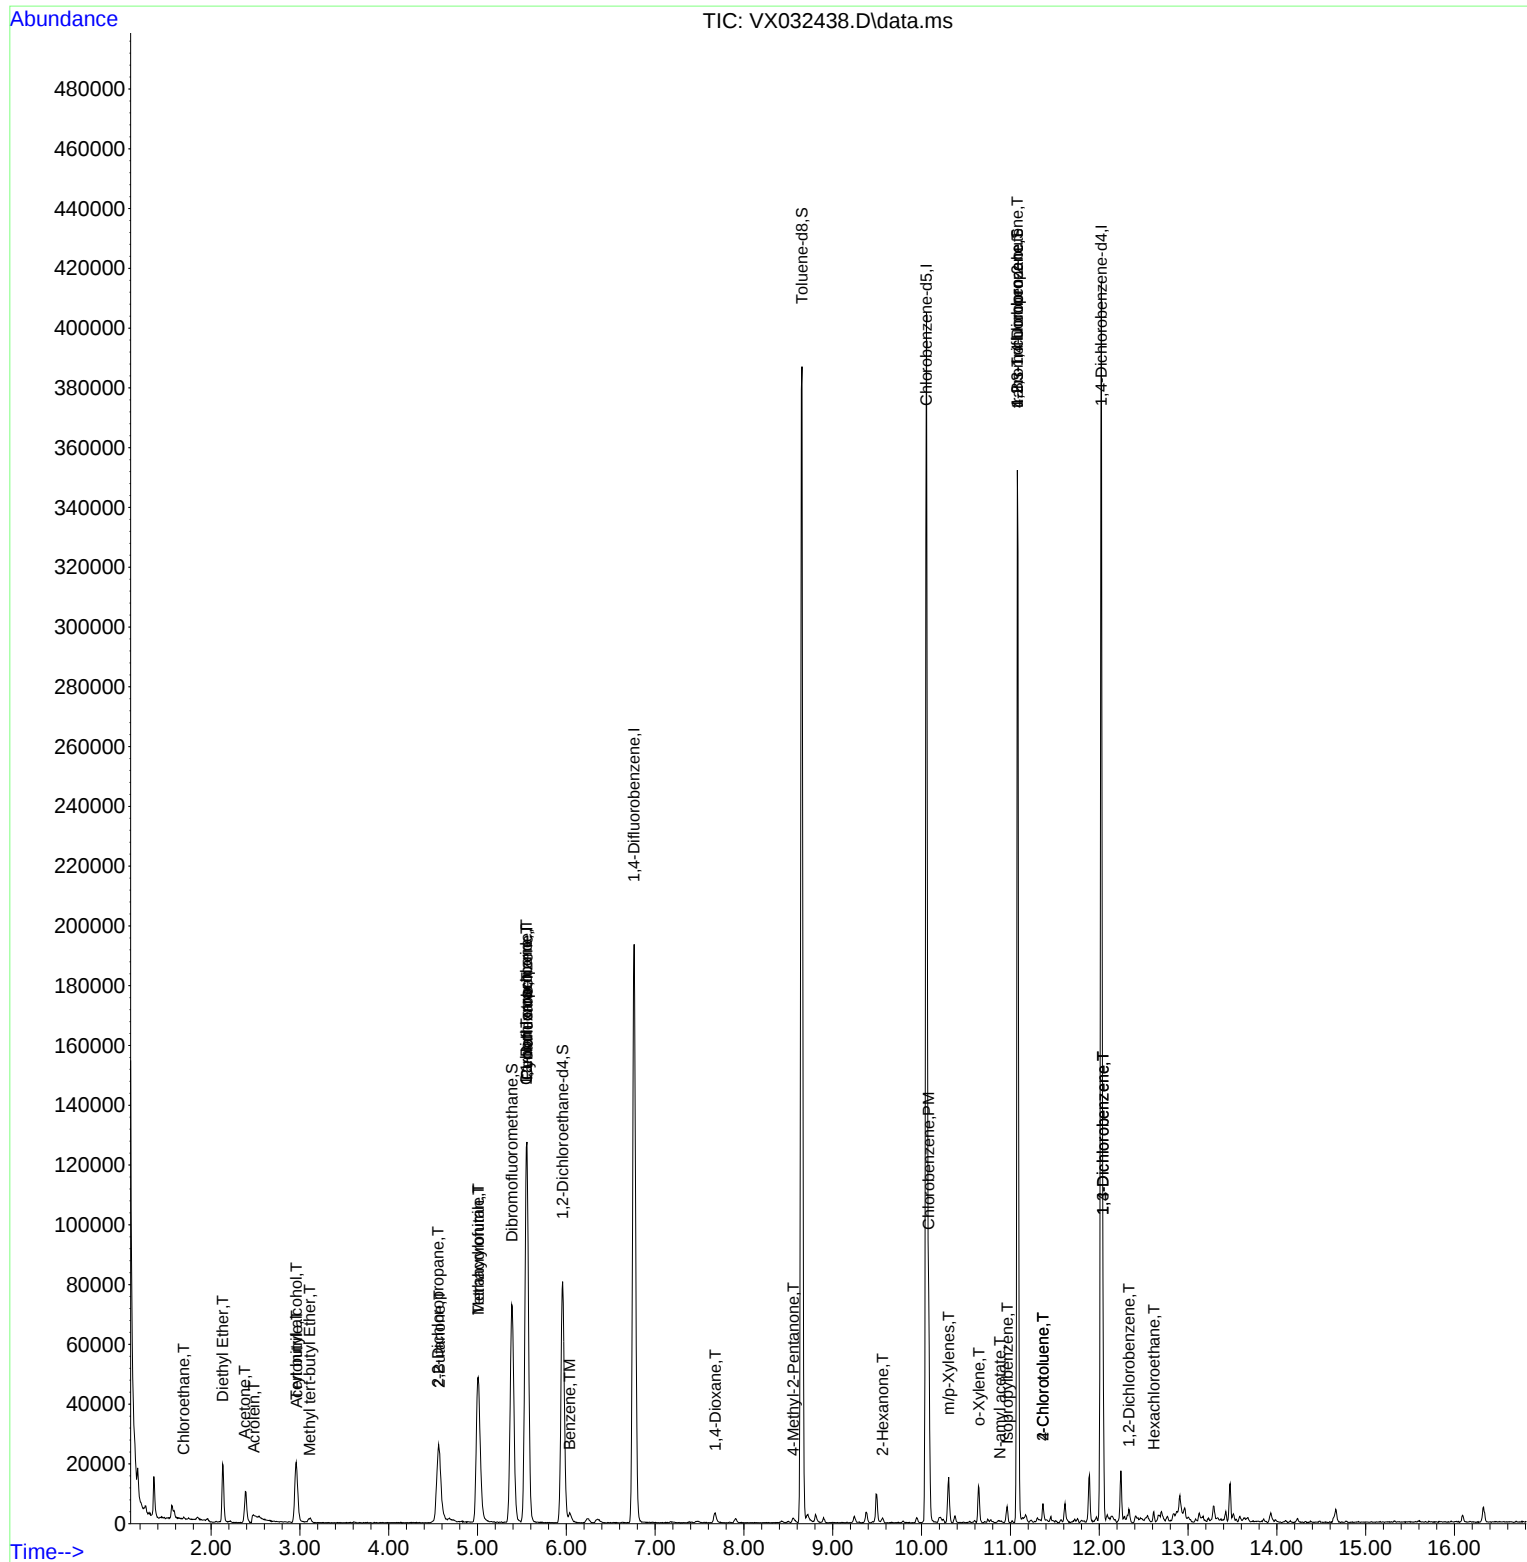




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion:168 Resp: 119966
Ion Ratio Lower Upper
168 100
99 59.1 46.1 69.1

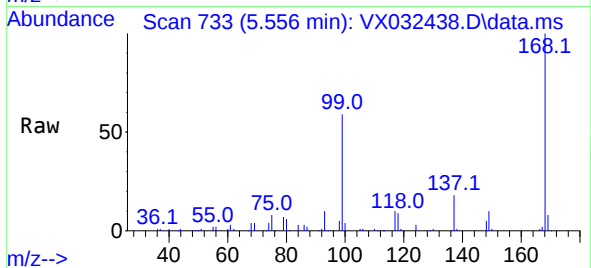

#6
Chloroethane
Concen: 0.336 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 64 Resp: 290
Ion Ratio Lower Upper
64 100
66 49.1 26.0 39.0#


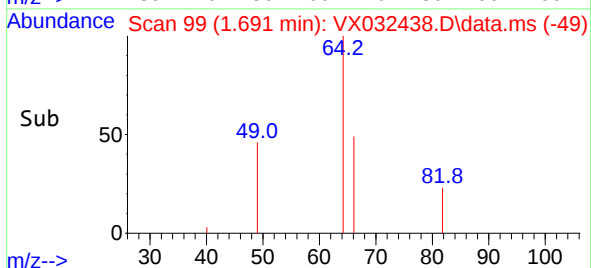
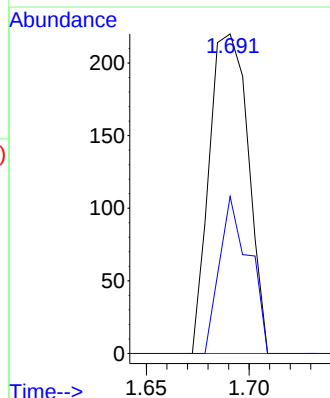



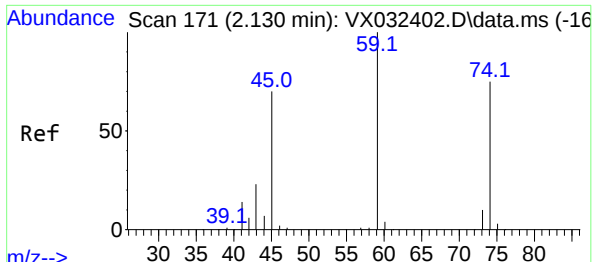

#8
Diethyl Ether
Concen: 8.476 ug/l
RT: 2.130 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion: 74 Resp: 6702
Ion Ratio Lower Upper
74 100
45 90.0 46.6 139.7

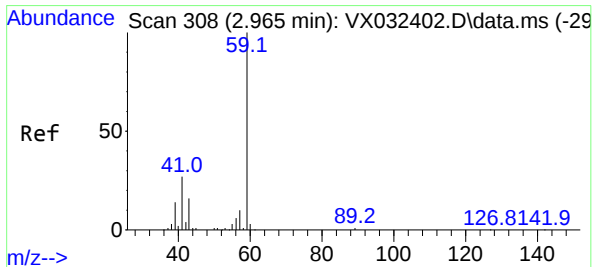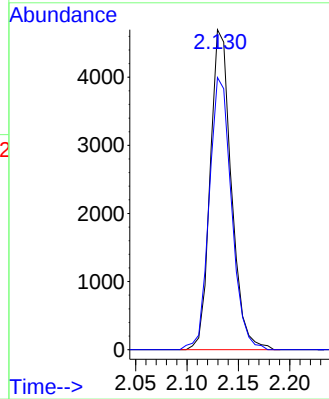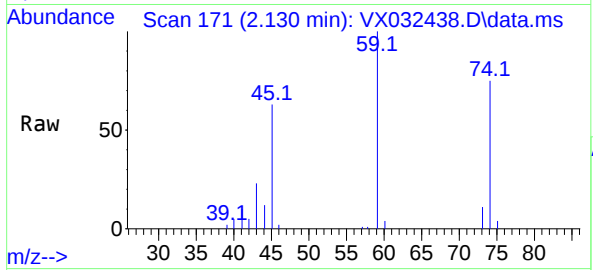

#11
Tert butyl alcohol
Concen: 92.278 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.006 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 59 Resp: 22388
Ion Ratio Lower Upper
59 100
57 10.7 8.2 12.4


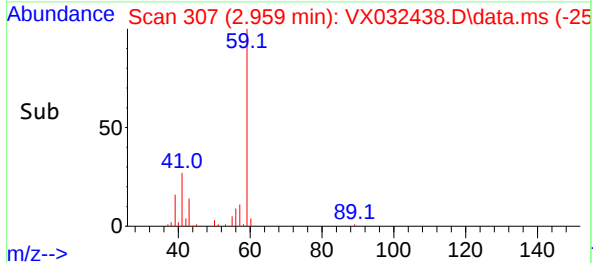
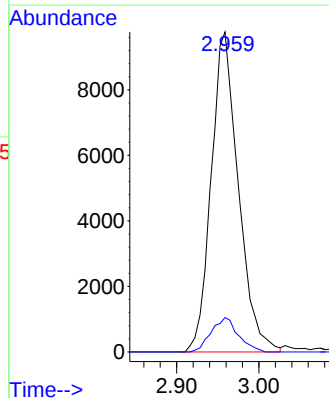
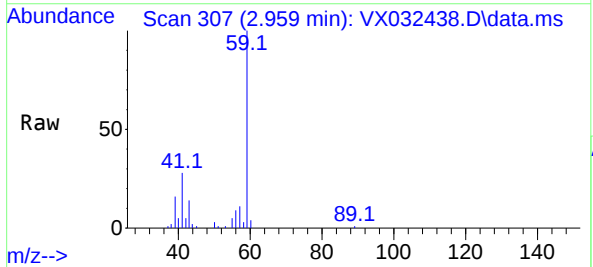




#13
Acrolein
Concen: 1.131 ug/l
RT: 2.483 min Scan# 21
Delta R.T. 0.250 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion: 56 Resp: 274
Ion Ratio Lower Upper
56 100
55 0.0 56.9 85.3#

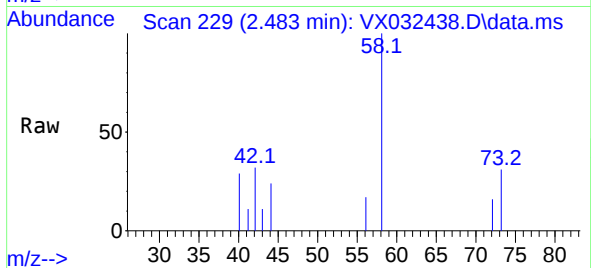

#15
Acrylonitrile
Concen: 0.481 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.098 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 53 Resp: 317
Ion Ratio Lower Upper
53 100
52 0.0 67.4 101.0#
51 118.0 30.3 45.5#


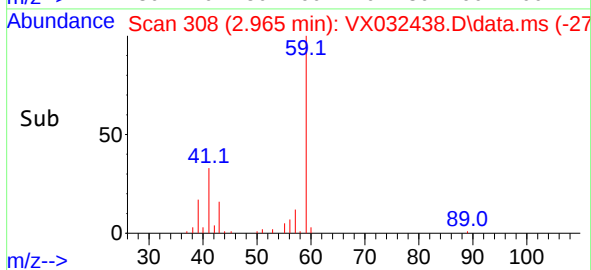






#16
Acetone
Concen: 6.082 ug/l
RT: 2.380 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion: 43 Resp: 3685
Ion Ratio Lower Upper
43 100
58 23.0 23.8 35.8#

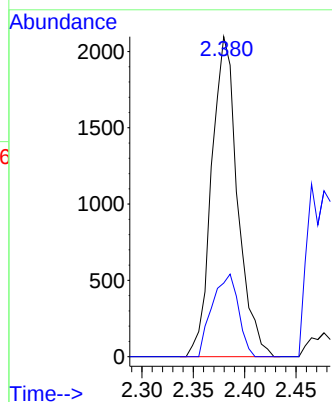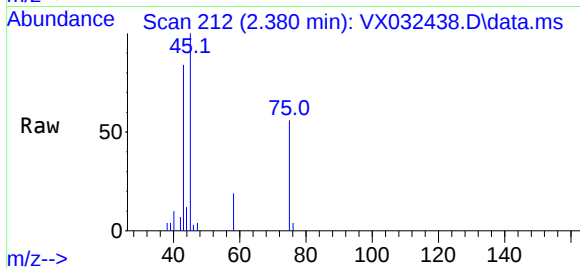

#19
Methyl tert-butyl Ether
Concen: 0.377 ug/l
RT: 3.111 min Scan# 332
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 73 Resp: 1593
Ion Ratio Lower Upper
73 100
57 27.8 16.6 25.0#

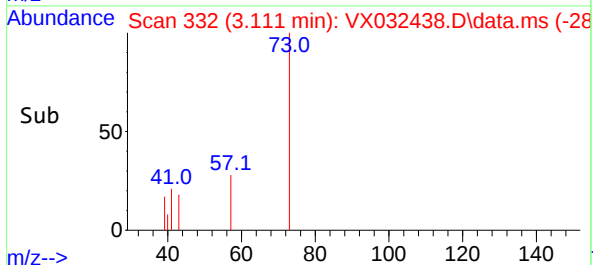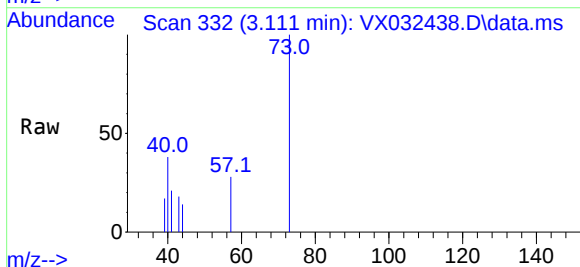



#25

2-Butanone

Concen: 2.691 ug/l

RT: 4.568 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX032438.D

Acq: 27 Oct 2022 19:00

Instrument :

MSVOA_X

ClientSampleId :





221026039-02-VOA

Tgt Ion: 43 Resp: 2526

Ion Ratio Lower Upper

43 100

72 15.0 22.2 33.2#

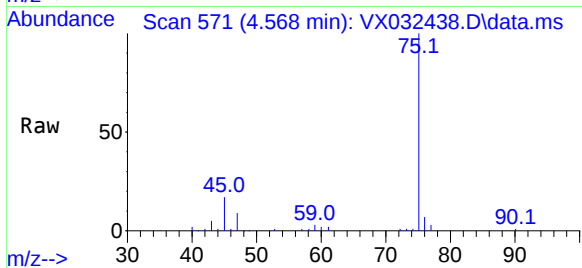

#26

2,2-Dichloropropane

Concen: 1.171 ug/l

RT: 4.556 min Scan# 569

Delta R.T. 0.079 min

Lab File: VX032438.D




Acq: 27 Oct 2022 19:00


Tgt Ion: 77 Resp: 2221

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.1#

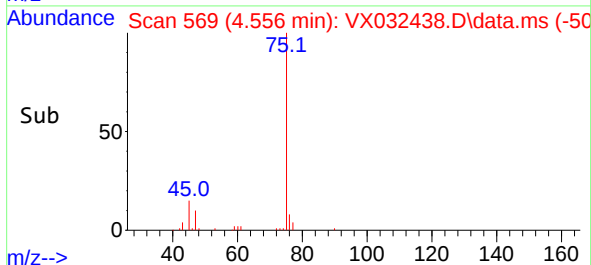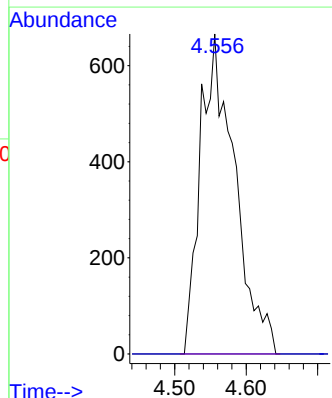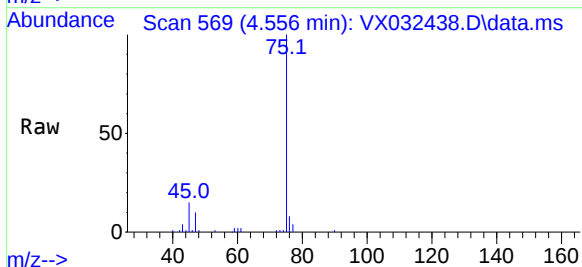



#29

Tetrahydrofuran

Concen: 76.320 ug/l

RT: 5.007 min Scan# 64

Delta R.T. 0.006 min

Lab File: VX032438.D

Acq: 27 Oct 2022 19:00

Instrument :





MSVOA_X

ClientSampleId :

221026039-02-VOA

Tgt Ion: 42 Resp: 45679

Ion	Ratio	Lower	Upper
42	100		
72	45.3	37.6	56.4
71	42.8	34.7	52.1

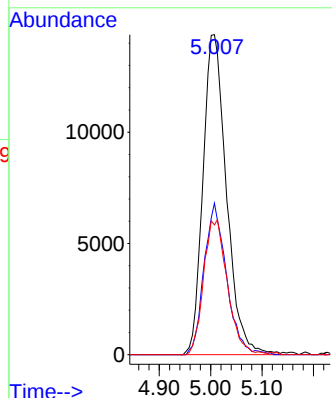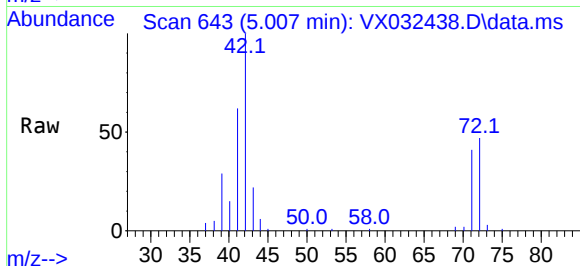

#31

Cyclohexane

Concen: 1.350 ug/l

RT: 5.556 min Scan# 733




Delta R.T. 0.085 min


Lab File: VX032438.D

Acq: 27 Oct 2022 19:00

Tgt Ion: 56 Resp: 2729

Ion	Ratio	Lower	Upper
56	100		
69	159.8	24.1	36.1#
84	117.4	66.9	100.3#


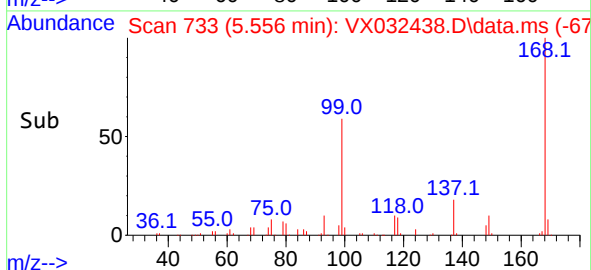
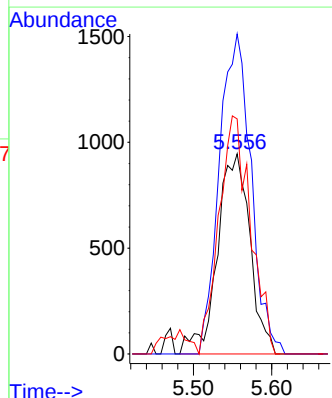
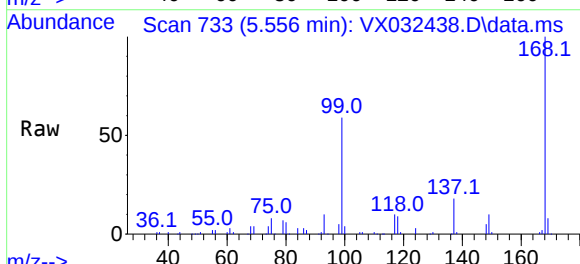




#33
1,2-Dichloroethane-d4
Concen: 48.185 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion: 65 Resp: 80319
Ion Ratio Lower Upper
65 100
67 50.2 0.0 101.8

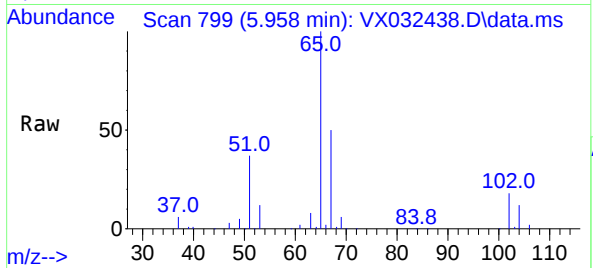

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00


Tgt Ion: 114 Resp: 195984
Ion Ratio Lower Upper
114 100
63 20.0 0.0 41.6
88 15.7 0.0 33.4

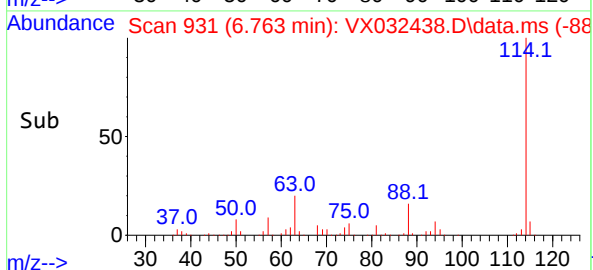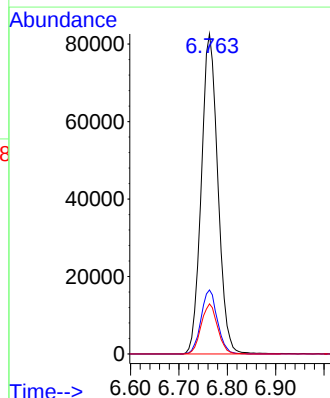






#35
Dibromofluoromethane
Concen: 44.919 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00


Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA





Tgt Ion:113 Resp: 62795
Ion Ratio Lower Upper
113 100
111 102.7 82.4 123.6
192 18.9 15.4 23.2

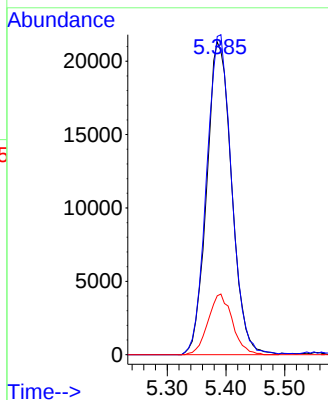


#36
1,1-Dichloropropene
Concen: 5.177 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.146 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Tgt Ion: 75 Resp: 10078
Ion Ratio Lower Upper
75 100
110 8.3 18.4 55.2#
77 0.0 24.5 36.7#

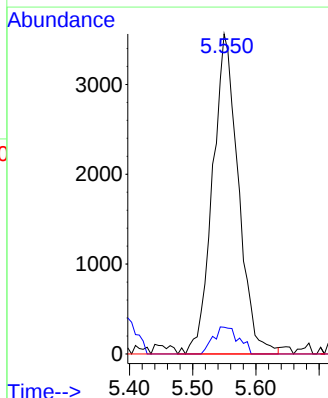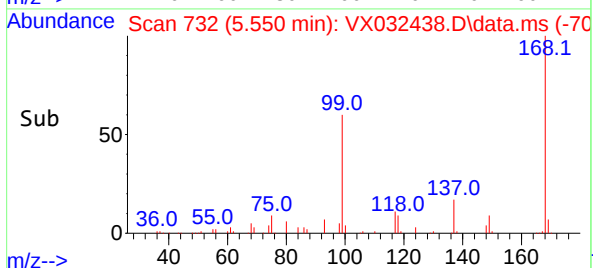



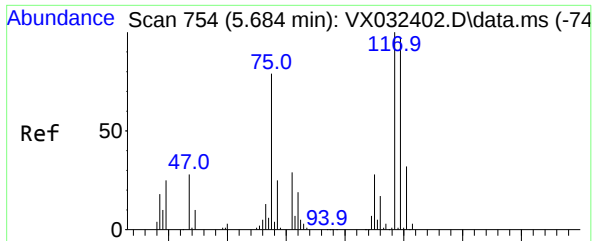


#38
Carbon Tetrachloride
Concen: 5.965 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA



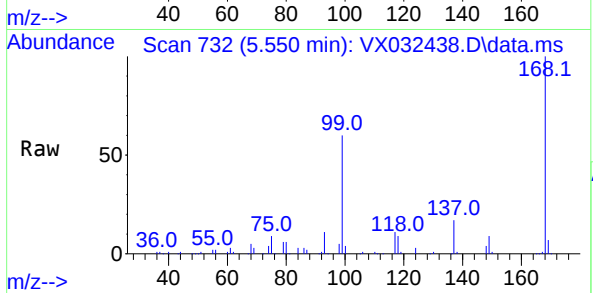



Tgt Ion:117 Resp: 12879
Ion Ratio Lower Upper
117 100
119 4.5 77.2 115.8#
121 0.0 25.8 38.6#

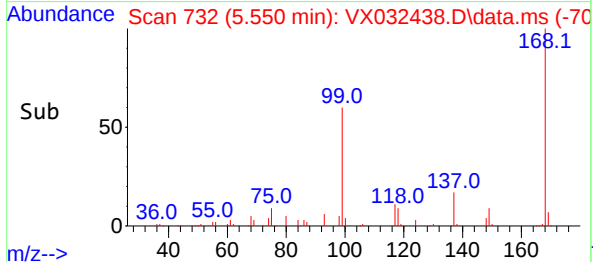

#40
Benzene
Concen: 0.591 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 78 Resp: 3254
Ion Ratio Lower Upper
78 100
77 25.6 19.0 28.4

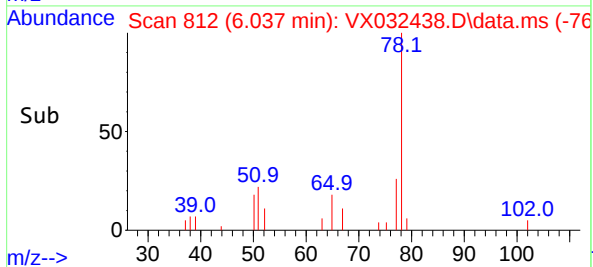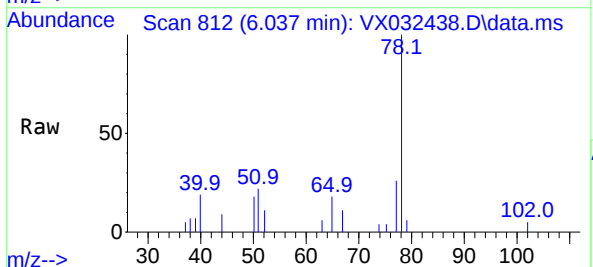







#41
Methacrylonitrile
Concen: 26.588 ug/l
RT: 5.007 min Scan# 641
Delta R.T. 0.085 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Tgt Ion: 41 Resp: 27446




Ion	Ratio	Lower	Upper
41	100		
39	50.9	47.5	71.3
67	0.0	60.5	90.7#
52	0.0	27.0	40.6#

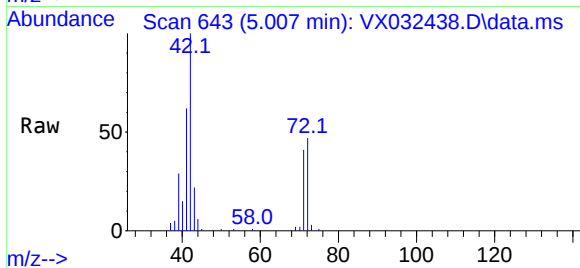


#49
1,4-Dioxane
Concen: 90.030 ug/l
RT: 7.677 min Scan# 1081
Delta R.T. 0.006 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 88 Resp: 2757

Ion	Ratio	Lower	Upper
88	100		
43	30.4	26.6	39.8
58	64.7	51.7	77.5

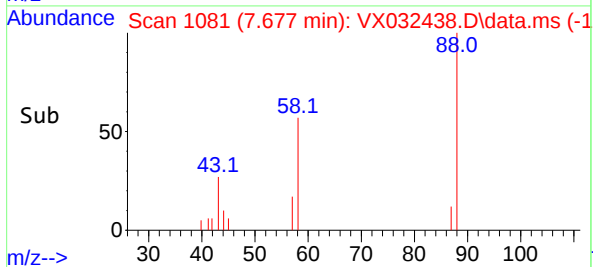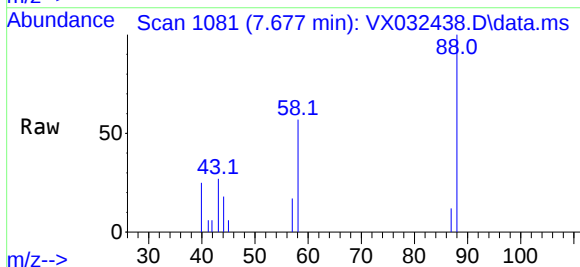



#50

Toluene-d8

Concen: 47.763 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX032438.D

Acq: 27 Oct 2022 19:00

Instrument :

MSVOA_X

ClientSampleId :





221026039-02-VOA

Tgt Ion: 98 Resp: 232180

Ion Ratio Lower Upper

98 100

100 64.6 50.9 76.3

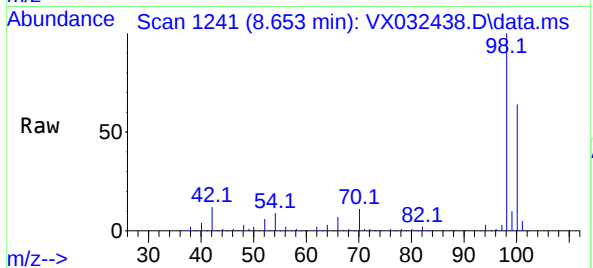

#51

4-Methyl-2-Pentanone

Concen: 0.540 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. -0.018 min

Lab File: VX032438.D




Acq: 27 Oct 2022 19:00


Tgt Ion: 43 Resp: 1058

Ion Ratio Lower Upper

43 100

58 6.4 30.9 46.3#

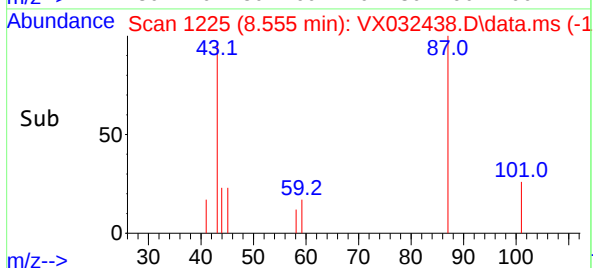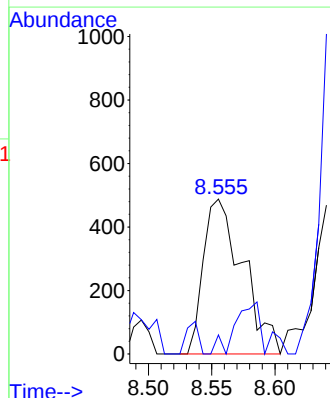



#59

2-Hexanone

Concen: 0.257 ug/l

RT: 9.561 min Scan# 1390

Delta R.T. 0.128 min

Lab File: VX032438.D

Acq: 27 Oct 2022 19:00

Instrument :

MSVOA_X

ClientSampleId :





221026039-02-VOA

Tgt Ion: 43 Resp: 374

Ion Ratio Lower Upper

43 100

58 50.0 26.5 79.5

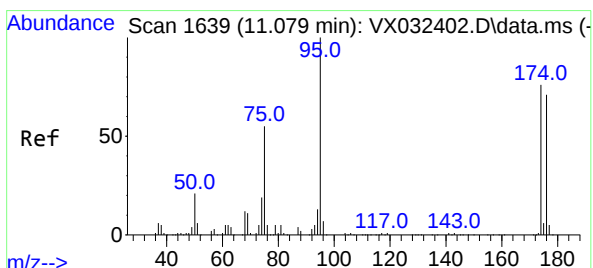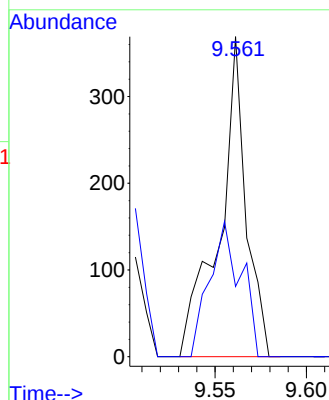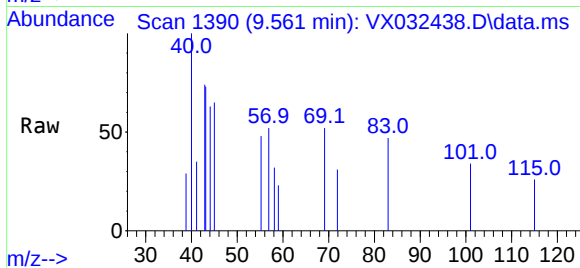

#62

4-Bromofluorobenzene

Concen: 46.171 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX032438.D

Acq: 27 Oct 2022 19:00




Tgt Ion: 95 Resp: 87672


Ion Ratio Lower Upper

95 100

174 80.1 0.0 164.0

176 77.9 0.0 154.4


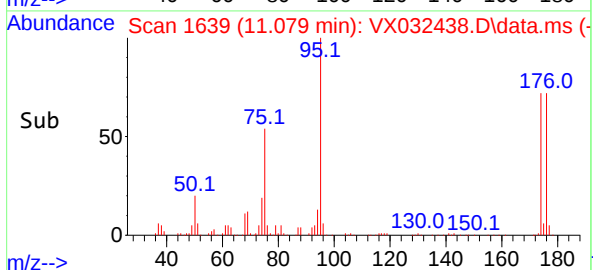
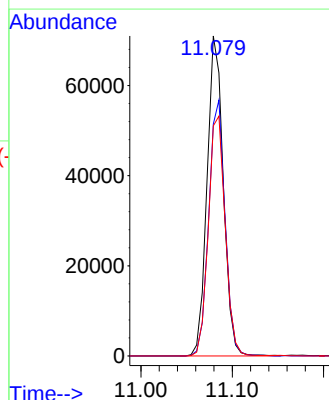
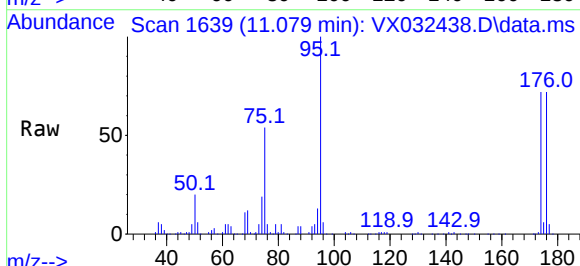




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion:117 Resp: 172221
Ion Ratio Lower Upper
117 100
82 56.5 44.3 66.5
119 32.4 25.7 38.5

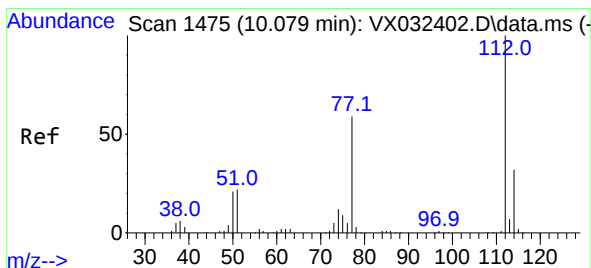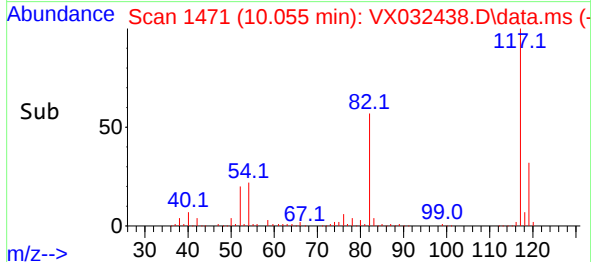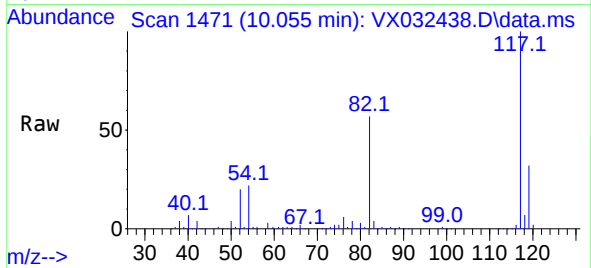

#65
Chlorobenzene
Concen: 7.733 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion:112 Resp: 29834
Ion Ratio Lower Upper
112 100
114 29.3 25.4 38.2


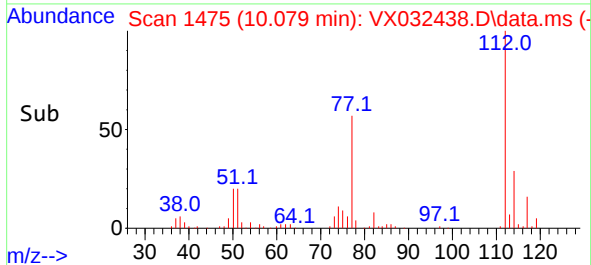

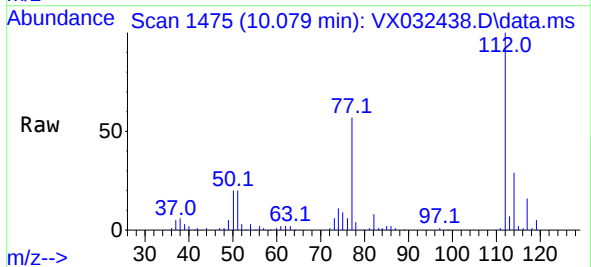




#68
m/p-Xylenes
Concen: 0.971 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion:106 Resp: 2600
Ion Ratio Lower Upper
106 100
91 221.8 164.5 246.7

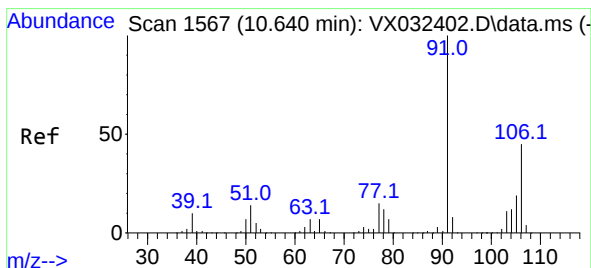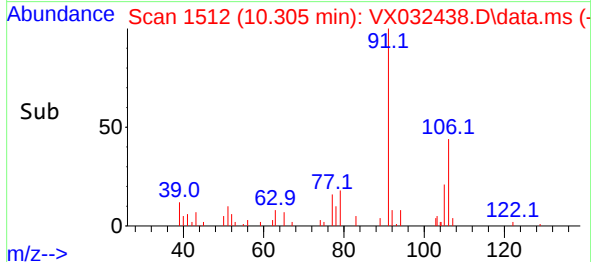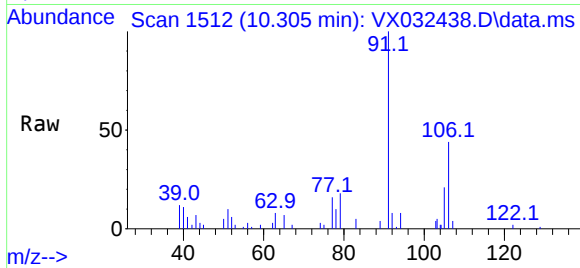

#69
o-Xylene
Concen: 1.023 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion:106 Resp: 2665
Ion Ratio Lower Upper
106 100
91 228.7 109.2 327.6


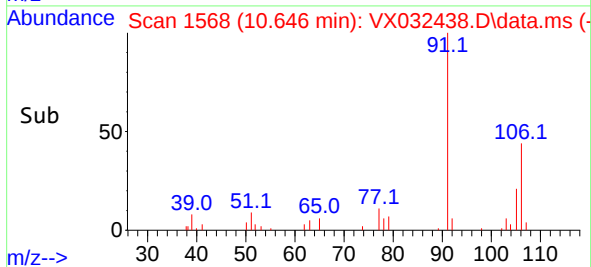

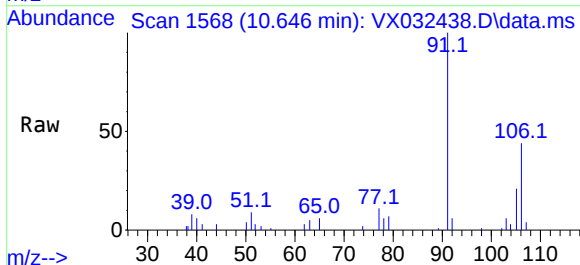




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion:152 Resp: 79333
Ion Ratio Lower Upper
152 100
115 58.7 44.0 132.0
150 159.4 0.0 351.8

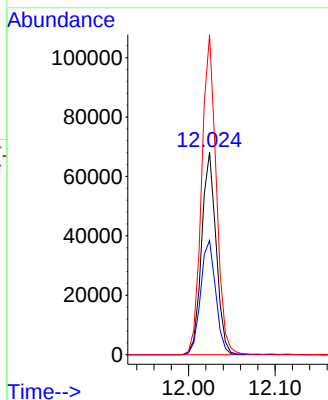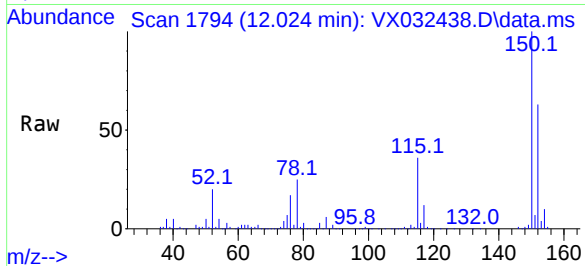

#73
Isopropylbenzene
Concen: 0.388 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion:105 Resp: 2441
Ion Ratio Lower Upper
105 100
120 26.2 13.1 39.3

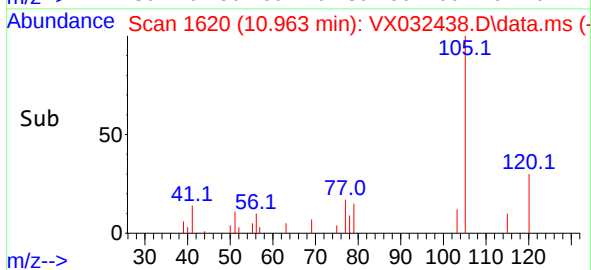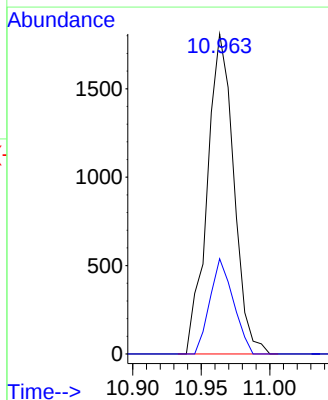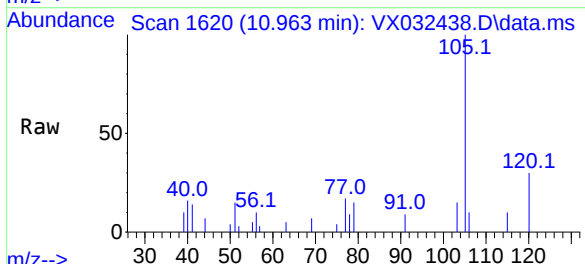







#74
N-amy1 acetate
Concen: 0.324 ug/l
RT: 10.884 min Scan# 1607
Delta R.T. 0.043 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Tgt Ion: 43 Resp: 769




Ion	Ratio	Lower	Upper
43	100		
70	0.0	33.6	50.4#
55	20.3	19.4	29.2
61	0.0	18.8	28.2#

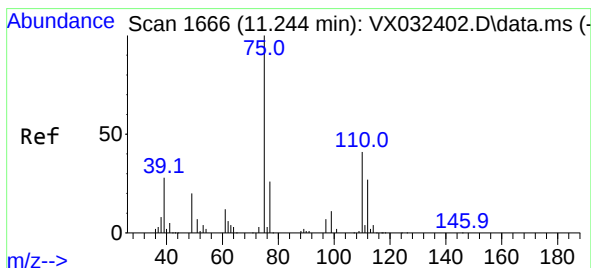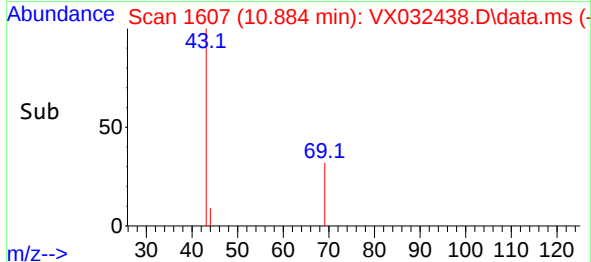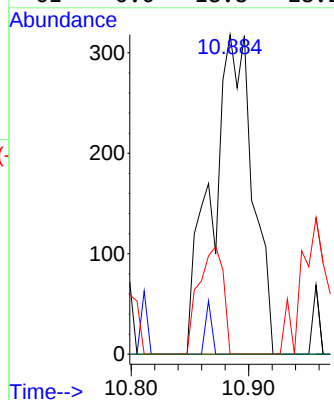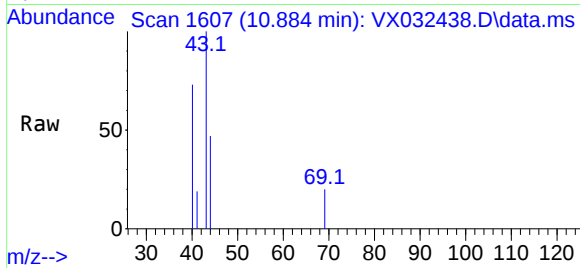


#76
1,2,3-Trichloropropane
Concen: 26.647 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 75 Resp: 47031


Ion	Ratio	Lower	Upper
75	100		
77	1.1	20.0	60.0#

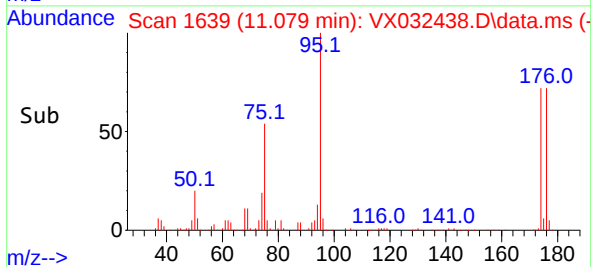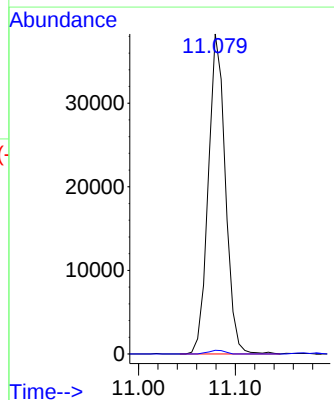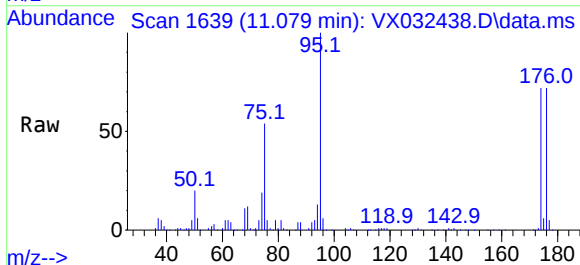






#79
2-Chlorotoluene
Concen: 0.645 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA



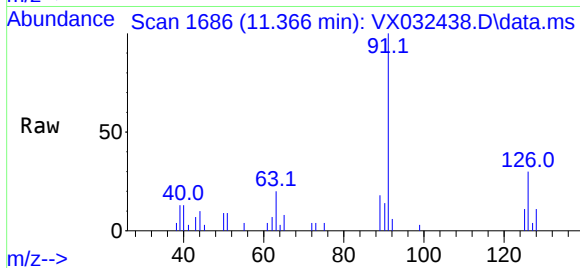



Tgt Ion: 91 Resp: 2797
Ion Ratio Lower Upper
91 100
126 28.2 17.1 51.2



#81
trans-1,4-Dichloro-2-butene
Concen: 84.791 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion: 75 Resp: 47031
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.1 38.3 57.5#


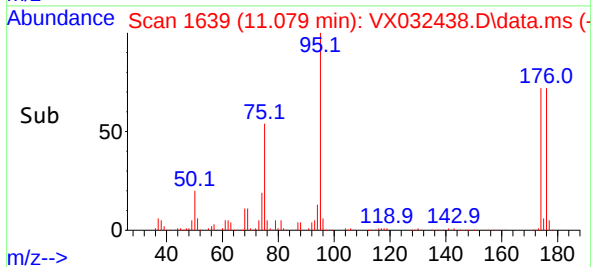

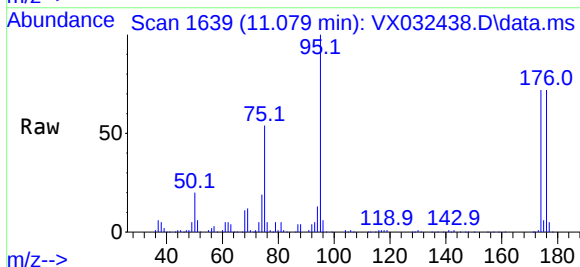




#82
4-Chlorotoluene
Concen: 0.551 ug/l
RT: 11.366 min Scan# 11
Delta R.T. -0.091 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion: 91 Resp: 2797
Ion Ratio Lower Upper
91 100
126 28.2 14.8 44.4

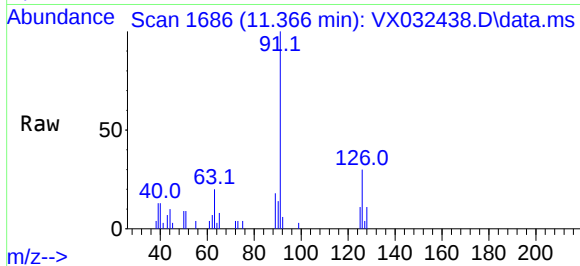

#87
1,3-Dichlorobenzene
Concen: 6.347 ug/l
RT: 12.043 min Scan# 1797
Delta R.T. 0.073 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion:146 Resp: 18452
Ion Ratio Lower Upper
146 100
111 45.5 20.6 61.8
148 64.6 31.7 95.1


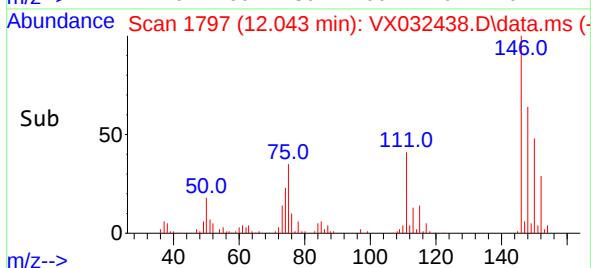

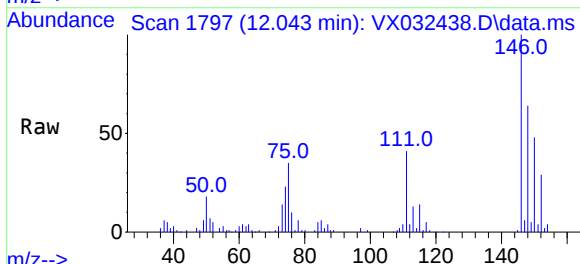




#88
1,4-Dichlorobenzene
Concen: 6.118 ug/l
RT: 12.043 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00




Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA


Tgt Ion:146 Resp: 18452
Ion Ratio Lower Upper
146 100
111 45.5 20.5 61.6
148 64.6 32.2 96.6

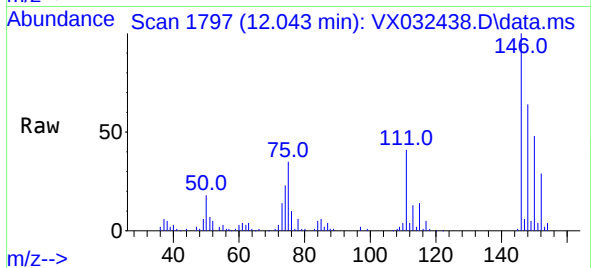

#90
Hexachloroethane
Concen: 0.254 ug/l
RT: 12.616 min Scan# 1891
Delta R.T. 0.073 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Tgt Ion:117 Resp: 227
Ion Ratio Lower Upper
117 100
201 0.0 37.6 112.9#

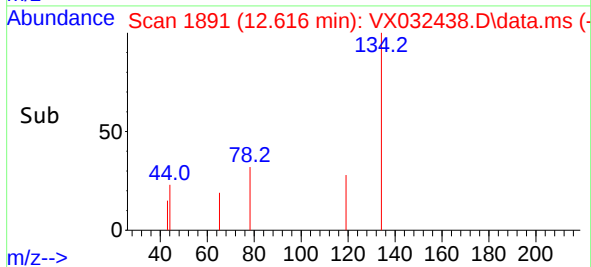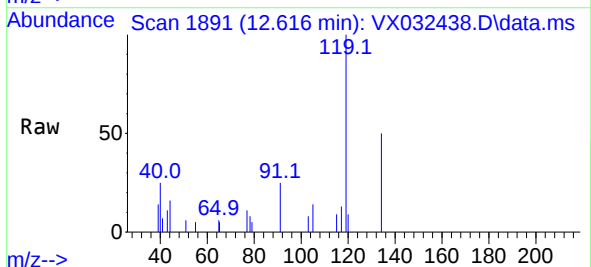



#91
1,2-Dichlorobenzene
Concen: 0.377 ug/l
RT: 12.335 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032438.D
Acq: 27 Oct 2022 19:00

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Tgt Ion:	146	Resp:	1080
Ion	Ratio	Lower	Upper
146	100		
111	47.2	21.5	64.5
148	62.0	32.0	96.2

