

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
 Data File : VX032421.D
 Acq On : 27 Oct 2022 12:14
 Operator : JC/MD
 Sample : VX1027WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1027WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.562	557	570	582	rBV3	2900	9985	1.52%	0.286%
2	5.385	694	705	719	rBV	82511	231694	35.18%	6.627%
3	5.550	721	732	748	rVB	140632	389226	59.10%	11.133%
4	5.952	789	798	812	rBV	86564	225319	34.21%	6.445%
5	6.763	921	931	944	rBV	204577	485714	73.74%	13.893%
6	8.647	1233	1240	1253	rBV	419079	658640	100.00%	18.839%
7	10.055	1465	1471	1485	rBV	417745	556170	84.44%	15.908%
8	11.079	1634	1639	1656	rBV	331393	426465	64.75%	12.198%
9	12.024	1788	1794	1804	rBV	406641	512915	77.87%	14.671%


Sum of corrected areas: 3496128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032421.D
Acq On : 27 Oct 2022 12:14
Operator : JC/MD
Sample : VX1027WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1027WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

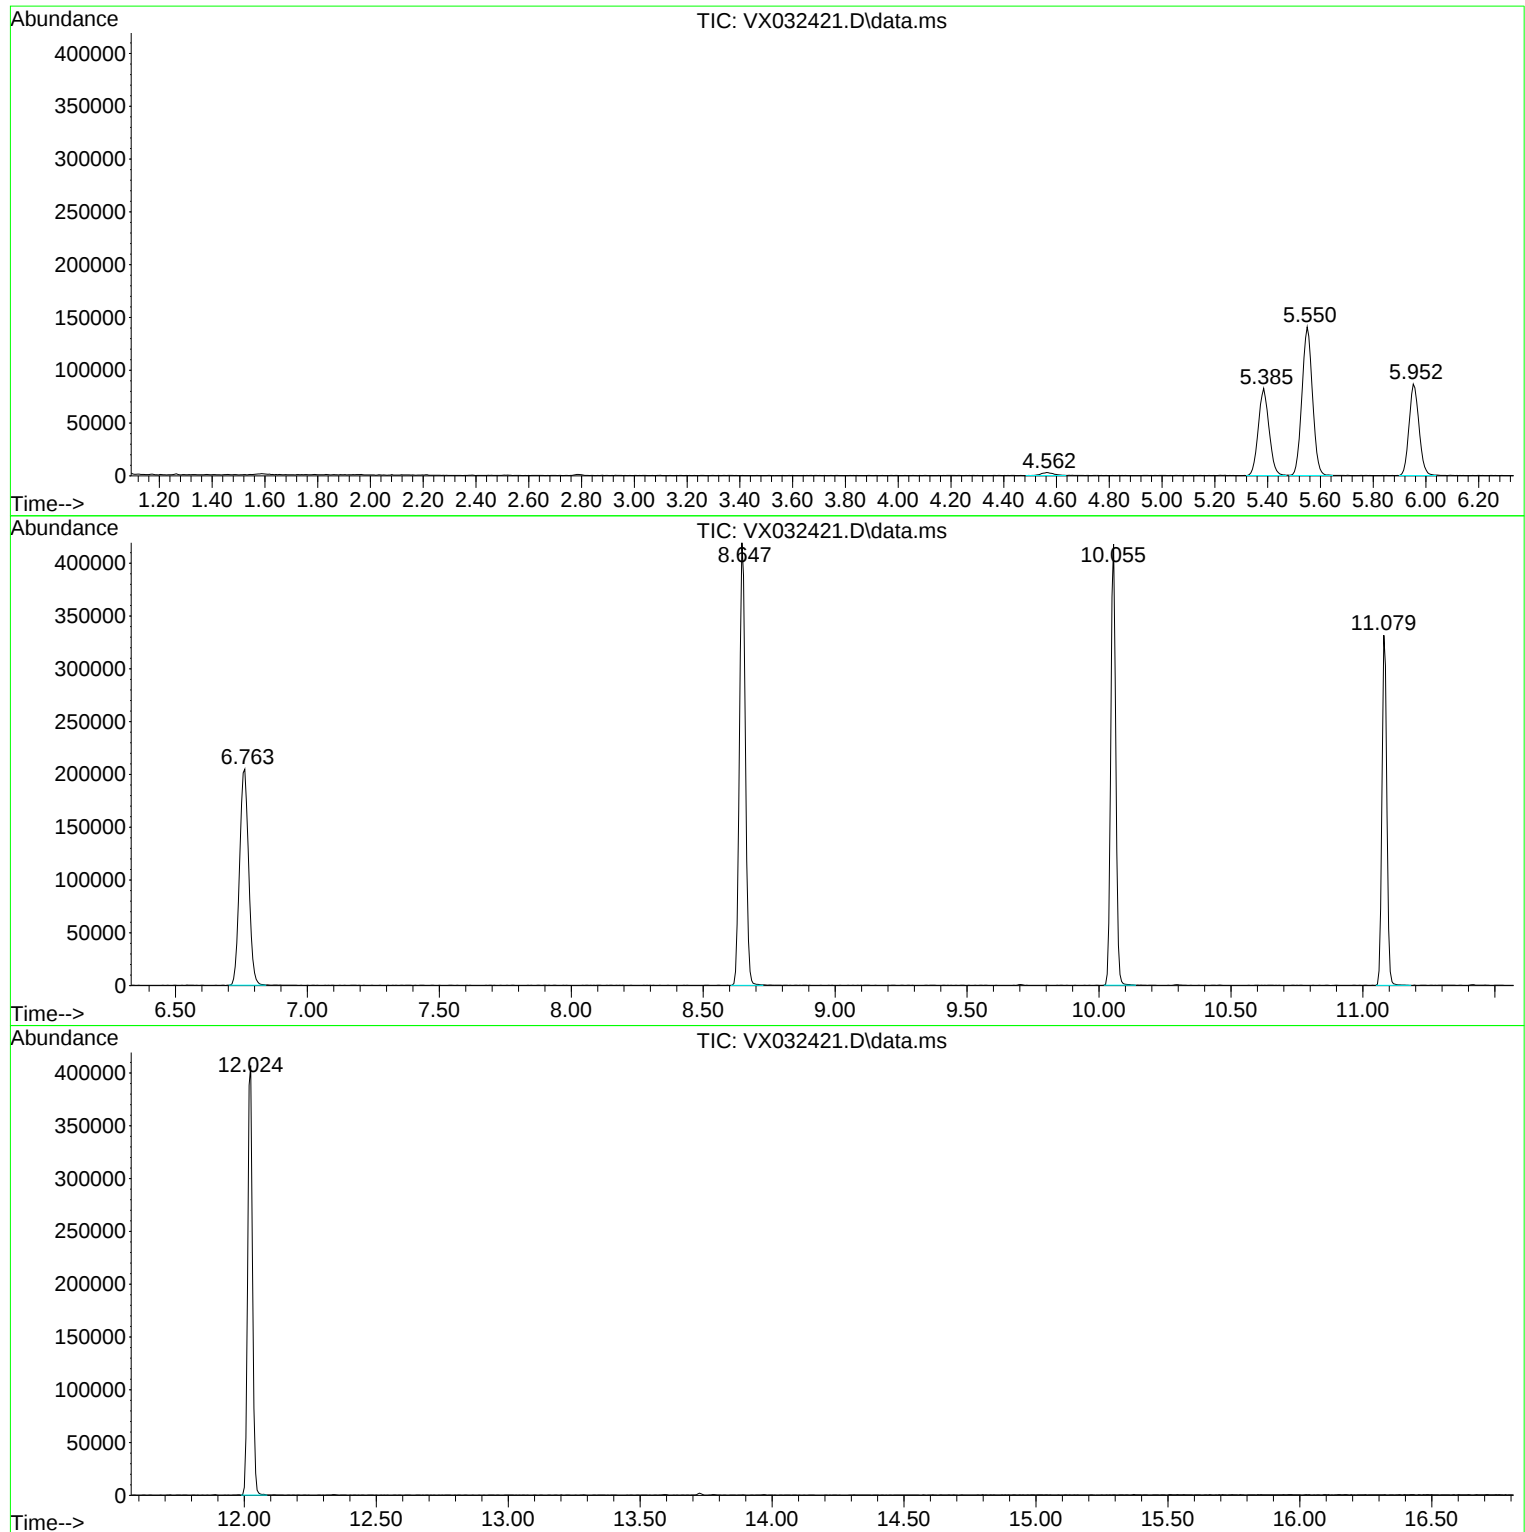

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032421.D
Acq On : 27 Oct 2022 12:14
Operator : JC/MD
Sample : VX1027WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1027WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032421.D
Acq On : 27 Oct 2022 12:14
Operator : JC/MD
Sample : VX1027WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1027WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------