

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032425.D
Acq On : 27 Oct 2022 13:57
Operator : JC/MD
Sample : N5290-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-7

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	72	79	84	rBV4	2836	6303	1.03%	0.193%
2	5.385	695	705	720	rBV	73056	215509	35.24%	6.589%
3	5.556	722	733	747	rVB	129522	362830	59.33%	11.093%
4	5.958	788	799	817	rBV	79204	212909	34.82%	6.509%
5	6.763	921	931	945	rBV	193983	457151	74.76%	13.976%
6	8.647	1234	1240	1258	rBV	379128	611526	100.00%	18.696%
7	10.055	1465	1471	1483	rBV	394062	519871	85.01%	15.894%
8	11.079	1634	1639	1648	rBV	332417	428557	70.08%	13.102%
9	12.024	1788	1794	1805	rBV	365693	456207	74.60%	13.948%


Sum of corrected areas: 3270863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032425.D
Acq On : 27 Oct 2022 13:57
Operator : JC/MD
Sample : N5290-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

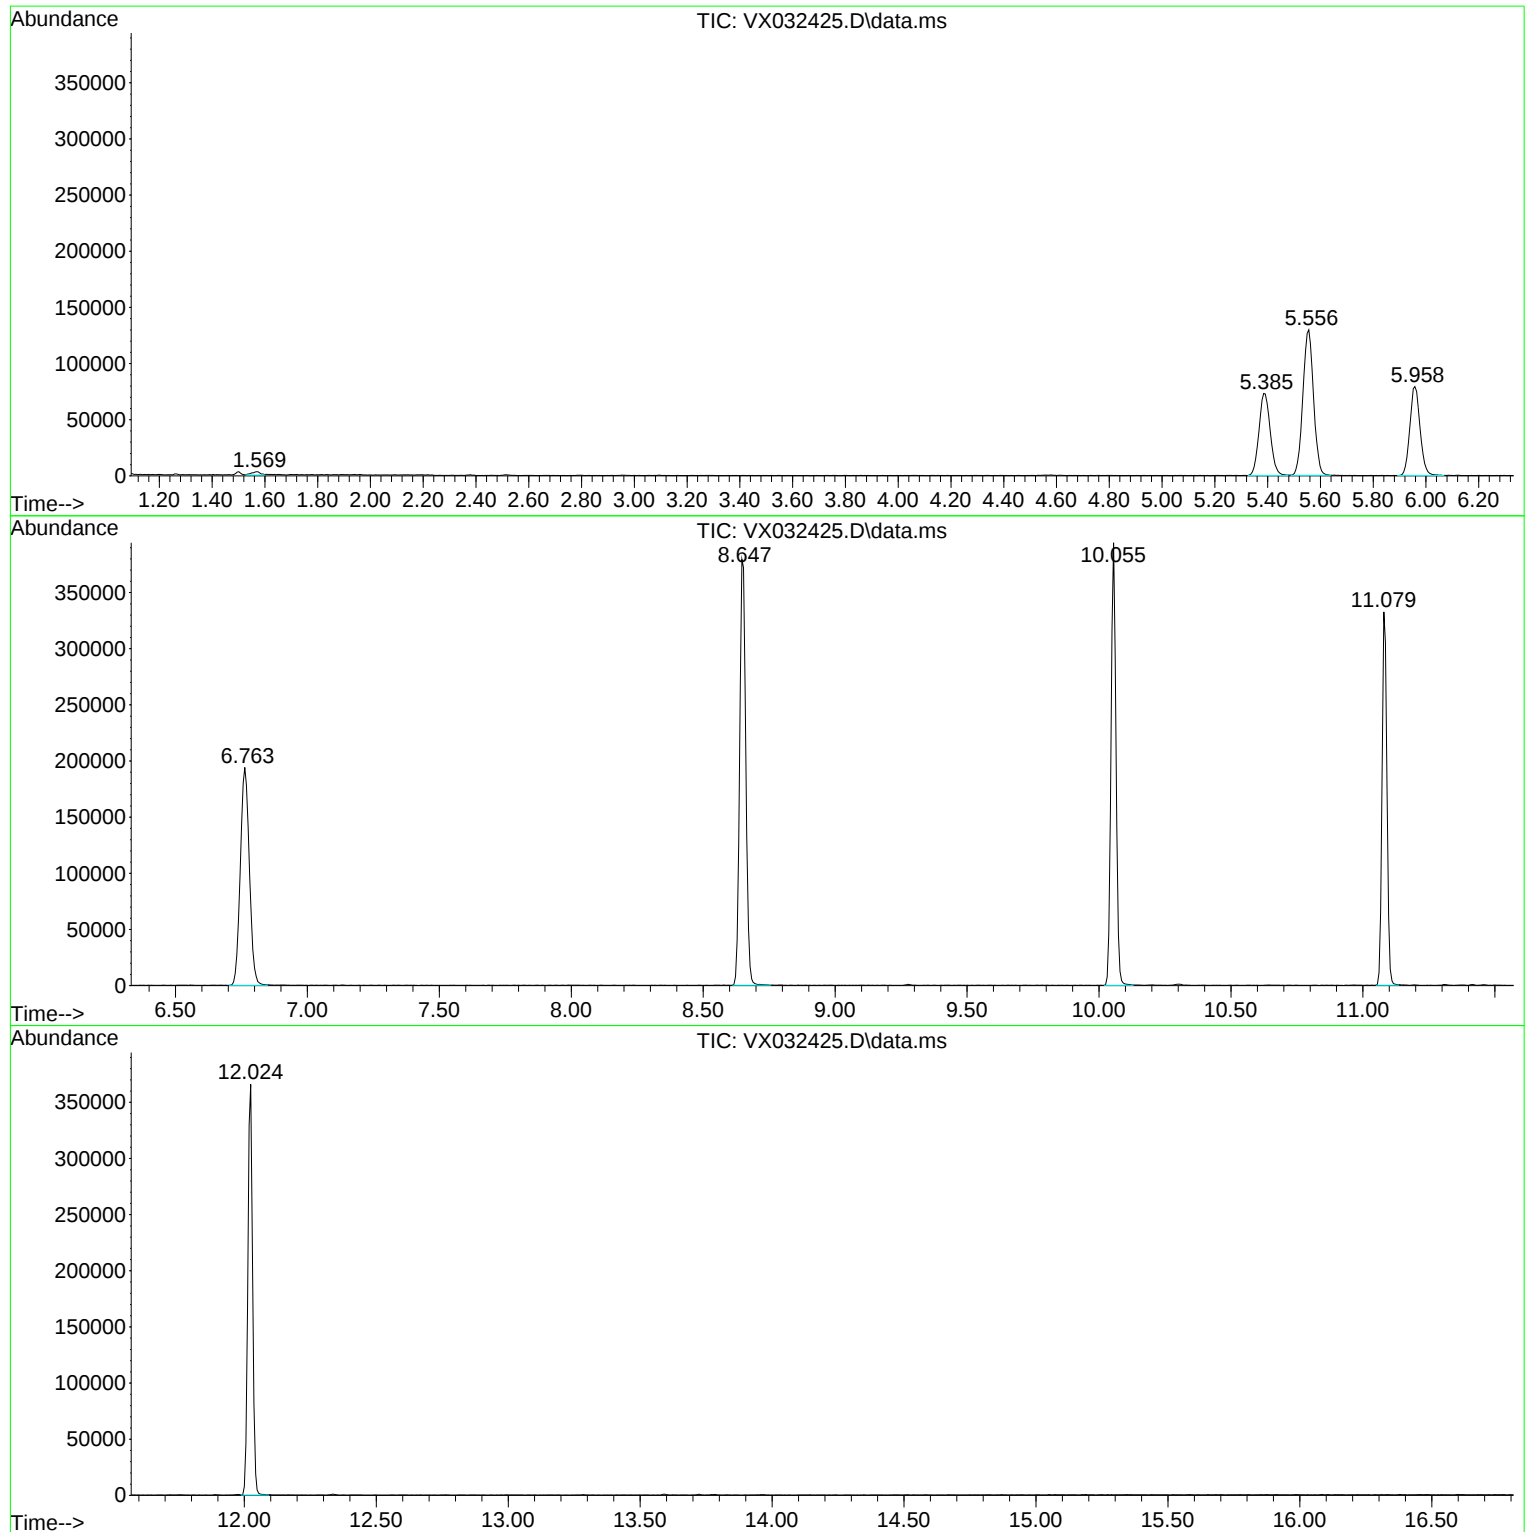

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032425.D
Acq On : 27 Oct 2022 13:57
Operator : JC/MD
Sample : N5290-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032425.D
Acq On : 27 Oct 2022 13:57
Operator : JC/MD
Sample : N5290-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------