

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032426.D
Acq On : 27 Oct 2022 14:20
Operator : JC/MD
Sample : N5290-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.496	63	67	72	rVB	5796	6959	1.13%	0.209%
2	5.391	694	706	718	rBV2	74984	218009	35.33%	6.549%
3	5.550	722	732	753	rVB	130161	368715	59.76%	11.077%
4	5.958	789	799	815	rBV	80878	215303	34.89%	6.468%
5	6.763	921	931	944	rBV	195444	463071	75.05%	13.911%
6	8.653	1234	1241	1251	rBV	390118	617024	100.00%	18.537%
7	10.055	1465	1471	1482	rBV	398451	525146	85.11%	15.776%
8	11.079	1634	1639	1651	rBV	332253	435230	70.54%	13.075%
9	12.024	1789	1794	1805	rBV	382993	479238	77.67%	14.397%




Sum of corrected areas: 3328695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032426.D
Acq On : 27 Oct 2022 14:20
Operator : JC/MD
Sample : N5290-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

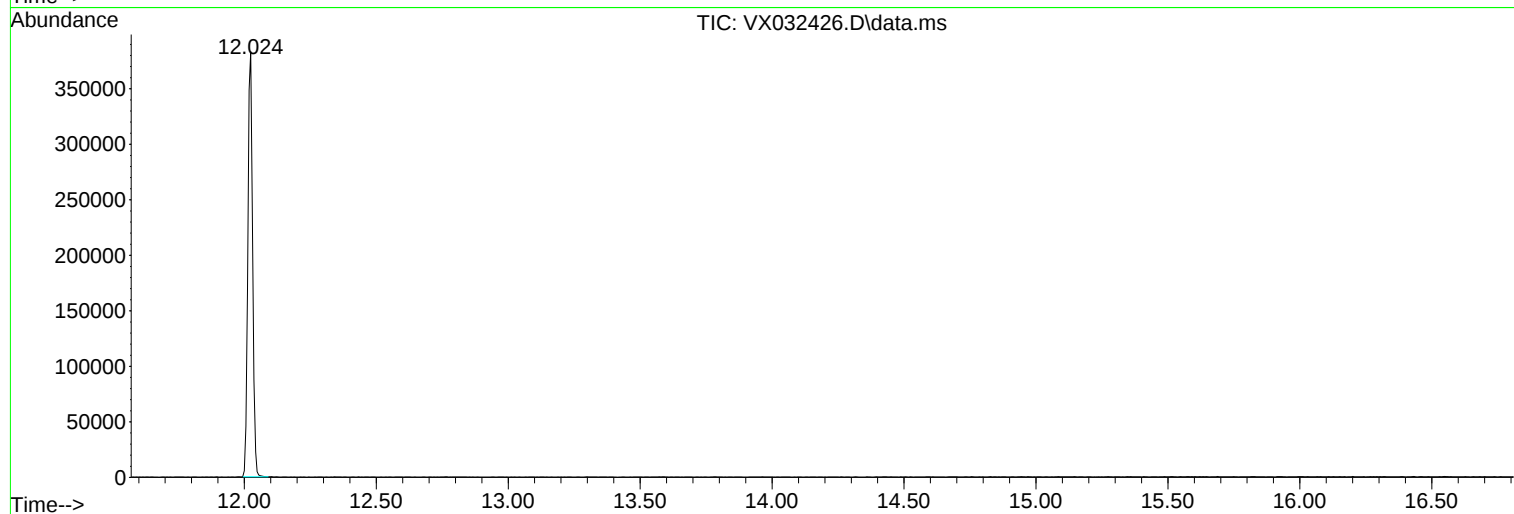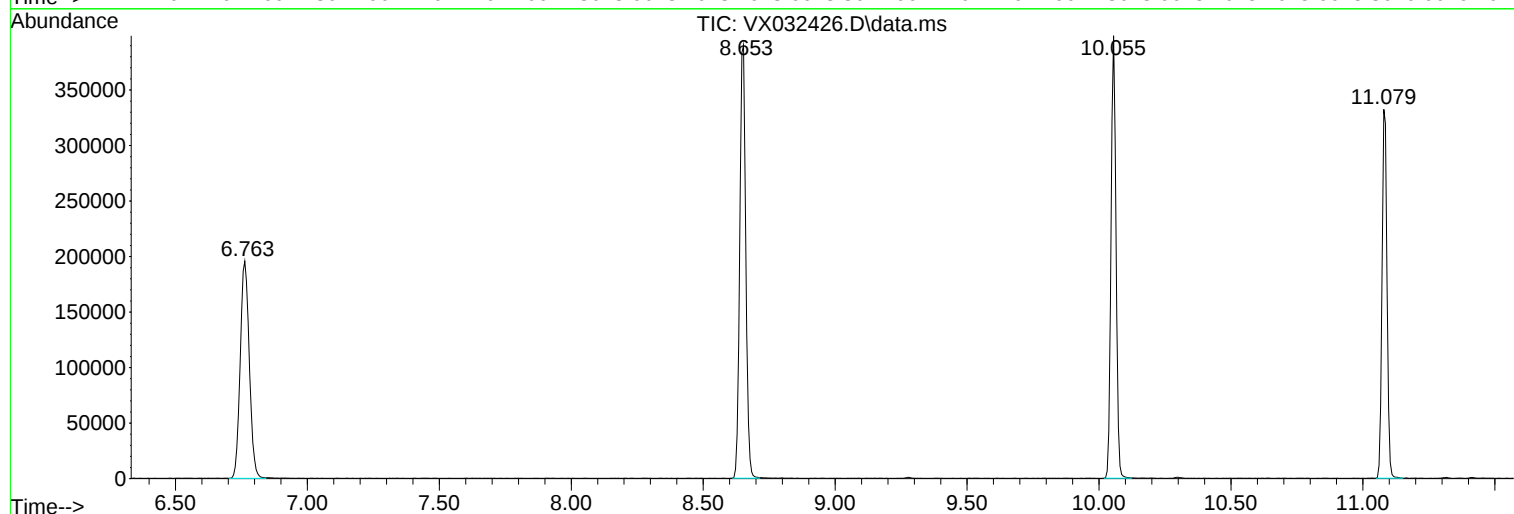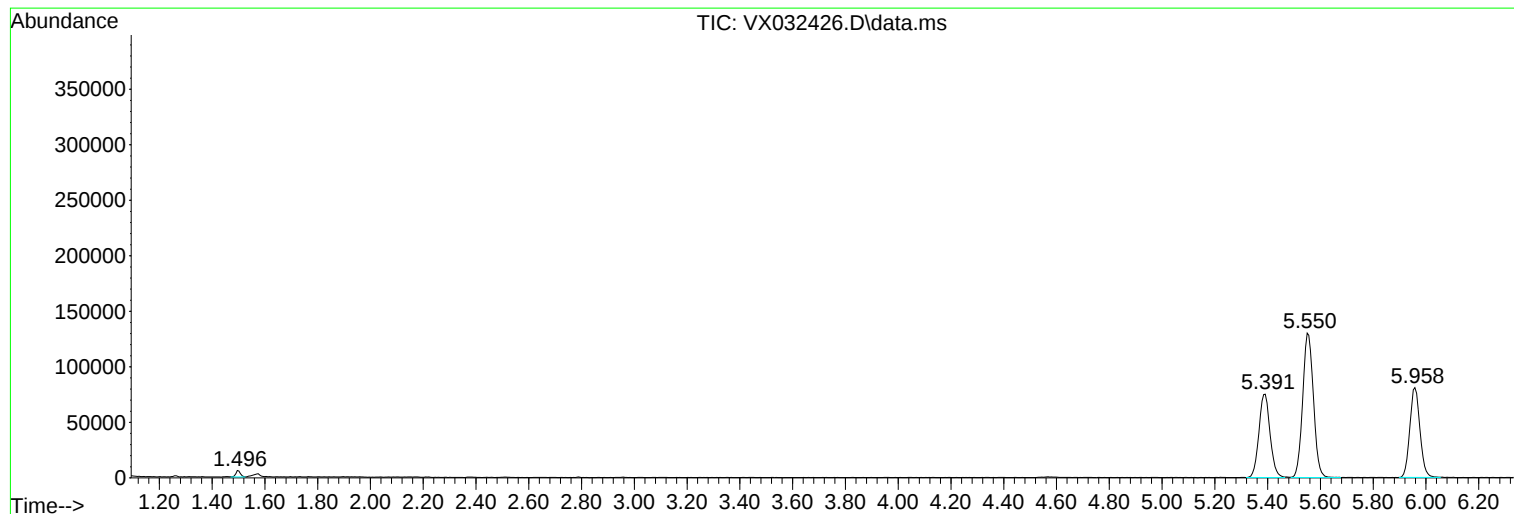

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032426.D
Acq On : 27 Oct 2022 14:20
Operator : JC/MD
Sample : N5290-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032426.D
Acq On : 27 Oct 2022 14:20
Operator : JC/MD
Sample : N5290-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
257248-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------