

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
 Data File : VX032438.D
 Acq On : 27 Oct 2022 19:00
 Operator : JC/MD
 Sample : N5315-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 221026039-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.173	12	14	24	rVB	13688	20959	3.35%	0.511%
2	1.355	40	44	53	rVB2	13957	18373	2.93%	0.448%
3	2.130	166	171	180	rVB	19459	28474	4.55%	0.694%
4	2.386	205	213	223	rBV2	10441	19037	3.04%	0.464%
5	2.477	223	228	235	rBV3	2595	8540	1.36%	0.208%
6	2.959	299	307	322	rBV2	20248	48424	7.73%	1.180%
7	4.562	553	570	583	rBV	26218	90453	14.45%	2.204%
8	5.007	632	643	660	rBV2	48522	153157	24.46%	3.732%
9	5.385	695	705	722	rBV	72843	212864	34.00%	5.187%
10	5.556	722	733	750	rVB	127308	361768	57.78%	8.815%
11	5.958	789	799	809	rBV	80671	214152	34.20%	5.218%
12	6.037	809	812	820	rVB4	3091	6489	1.04%	0.158%
13	6.763	922	931	945	rBV	193485	457675	73.09%	11.152%
14	7.677	1074	1081	1089	rBV3	3308	7176	1.15%	0.175%
15	8.653	1234	1241	1248	rBV	386729	617726	98.65%	15.051%
16	9.488	1373	1378	1386	rBV2	9403	14787	2.36%	0.360%
17	10.055	1465	1471	1485	rVB2	404796	626152	100.00%	15.257%
18	10.305	1505	1512	1519	rBV	15274	21886	3.50%	0.533%
19	10.640	1563	1567	1575	rVB	12313	16897	2.70%	0.412%
20	10.963	1614	1620	1626	rVB3	5476	7659	1.22%	0.187%
21	11.079	1634	1639	1646	rBV	352086	445336	71.12%	10.851%
22	11.366	1683	1686	1691	rBV	5728	6686	1.07%	0.163%
23	11.616	1722	1727	1734	rVB	6325	8973	1.43%	0.219%
24	11.890	1766	1772	1778	rBV2	15824	21732	3.47%	0.530%
25	12.024	1788	1794	1802	rBV2	414544	572088	91.37%	13.939%
26	12.244	1822	1830	1834	rBV2	17281	23458	3.75%	0.572%
27	12.335	1839	1845	1852	rVB4	4607	8602	1.37%	0.210%
28	12.908	1935	1939	1944	rVV2	7976	15044	2.40%	0.367%
29	13.286	1995	2001	2006	rBV6	5028	8169	1.30%	0.199%
30	13.475	2027	2032	2035	rBV2	12592	17074	2.73%	0.416%
31	13.932	2101	2107	2113	rBV5	3328	6740	1.08%	0.164%
32	14.664	2220	2227	2233	rBV4	4372	8856	1.41%	0.216%
33	16.328	2493	2500	2506	rBV	5008	8698	1.39%	0.212%




Sum of corrected areas: 4104104

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032438.D
Acq On : 27 Oct 2022 19:00
Operator : JC/MD
Sample : N5315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

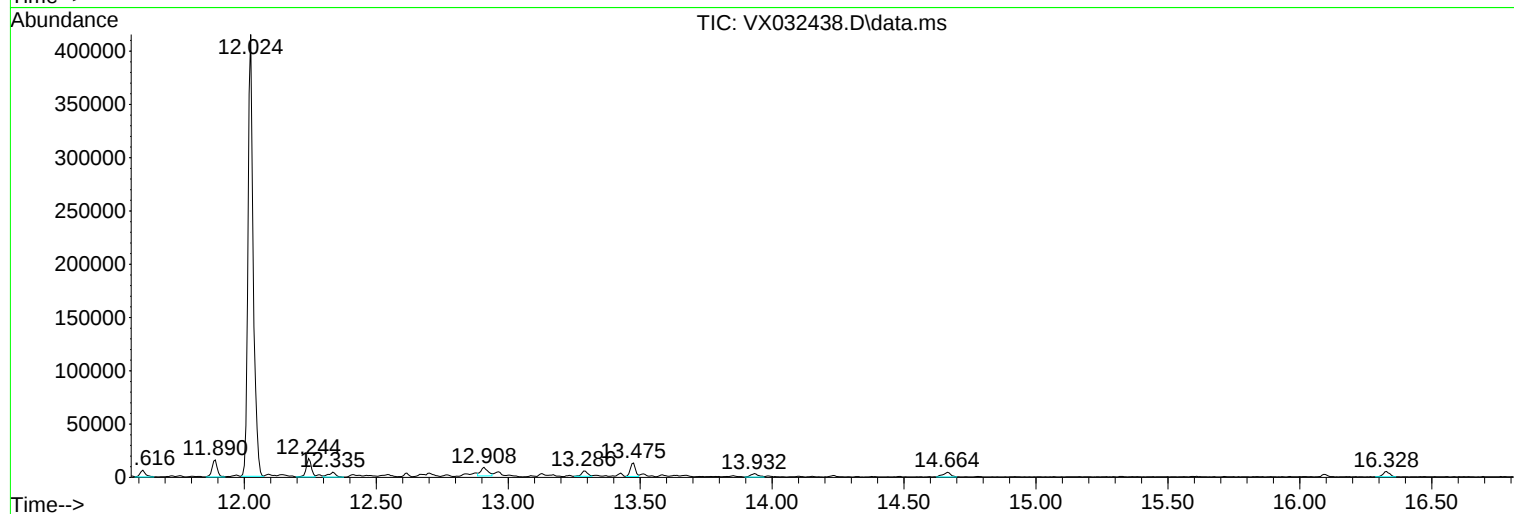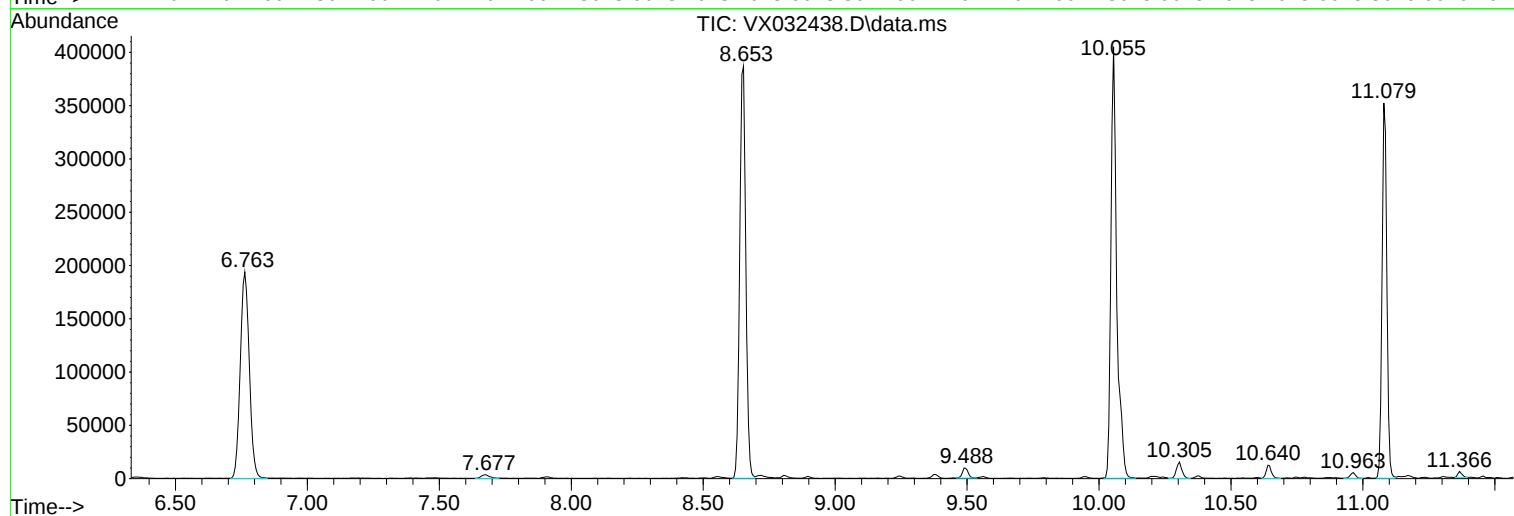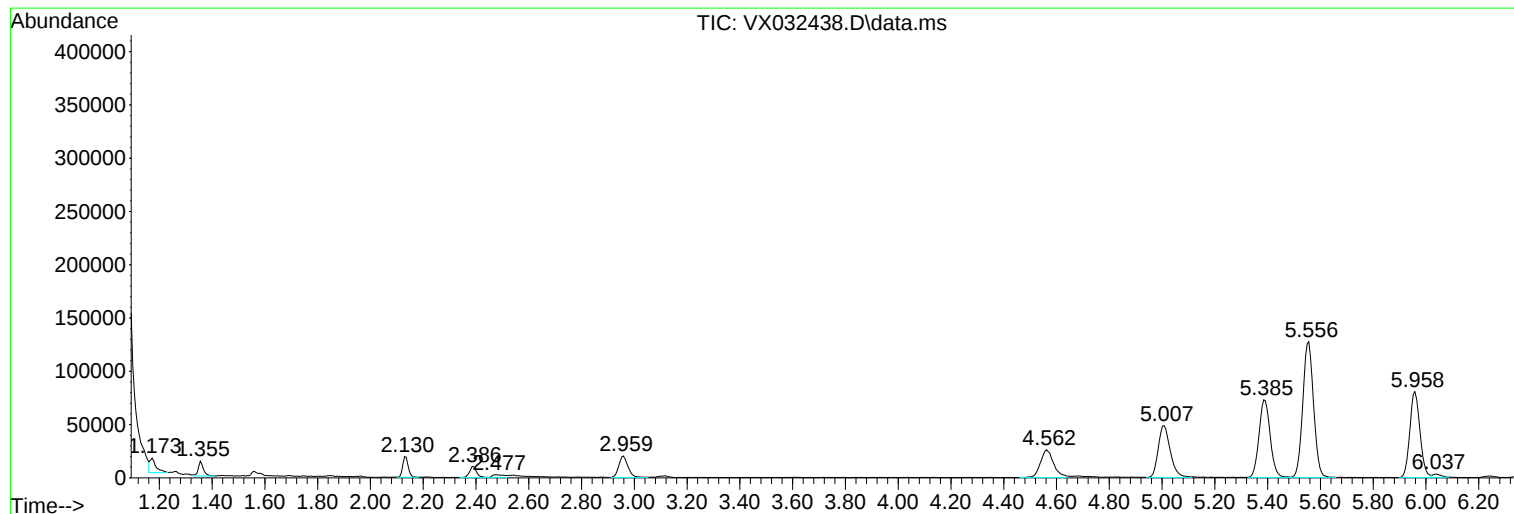

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032438.D
Acq On : 27 Oct 2022 19:00
Operator : JC/MD
Sample : N5315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032438.D
Acq On : 27 Oct 2022 19:00
Operator : JC/MD
Sample : N5315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
221026039-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------