

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
 Data File : VX032441.D
 Acq On : 27 Oct 2022 20:09
 Operator : JC/MD
 Sample : N5323-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 024-OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	74	83	90	rBV3	3446	8606	1.39%	0.246%
2	2.380	206	212	223	rBV	7284	11917	1.92%	0.340%
3	5.391	694	706	722	rBV	74411	216267	34.87%	6.173%
4	5.556	722	733	751	rVB	129197	362007	58.36%	10.333%
5	5.958	789	799	815	rBV	79524	214402	34.57%	6.120%
6	6.763	918	931	946	rBV	193688	461987	74.48%	13.187%
7	8.653	1234	1241	1252	rBV	389609	620275	100.00%	17.706%
8	10.055	1465	1471	1482	rBV	395896	530926	85.60%	15.155%
9	10.659	1565	1570	1580	rVB	38224	50467	8.14%	1.441%
10	11.079	1634	1639	1654	rBV	349387	452440	72.94%	12.915%
11	11.750	1745	1749	1757	rBV	37262	51434	8.29%	1.468%
12	12.024	1788	1794	1804	rBV	409795	511673	82.49%	14.606%
13	12.622	1888	1892	1904	rBV4	5346	10878	1.75%	0.311%




Sum of corrected areas: 3503279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032441.D
Acq On : 27 Oct 2022 20:09
Operator : JC/MD
Sample : N5323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
024-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

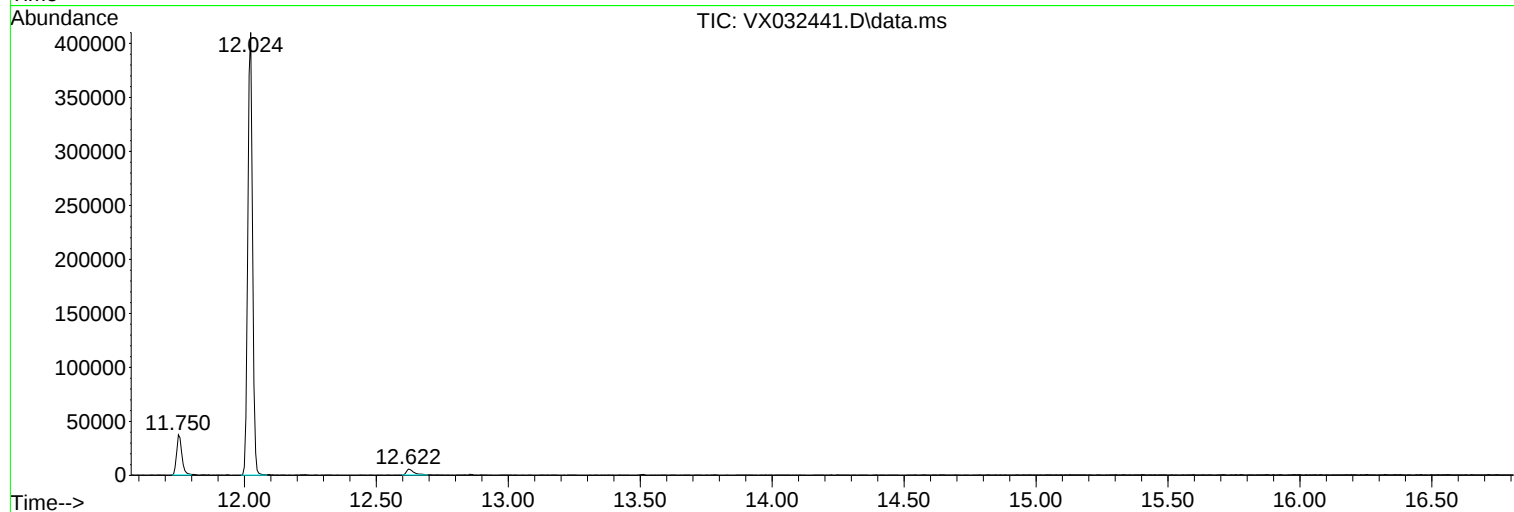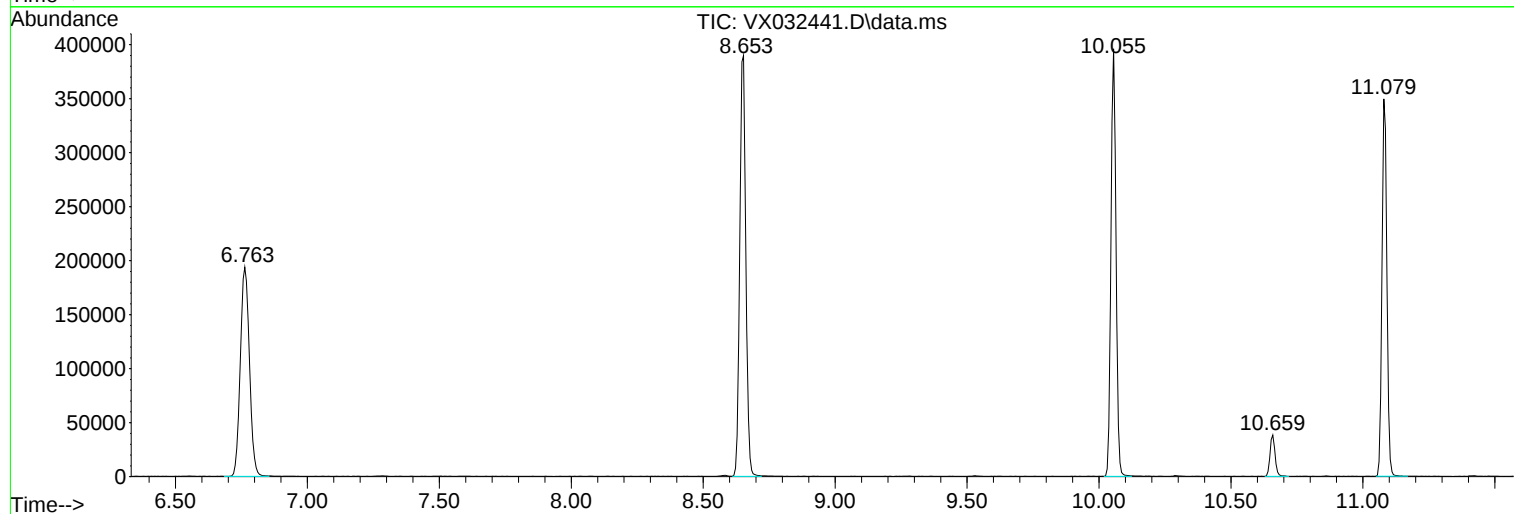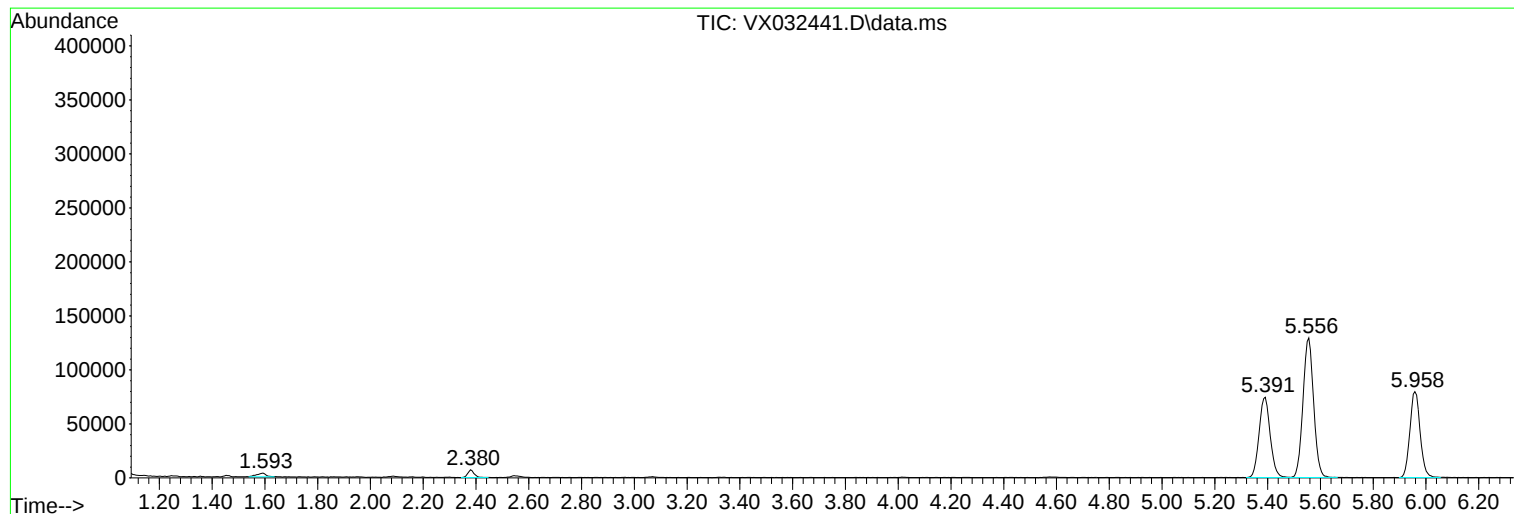

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032441.D
Acq On : 27 Oct 2022 20:09
Operator : JC/MD
Sample : N5323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
024-OUTFALL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzaldehyde Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.750	5.03 ug/l	51434	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzaldehyde	106	C7H6O	000100-52-7	97
2			2-fluoro-1-phenylethanone	138	C8H7FO	1000456-25-8	53
3			Ethanone, 2-bromo-1-phenyl-	198	C8H7BrO	000070-11-1	50
4			Benzenepropanenitrile, .beta.-oxo-	145	C9H7NO	000614-16-4	50
5			Benzoyl bromide	184	C7H5BrO	000618-32-6	50

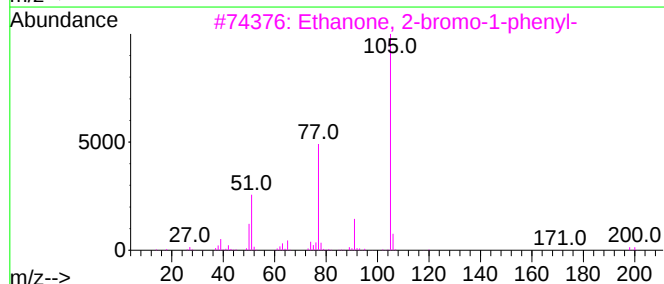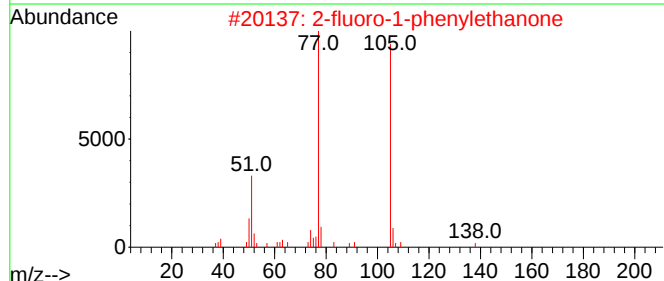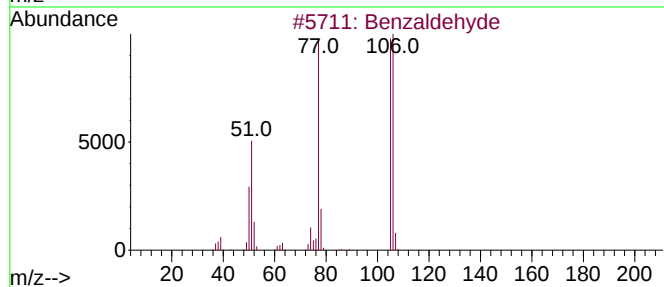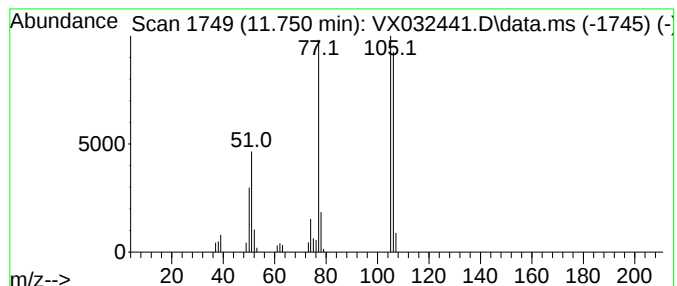

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102722\
Data File : VX032441.D
Acq On : 27 Oct 2022 20:09
Operator : JC/MD
Sample : N5323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
024-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzaldehyde	11.750	5.0	ug/l	51434	4	12.024	511673	50.0