


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102820\
 Data File : VX019155.D
 Acq On : 28 Oct 2020 10:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
 Title : SW846 8260
 Last Update : Tue Oct 27 13:55:07 2020

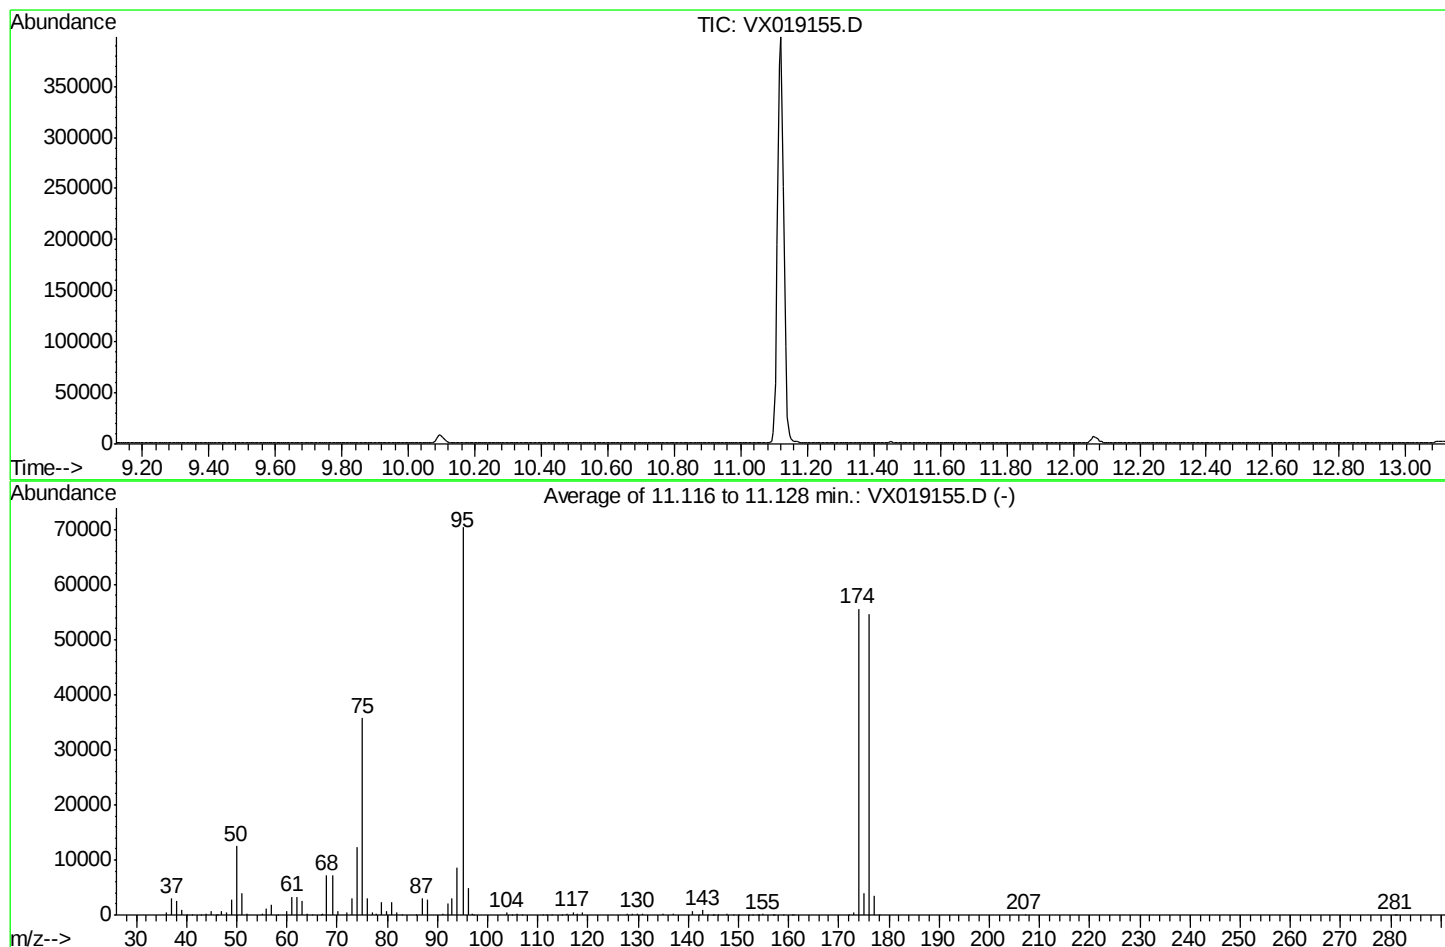

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12454	PASS
75	95	30	60	50.8	35720	PASS
95	95	100	100	100.0	70354	PASS
96	95	5	9	6.8	4793	PASS
173	174	0.00	2	0.8	471	PASS
174	95	50	100	79.0	55562	PASS
175	174	5	9	7.2	4007	PASS
176	174	95	101	98.3	54602	PASS
177	176	5	9	6.3	3438	PASS