

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025003.D
 Acq On : 28 Oct 2021 13:54
 Operator : JC/MD
 Sample : VX1028WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 29 06:47:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 28 12:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	152841	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	10.055	117	135524	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	59888	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	49827	51.142	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 102.280%			
7) Chloroethane-d5	1.666	69	37306	56.018	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 112.040%			
11) 1,1-Dichloroethene-d2	2.306	63	92543	38.547	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.100%			
21) 2-Butanone-d5	4.465	46	107989	110.968	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 110.970%			
24) Chloroform-d	5.062	84	128008	50.213	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.420%			
26) 1,2-Dichloroethane-d4	5.964	65	98845	52.874	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.740%			
32) Benzene-d6	5.977	84	205479	53.417	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.840%			
36) 1,2-Dichloropropane-d6	7.312	67	71314	54.400	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 108.800%			
41) Toluene-d8	8.653	98	197372	53.632	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.260%			
43) trans-1,3-Dichloroprop...	8.952	79	40807	54.167	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 108.340%			
47) 2-Hexanone-d5	9.458	63	474	0.710	ug/L	0.07
Spiked Amount 100.000	Range 45 - 130		Recovery = 0.710%#			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	96589	54.488	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 108.980%			
66) 1,2-Dichlorobenzene-d4	12.323	152	62149	53.480	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 106.960%			
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.300	96	780	0.820	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025003.D
Acq On : 28 Oct 2021 13:54
Operator : JC/MD
Sample : VX1028WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Oct 29 06:47:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 28 12:38:37 2021
Response via : Initial Calibration

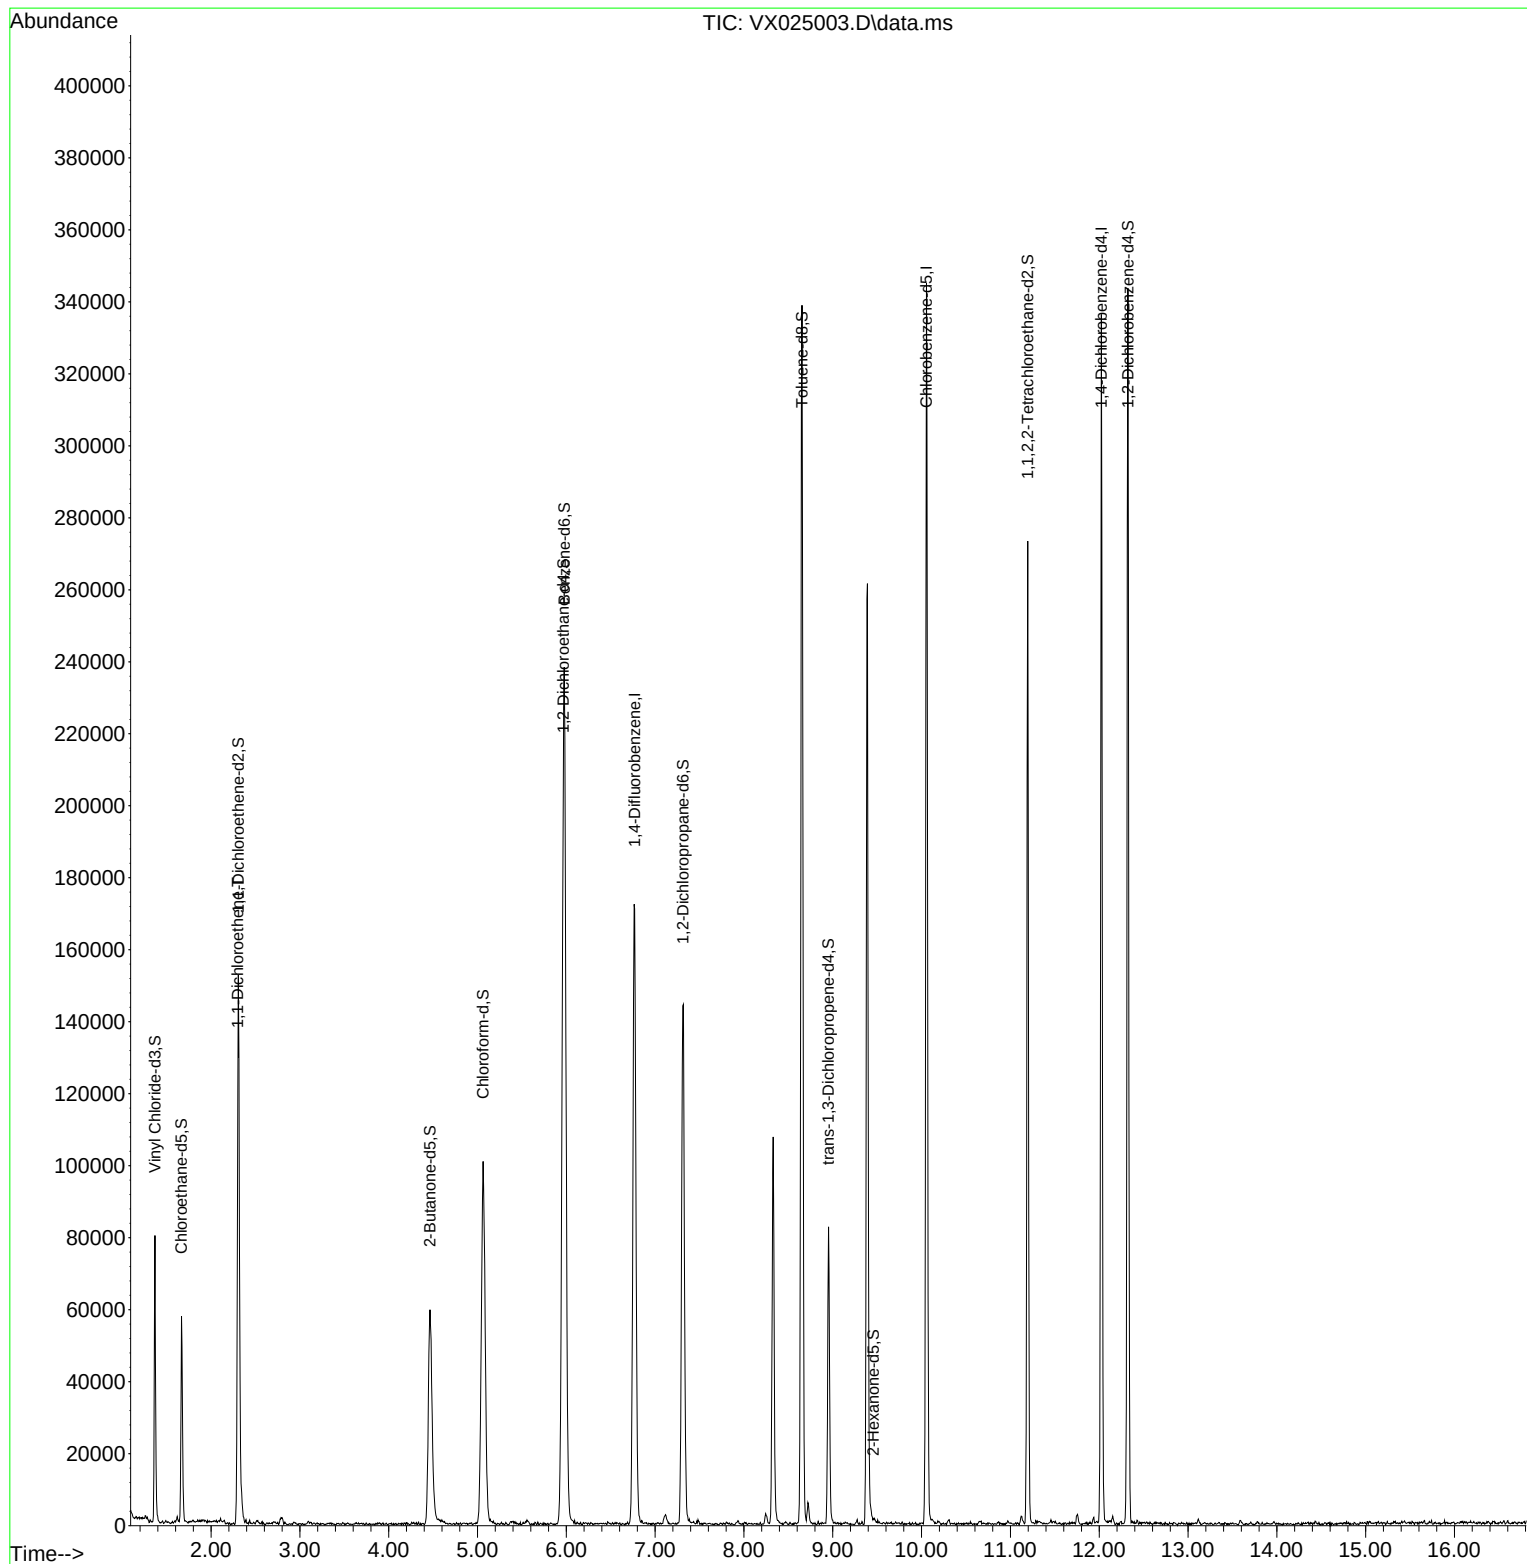

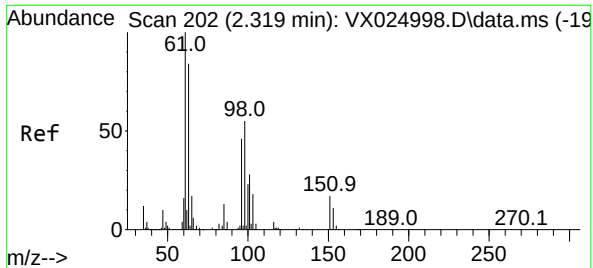

#12
 1,1-Dichloroethene
 Concen: 0.820 ug/L
 RT: 2.300 min Scan# 199
 Delta R.T. -0.018 min
 Lab File: VX025003.D
 Acq: 28 Oct 2021 13:54

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 96 Resp: 780
 Ion Ratio Lower Upper
 96 100
 61 1190.9 109.9 204.1#
 63 9861.5 92.4 171.6#

