




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025003.D
Acq On : 28 Oct 2021 13:54
Operator : JC/MD
Sample : VX1028WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK616

Manual Integrations
APPROVED

MMDadoda
11/1/2021 12:58:38 PM

Quant Time: Oct 29 06:47:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 28 12:38:37 2021
Response via : Initial Calibration

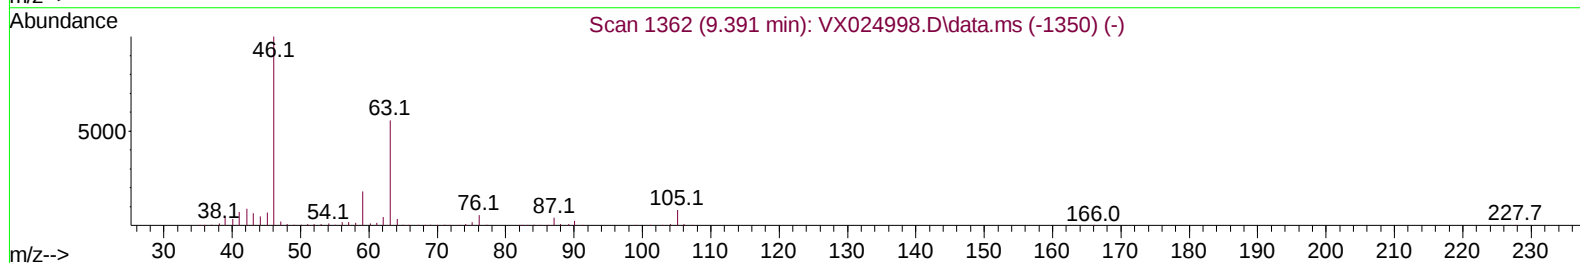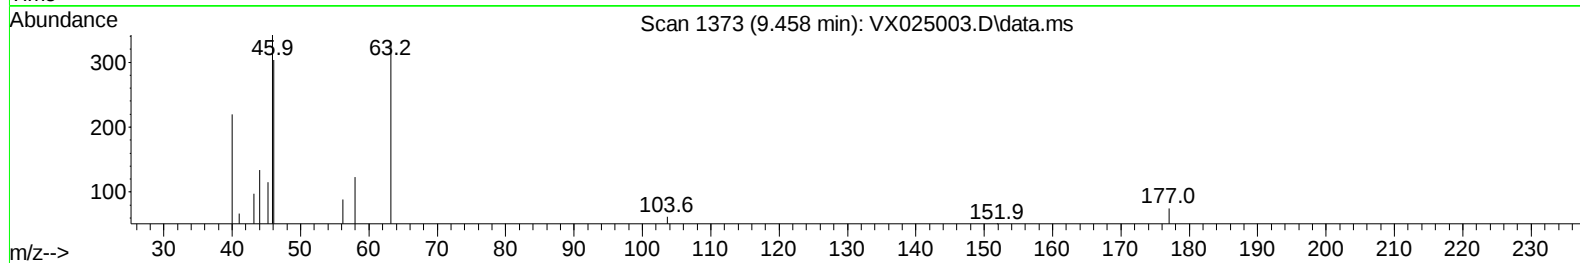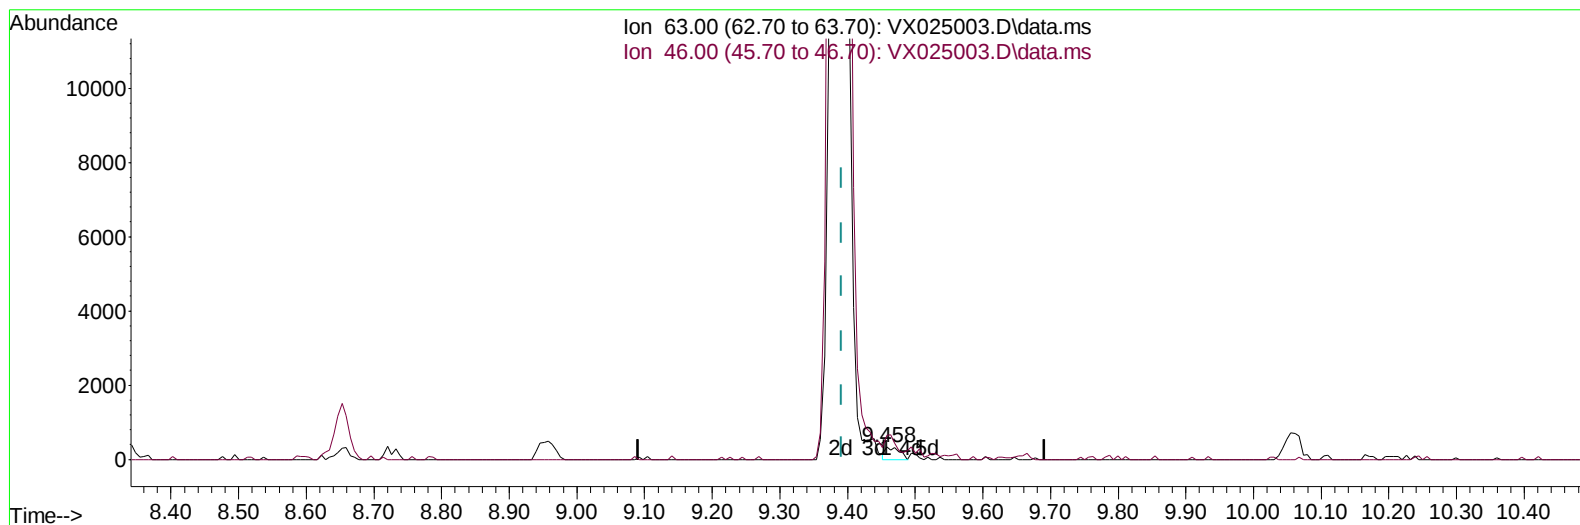

TIC: VX025003.D\data.ms

(47) 2-Hexanone-d5 (S)

9.458min (+ 0.067) 0.71 ug/L

response 474

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	140.40	166.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025003.D
 Acq On : 28 Oct 2021 13:54
 Operator : JC/MD
 Sample : VX1028WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK616

Manual Integrations
 APPROVED

MMDadoda
 11/1/2021 12:58:38 PM

Quant Time: Oct 29 06:47:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 28 12:38:37 2021
 Response via : Initial Calibration

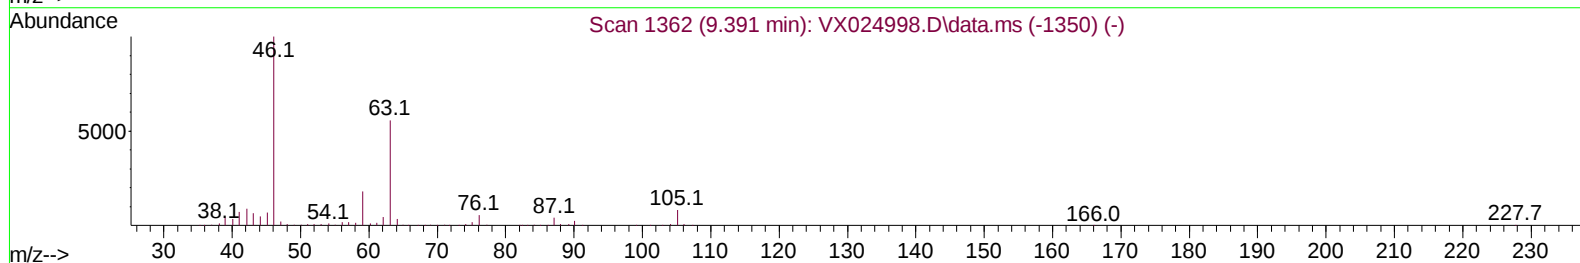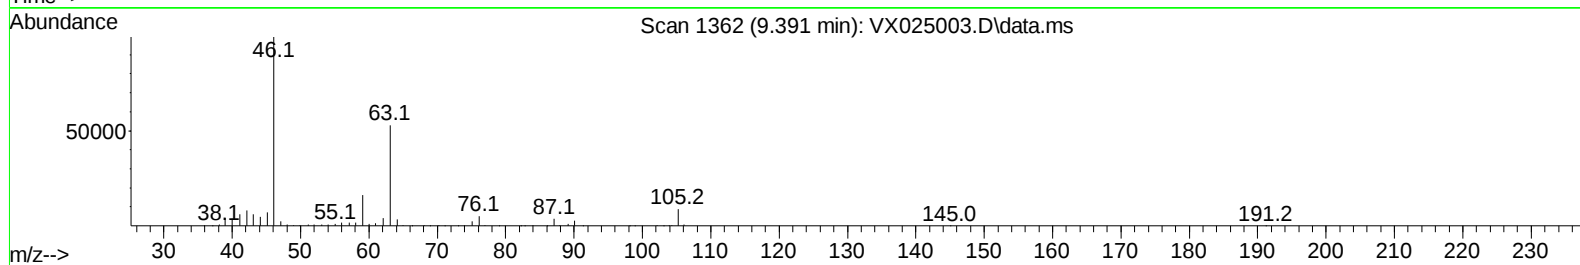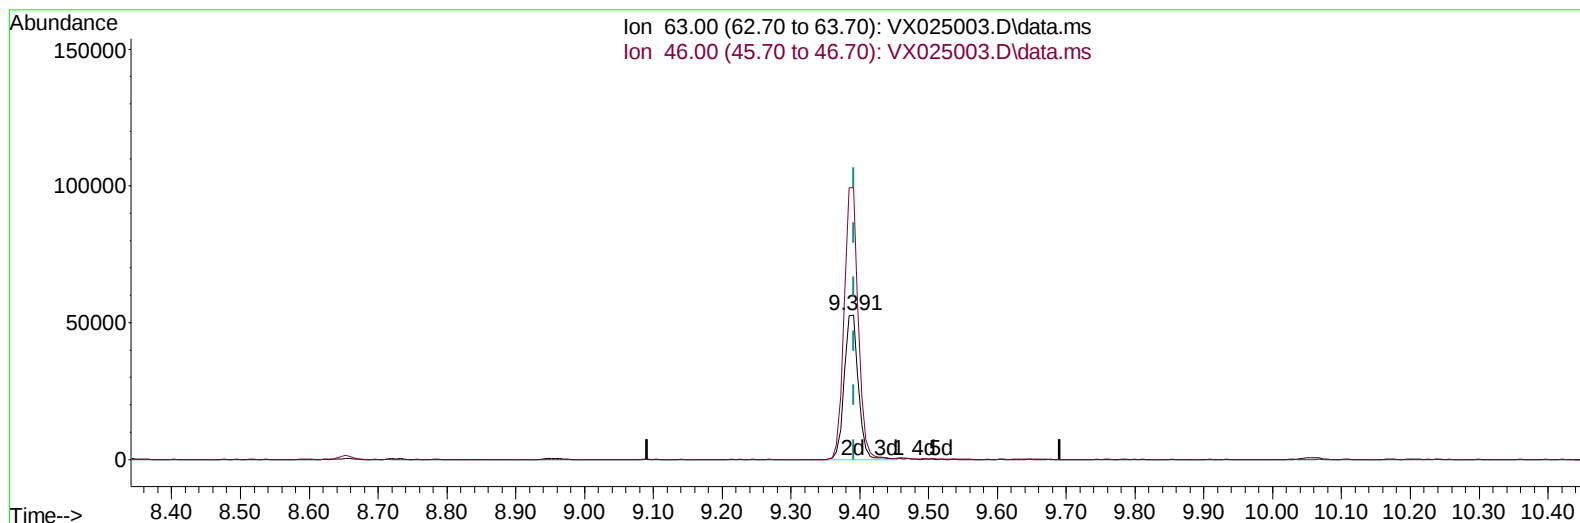

TIC: VX025003.D\data.ms

(47) 2-Hexanone-d5 (S)

9.391min (-0.000) 111.76 ug/L m

response 74590

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	140.40	1.06#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025003.D
 Acq On : 28 Oct 2021 13:54
 Operator : JC/MD
 Sample : VX1028WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK616

Manual Integrations
 APPROVED

MMDadoda
 11/1/2021 12:58:38 PM

Quant Time: Oct 29 06:47:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 28 12:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	152841	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	10.055	117	135524	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	59888	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	49827	51.142	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	102.280%	
7) Chloroethane-d5	1.666	69	37306	56.018	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	112.040%	
11) 1,1-Dichloroethene-d2	2.306	63	92543	38.547	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	77.100%	
21) 2-Butanone-d5	4.465	46	107989	110.968	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	110.970%	
24) Chloroform-d	5.062	84	128008	50.213	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.420%	
26) 1,2-Dichloroethane-d4	5.964	65	98845	52.874	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	105.740%	
32) Benzene-d6	5.977	84	205479	53.417	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.840%	
36) 1,2-Dichloropropane-d6	7.312	67	71314	54.400	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	108.800%	
41) Toluene-d8	8.653	98	197372	53.632	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	107.260%	
43) trans-1,3-Dichloroprop...	8.952	79	40807	54.167	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	108.340%	
47) 2-Hexanone-d5	9.391	63	74590m	111.756	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	111.760%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	96589	54.488	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	108.980%	
66) 1,2-Dichlorobenzene-d4	12.323	152	62149	53.480	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	106.960%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025003.D
Acq On : 28 Oct 2021 13:54
Operator : JC/MD
Sample : VX1028WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK616

Manual Integrations
APPROVED

MMDadoda
11/1/2021 12:58:38 PM

Quant Time: Oct 29 06:47:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 28 12:38:37 2021
Response via : Initial Calibration

