




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025005.D
Acq On : 28 Oct 2021 14:41
Operator : JC/MD
Sample : VX1028MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK618

Manual Integrations
APPROVED

MMDadoda
11/1/2021 12:58:48 PM

Quant Time: Oct 29 06:48:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 28 12:38:37 2021
Response via : Initial Calibration

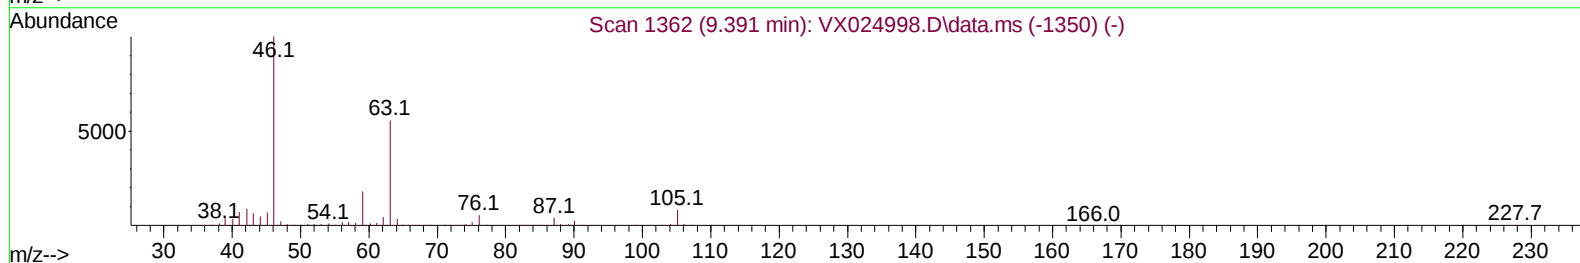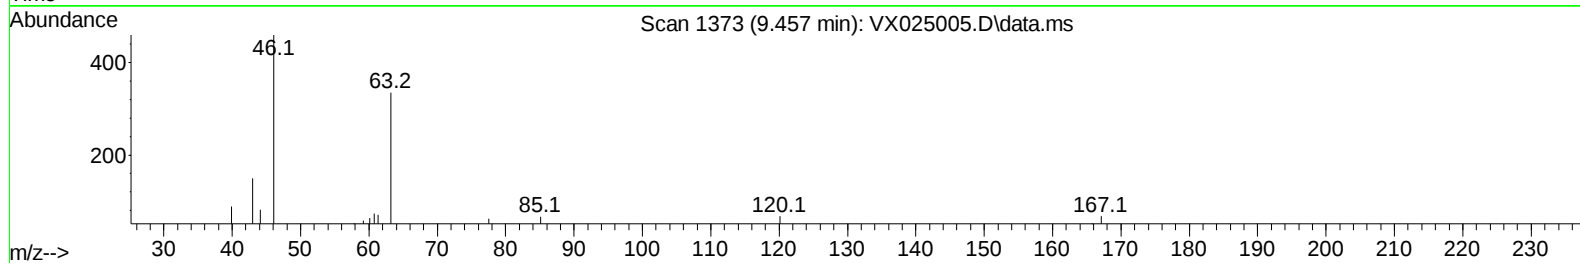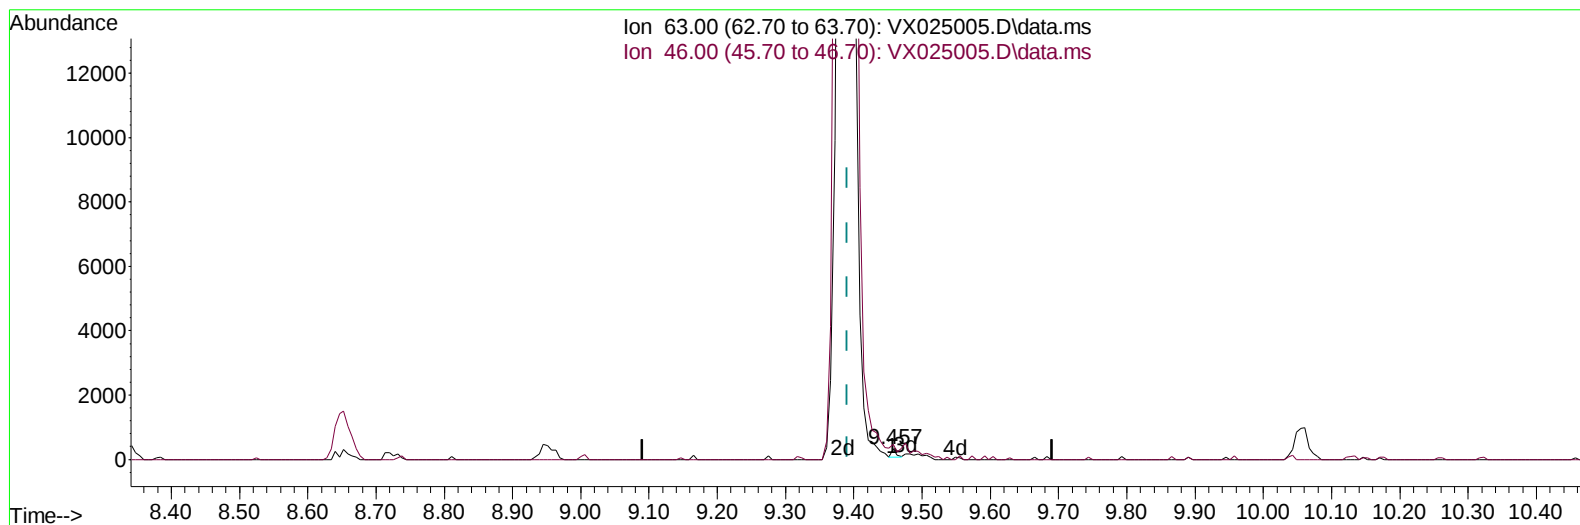

TIC: VX025005.D\data.ms

(47) 2-Hexanone-d5 (S)

9.457min (+ 0.066) 0.20 ug/L

response 131

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	140.40	126.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025005.D
 Acq On : 28 Oct 2021 14:41
 Operator : JC/MD
 Sample : VX1028MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK618

Manual Integrations
 APPROVED

MMDadoda
 11/1/2021 12:58:48 PM

Quant Time: Oct 29 06:48:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 28 12:38:37 2021
 Response via : Initial Calibration

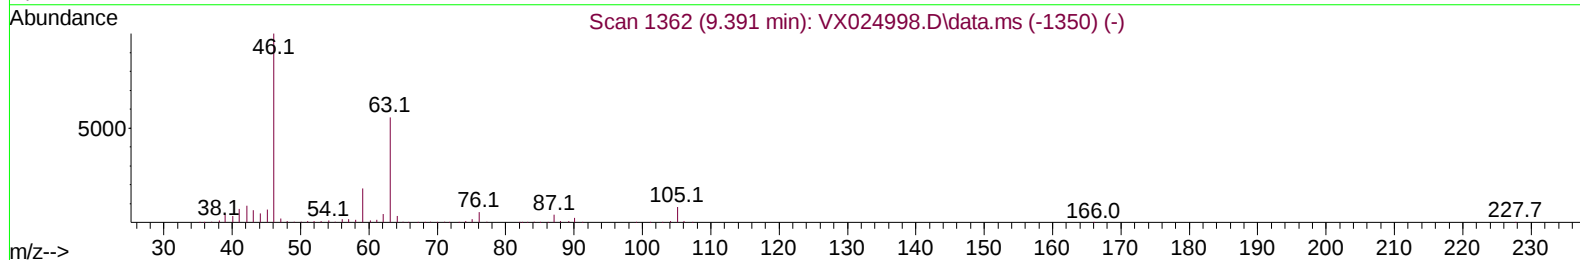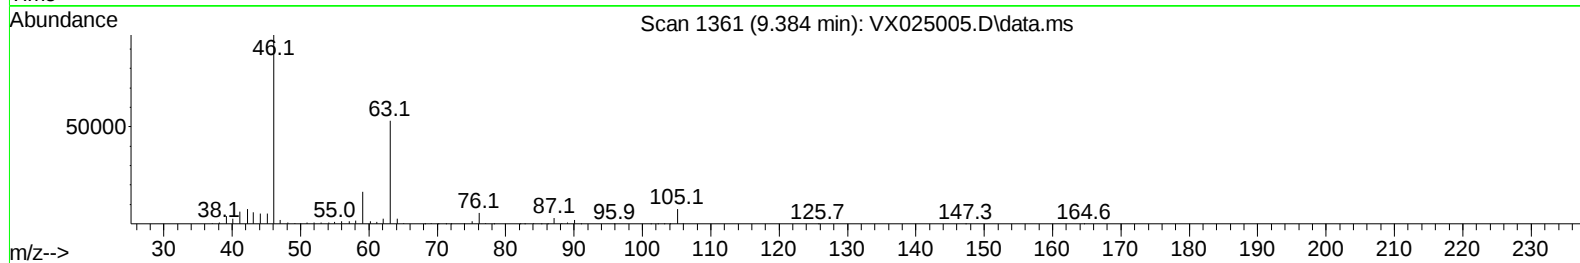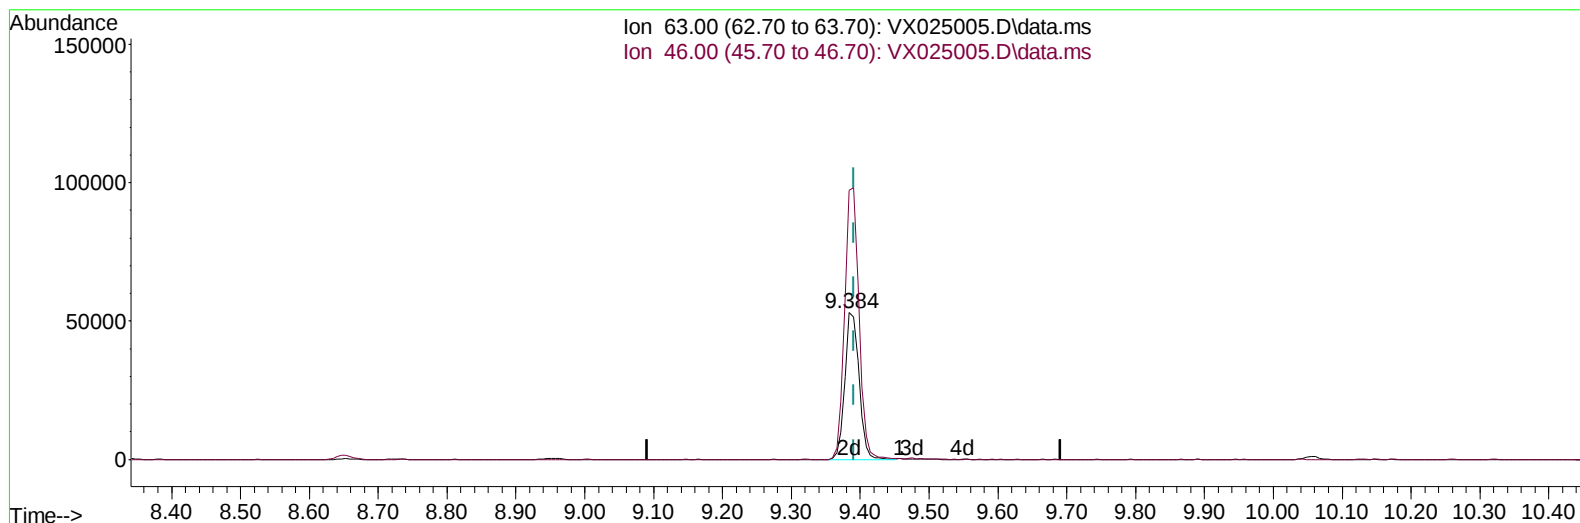

TIC: VX025005.D\data.ms

(47) 2-Hexanone-d5 (S)

9.384min (-0.007) 114.87 ug/L m

response 75566

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	140.40	0.22#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025005.D
 Acq On : 28 Oct 2021 14:41
 Operator : JC/MD
 Sample : VX1028MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 VBLK618

Manual Integrations
 APPROVED

MMDadoda
 11/1/2021 12:58:48 PM

Quant Time: Oct 29 06:48:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 28 12:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	147435	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	10.055	117	133576	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	56069	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	50246	53.464	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	106.920%	
7) Chloroethane-d5	1.672	69	36983	57.570	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	115.140%	
11) 1,1-Dichloroethene-d2	2.306	63	91874	39.672	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.340%	
21) 2-Butanone-d5	4.470	46	106220	113.153	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	113.150%	
24) Chloroform-d	5.068	84	130408	53.030	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.060%	
26) 1,2-Dichloroethane-d4	5.964	65	97953	54.318	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.640%	
32) Benzene-d6	5.976	84	204496	53.937	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.880%	
36) 1,2-Dichloropropane-d6	7.311	67	71136	55.056	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	110.120%	
41) Toluene-d8	8.653	98	189349	52.202	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	104.400%	
43) trans-1,3-Dichloroprop...	8.951	79	39708	53.477	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	106.960%	
47) 2-Hexanone-d5	9.384	63	75566m	114.869	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	114.870%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	96395	55.172	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	110.340%	
66) 1,2-Dichlorobenzene-d4	12.323	152	61912	56.905	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	113.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025005.D
Acq On : 28 Oct 2021 14:41
Operator : JC/MD
Sample : VX1028MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK618

Manual Integrations
APPROVED

MMDadoda
11/1/2021 12:58:48 PM

Quant Time: Oct 29 06:48:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 28 12:38:37 2021
Response via : Initial Calibration

