

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025004.D
 Acq On : 28 Oct 2021 14:18
 Operator : JC/MD
 Sample : VX1028WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK617

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	78655	81320	11.59%	1.537%
2	1.672	91	96	104	rBV	57158	73007	10.41%	1.379%
3	2.307	194	200	213	rBV	154441	244208	34.82%	4.614%
4	2.520	231	235	238	rBV3	1424	2173	0.31%	0.041%
5	2.630	251	253	254	rVB	990	685	0.10%	0.013%
6	2.886	293	295	297	rVB	821	705	0.10%	0.013%
7	3.227	349	351	355	rVB2	893	945	0.13%	0.018%
8	3.258	355	356	360	rBV2	898	855	0.12%	0.016%
9	3.599	407	412	414	rBV2	548	740	0.11%	0.014%
10	3.636	417	418	421	rVB	842	592	0.08%	0.011%
11	3.794	442	444	447	rBV	388	593	0.08%	0.011%
12	3.843	451	452	460	rVB2	701	959	0.14%	0.018%
13	3.971	471	473	476	rVV2	614	547	0.08%	0.010%
14	4.007	476	479	483	rVB3	471	767	0.11%	0.014%
15	4.257	518	520	523	rVB2	552	564	0.08%	0.011%
16	4.471	546	555	571	rBV	57206	172267	24.56%	3.255%
17	4.654	581	585	587	rBV	643	593	0.08%	0.011%
18	4.678	587	589	594	rVB4	625	819	0.12%	0.015%
19	4.776	603	605	608	rBV	1016	1000	0.14%	0.019%
20	4.830	610	614	616	rBV	542	616	0.09%	0.012%
21	4.891	622	624	626	rBV	538	529	0.08%	0.010%
22	4.922	626	629	631	rBV2	456	724	0.10%	0.014%
23	5.062	639	652	670	rBV	100619	311157	44.36%	5.879%
24	5.379	701	704	706	rBV	972	1158	0.17%	0.022%
25	5.458	714	717	719	rBV	443	550	0.08%	0.010%
26	5.525	725	728	729	rBV	709	727	0.10%	0.014%
27	5.544	729	731	733	rVV	963	823	0.12%	0.016%
28	5.653	742	749	751	rBV2	940	1456	0.21%	0.028%
29	5.855	777	782	783	rBV	467	599	0.09%	0.011%
30	5.977	789	802	818	rBV2	235918	701410	100.00%	13.253%
31	6.196	836	838	841	rVB	779	775	0.11%	0.015%
32	6.769	919	932	942	rBV	172094	416387	59.36%	7.868%
33	6.879	948	950	952	rVB2	725	551	0.08%	0.010%
34	7.111	981	988	991	rBV4	3153	5811	0.83%	0.110%
35	7.208	1002	1004	1006	rBV4	630	549	0.08%	0.010%
36	7.312	1012	1021	1033	rBV	148376	324668	46.29%	6.135%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025004.D
 Acq On : 28 Oct 2021 14:18
 Operator : JC/MD
 Sample : VX1028WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK617

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis

37	7.489	1046	1050	1053	rBV4	1313	1735	0.25%	0.033%
38	7.629	1071	1073	1075	rVV2	760	531	0.08%	0.010%
39	7.653	1075	1077	1079	rVB2	774	764	0.11%	0.014%
40	7.751	1092	1093	1096	rBV3	700	631	0.09%	0.012%
41	7.867	1110	1112	1116	rBV3	577	555	0.08%	0.010%
42	7.921	1119	1121	1122	rBV	1063	912	0.13%	0.017%
43	8.330	1181	1188	1198	rVV	105171	170084	24.25%	3.214%
44	8.446	1206	1207	1210	rVB	996	537	0.08%	0.010%
45	8.476	1210	1212	1214	rBV2	650	820	0.12%	0.015%
46	8.586	1227	1230	1232	rBV	605	566	0.08%	0.011%
47	8.653	1234	1241	1248	rBV	345908	534120	76.15%	10.092%
48	8.952	1284	1290	1300	rVV	78356	120277	17.15%	2.273%
49	9.202	1329	1331	1335	rVB	770	875	0.12%	0.017%
50	9.287	1341	1345	1347	rVV3	711	1024	0.15%	0.019%
51	9.391	1355	1362	1378	rBV	253546	383187	54.63%	7.240%
52	9.665	1403	1407	1412	rVB2	504	971	0.14%	0.018%
53	9.708	1412	1414	1415	rVV2	863	530	0.08%	0.010%
54	9.976	1456	1458	1460	rVB2	742	540	0.08%	0.010%
55	10.055	1465	1471	1481	rBV	360780	479927	68.42%	9.068%
56	10.250	1500	1503	1505	rBV2	648	624	0.09%	0.012%
57	10.305	1509	1512	1517	rVB2	1321	1578	0.22%	0.030%
58	10.409	1525	1529	1530	rBV	530	527	0.08%	0.010%
59	10.586	1555	1558	1560	rBV	699	743	0.11%	0.014%
60	10.640	1565	1567	1568	rBV	937	704	0.10%	0.013%
61	10.884	1604	1607	1608	rBV	595	634	0.09%	0.012%
62	11.012	1625	1628	1632	rBV2	575	678	0.10%	0.013%
63	11.055	1632	1635	1638	rBV2	647	761	0.11%	0.014%
64	11.122	1643	1646	1652	rVV3	2853	3563	0.51%	0.067%
65	11.195	1652	1658	1667	rVV	263595	333475	47.54%	6.301%
66	11.305	1674	1676	1679	rVB2	759	660	0.09%	0.012%
67	11.378	1685	1688	1689	rBV2	585	681	0.10%	0.013%
68	11.445	1697	1699	1704	rVB2	1160	950	0.14%	0.018%
69	11.665	1733	1735	1740	rVB2	593	568	0.08%	0.011%
70	11.707	1740	1742	1745	rVB	647	669	0.10%	0.013%
71	11.756	1745	1750	1755	rBV4	2836	4345	0.62%	0.082%
72	11.841	1762	1764	1766	rBV2	693	609	0.09%	0.012%
73	11.933	1775	1779	1783	rVV2	1332	2340	0.33%	0.044%
74	11.969	1783	1785	1786	rVV2	681	582	0.08%	0.011%
75	12.024	1789	1794	1802	rVV	336102	422563	60.24%	7.984%
76	12.250	1828	1831	1832	rBV	727	582	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025004.D
 Acq On : 28 Oct 2021 14:18
 Operator : JC/MD
 Sample : VX1028WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK617

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1853	rBV	353309	445352	63.49%	8.415%
78	12.427	1858	1860	1863	rVB3	670	687	0.10%	0.013%
79	13.036	1957	1960	1962	rBV	641	810	0.12%	0.015%
80	13.164	1979	1981	1984	rVB2	821	772	0.11%	0.015%
81	13.286	1999	2001	2003	rBV	474	535	0.08%	0.010%
82	13.780	2080	2082	2085	rBV2	949	915	0.13%	0.017%
83	13.878	2096	2098	2102	rBV2	453	667	0.10%	0.013%
84	14.225	2153	2155	2158	rVB	761	831	0.12%	0.016%
85	14.274	2158	2163	2165	rBV2	564	809	0.12%	0.015%
86	14.329	2169	2172	2176	rVB	551	832	0.12%	0.016%
87	14.432	2185	2189	2192	rVB	498	645	0.09%	0.012%
88	14.469	2192	2195	2196	rBV	760	699	0.10%	0.013%
89	14.609	2215	2218	2219	rBV	719	856	0.12%	0.016%
90	14.884	2259	2263	2267	rVB	831	1440	0.21%	0.027%
91	15.030	2285	2287	2289	rBV2	602	530	0.08%	0.010%
92	15.560	2372	2374	2376	rVB	954	683	0.10%	0.013%
93	15.591	2376	2379	2382	rBV3	1052	1388	0.20%	0.026%
94	15.682	2390	2394	2395	rBV2	879	934	0.13%	0.018%
95	15.755	2403	2406	2408	rBV	675	777	0.11%	0.015%
96	16.042	2451	2453	2456	rBV	942	1074	0.15%	0.020%
97	16.341	2499	2502	2504	rBV2	644	620	0.09%	0.012%
98	16.365	2504	2506	2508	rVB3	789	711	0.10%	0.013%
99	16.444	2517	2519	2522	rBV3	717	1056	0.15%	0.020%
100	16.548	2534	2536	2538	rBV3	498	530	0.08%	0.010%

Sum of corrected areas: 5292404




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025004.D
Acq On : 28 Oct 2021 14:18
Operator : JC/MD
Sample : VX1028WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
VBLK617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

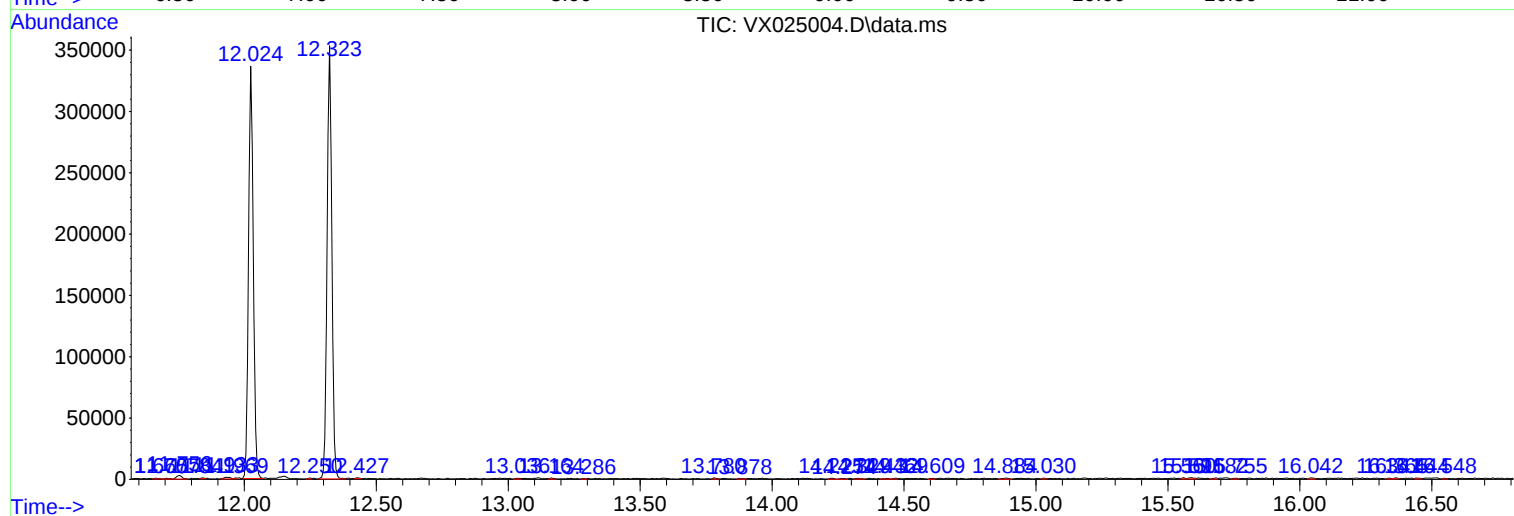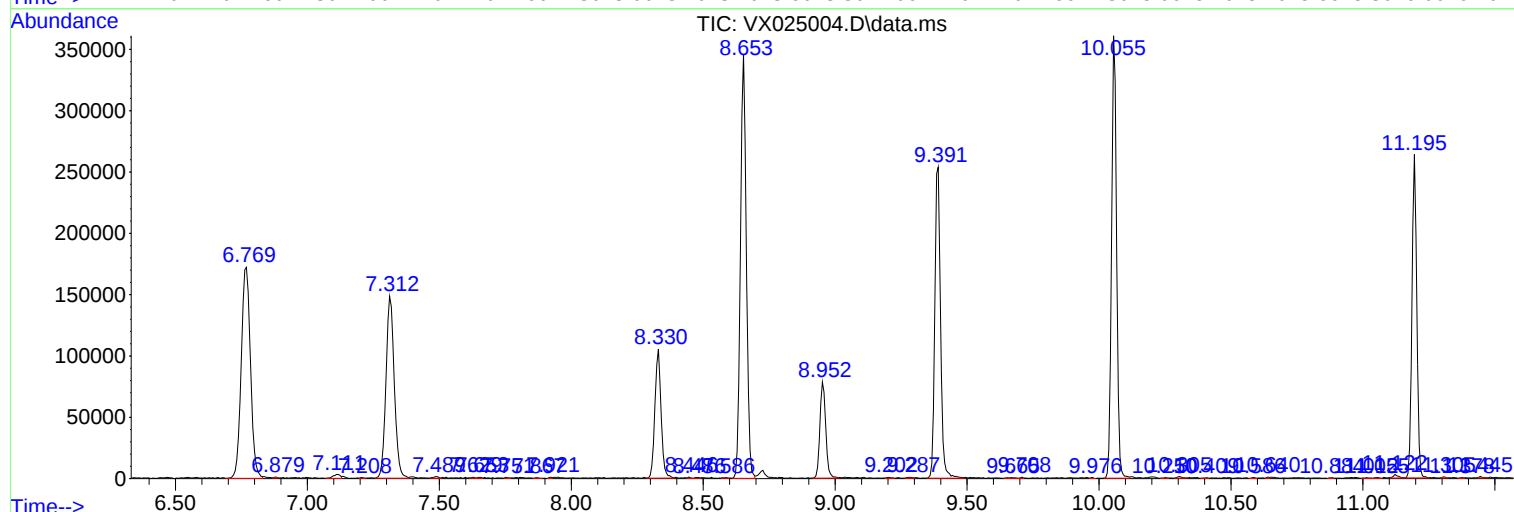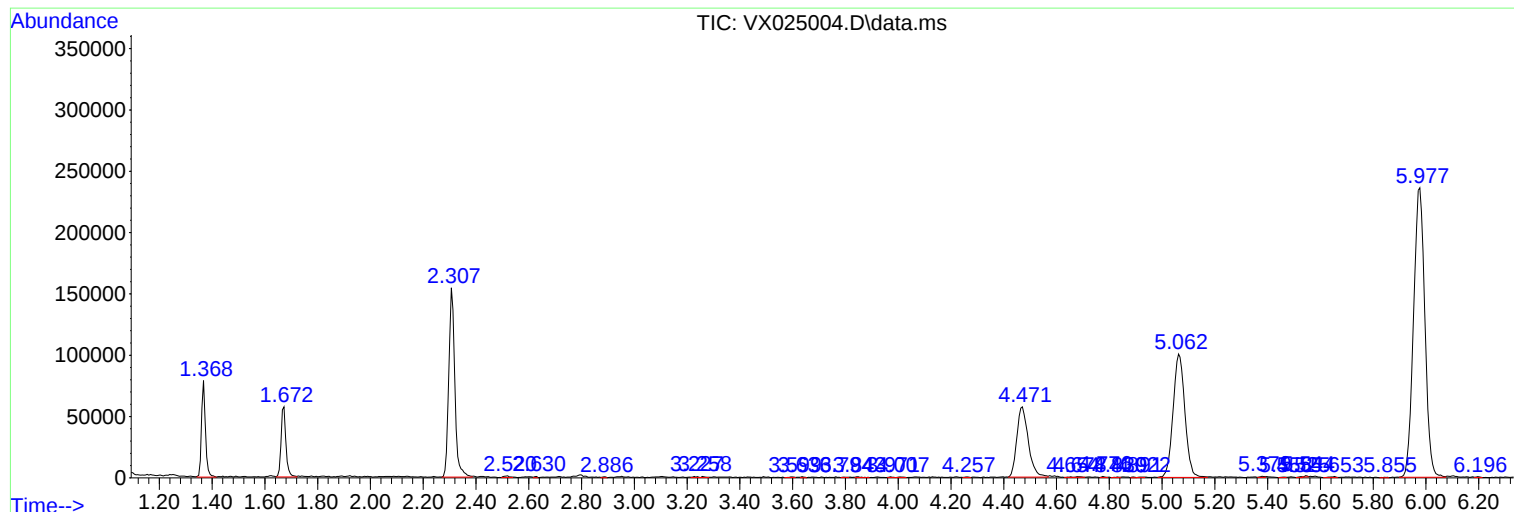

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025004.D
Acq On : 28 Oct 2021 14:18
Operator : JC/MD
Sample : VX1028WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025004.D
Acq On : 28 Oct 2021 14:18
Operator : JC/MD
Sample : VX1028WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
